




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026280.D
 Acq On : 15 Jun 2022 16:09
 Operator : SY/MD
 Sample : N3275-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD4

Manual IntegrationsAPPROVED

Quant Time: Jun 16 01:40:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 16 01:38:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/17/2022

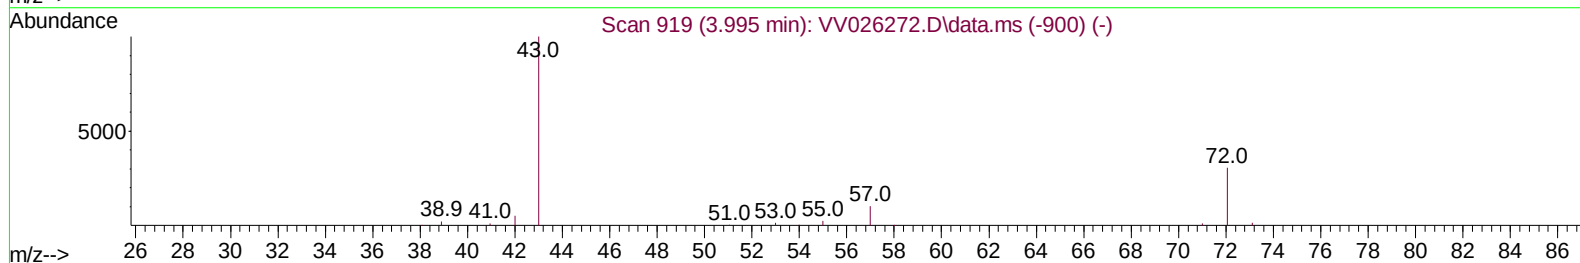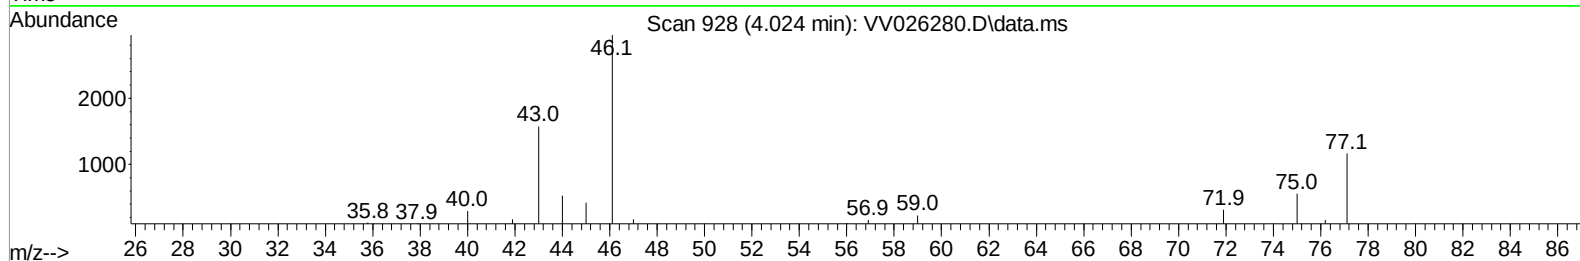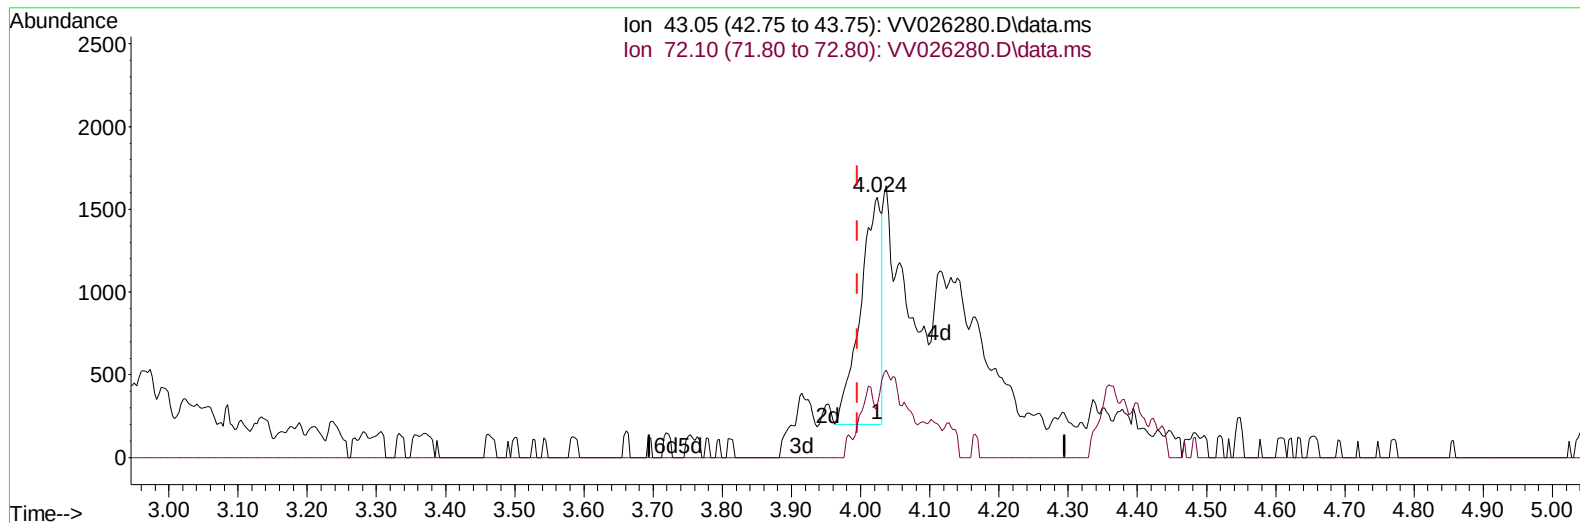

TIC: VV026280.D\data.ms

(21) 2-Butanone (T)

4.024min (+ 0.029) 1.80 ug/L

response 2923

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	15.70
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026280.D
 Acq On : 15 Jun 2022 16:09
 Operator : SY/MD
 Sample : N3275-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD4

Manual IntegrationsAPPROVED

Quant Time: Jun 16 01:40:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 16 01:38:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/17/2022

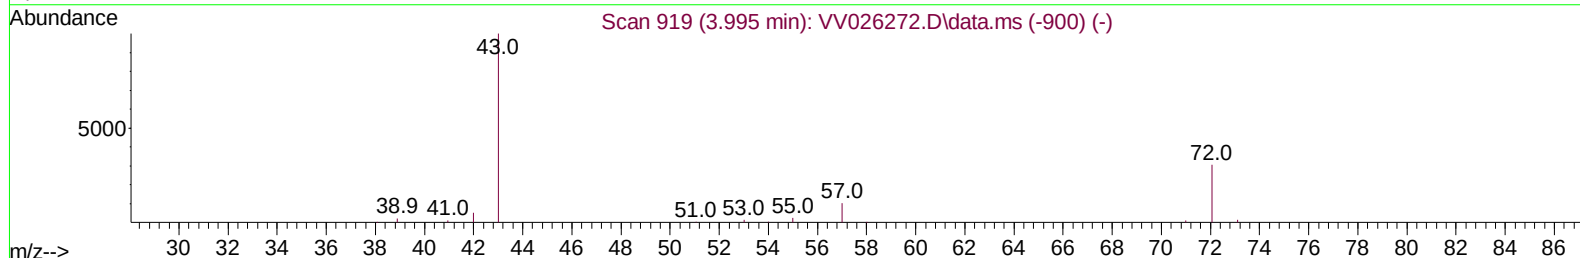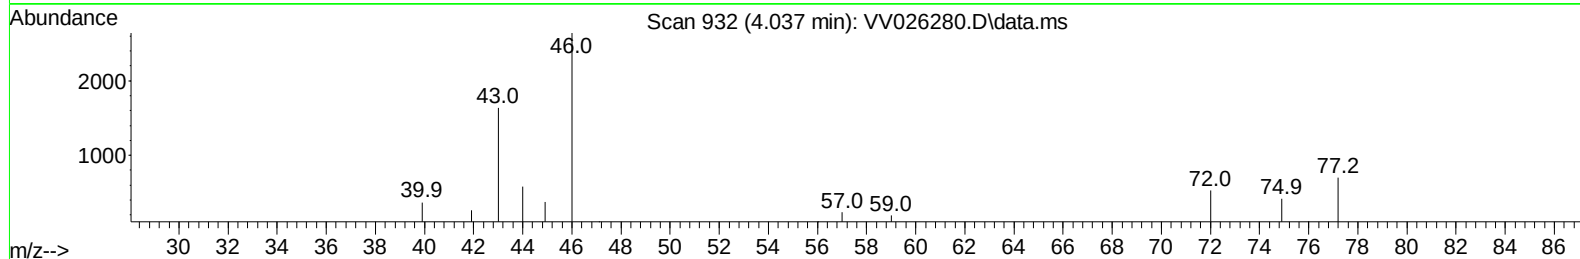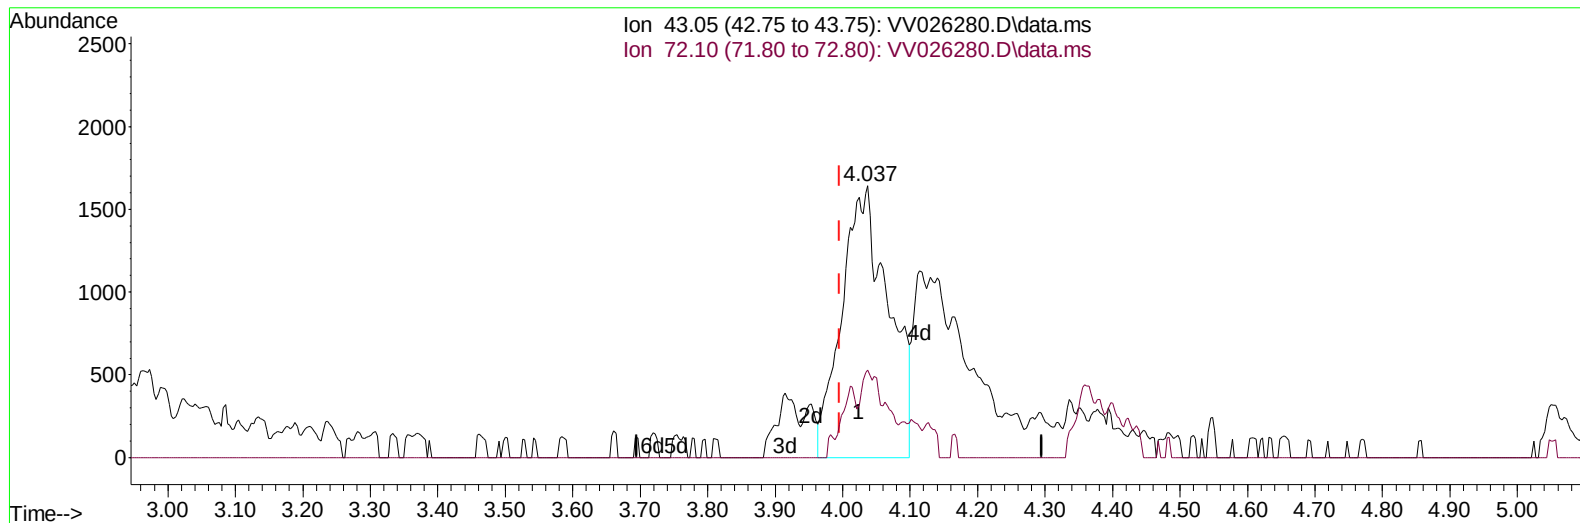

TIC: VV026280.D\data.ms

(21) 2-Butanone (T)

4.037min (+ 0.042) 4.83 ug/L m

response 7856

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	5.84#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026280.D
 Acq On : 15 Jun 2022 16:09
 Operator : SY/MD
 Sample : N3275-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD4

Manual IntegrationsAPPROVED

Quant Time: Jun 16 01:40:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 16 01:38:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/17/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	191261	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	185870	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	79290	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	77216	4.648	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	93.000%	
7) Chloroethane-d5	1.577	69	62689	4.799	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	96.000%	
11) 1,1-Dichloroethene-d2	2.118	63	105617	3.702	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	74.000%	
20) 2-Butanone-d5	3.918	46	92738	57.211	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	114.420%	
24) Chloroform-d	4.359	84	122746	5.041	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	100.800%	
26) 1,2-Dichloroethane-d4	5.040	65	50610	4.913	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	98.200%	
32) Benzene-d6	5.056	84	240194	4.834	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	96.600%	
36) 1,2-Dichloropropane-d6	6.076	67	72330	4.987	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	99.800%	
41) Toluene-d8	7.320	98	195111	4.306	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	86.200%	
43) trans-1,3-Dichloroprop...	7.629	79	18739	3.985	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	79.600%	
46) 2-Hexanone-d5	8.092	63	69896	49.201	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	98.400%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	43682	4.889	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	97.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	65120	5.332	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	106.600%	
Target Compounds						
9) Trichlorofluoromethane	1.764	101	45181	1.983	ug/L	96
13) Acetone	2.204	43	61308	48.804	ug/L	88
21) 2-Butanone	4.037	43	7856m	4.833	ug/L	
34) Trichloroethene	5.924	95	6115	0.470	ug/L	94
47) Tetrachloroethene	7.976	164	47643	4.944	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026280.D
Acq On : 15 Jun 2022 16:09
Operator : SY/MD
Sample : N3275-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD4

Manual IntegrationsAPPROVED

Quant Time: Jun 16 01:40:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 16 01:38:03 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
Supervised By :Mahesh Dadoda 06/17/2022

