




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026283.D
 Acq On : 15 Jun 2022 17:21
 Operator : SY/MD
 Sample : N3275-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD7

Manual IntegrationsAPPROVED

Quant Time: Jun 16 01:41:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 16 01:38:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/17/2022

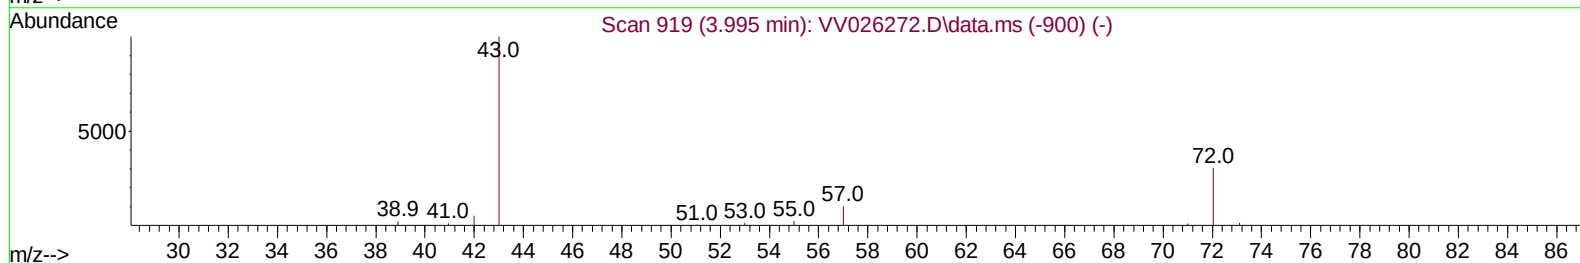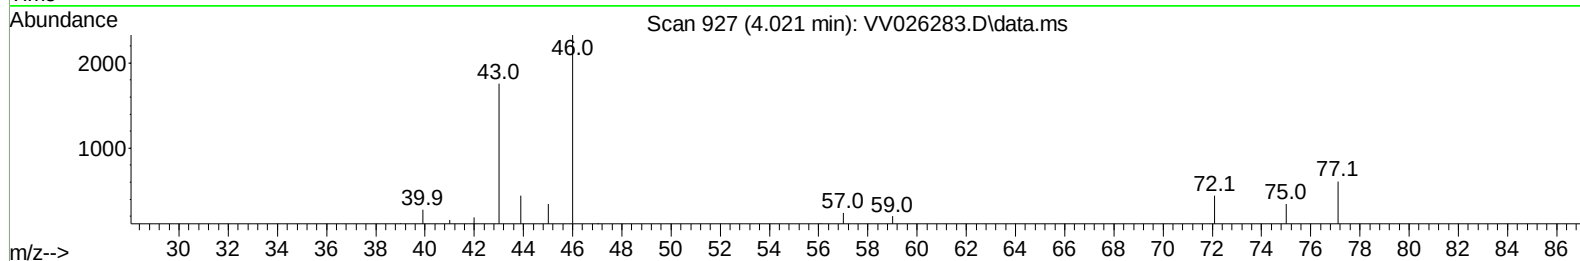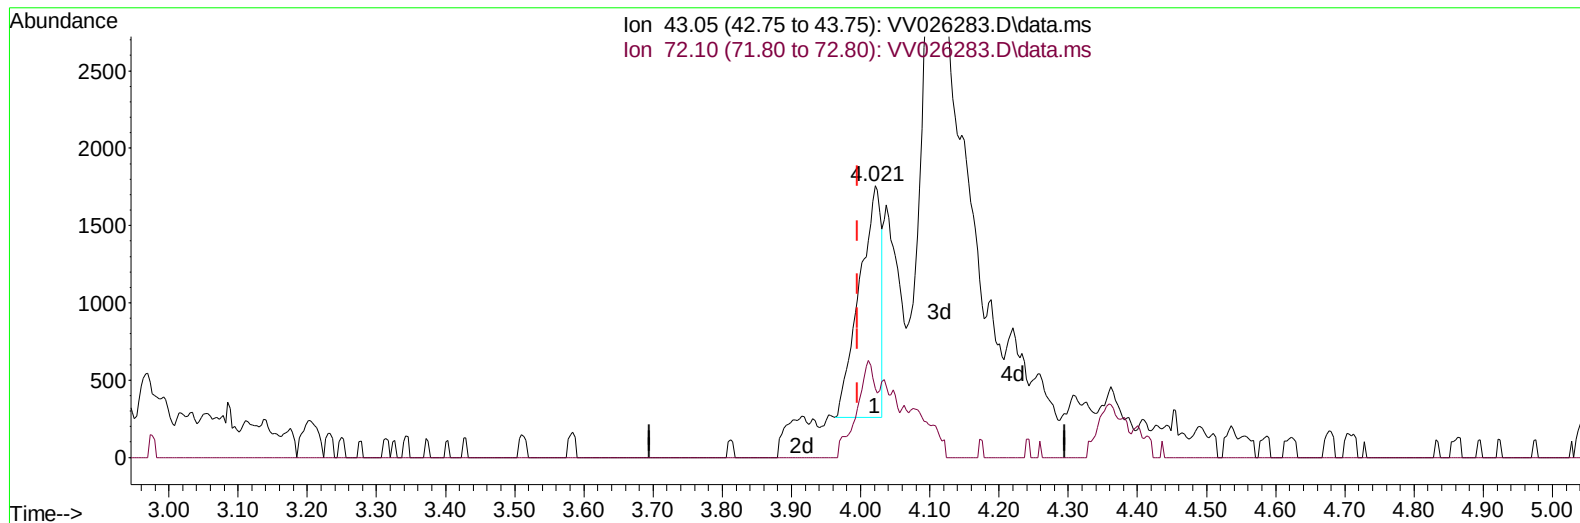

TIC: VV026283.D\data.ms

(21) 2-Butanone (T)

4.021min (+ 0.026) 2.07 ug/L

response 3273

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	36.02
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026283.D
 Acq On : 15 Jun 2022 17:21
 Operator : SY/MD
 Sample : N3275-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD7

Manual IntegrationsAPPROVED

Quant Time: Jun 16 01:41:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 16 01:38:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/17/2022

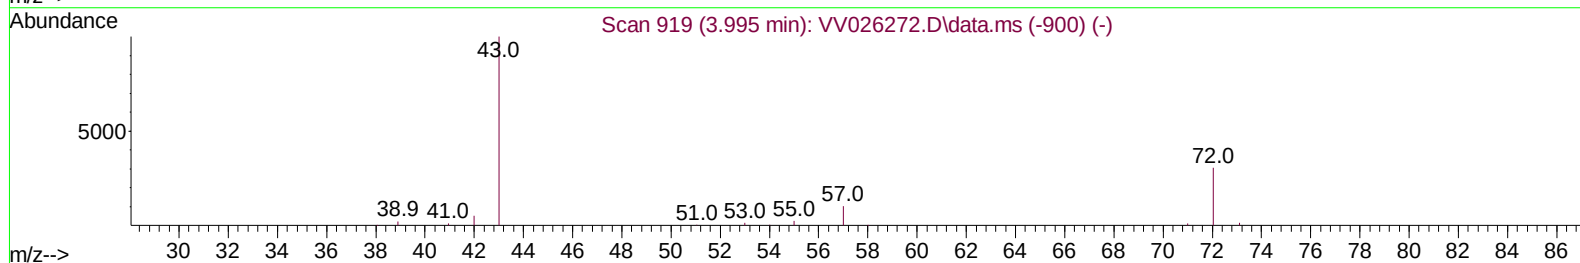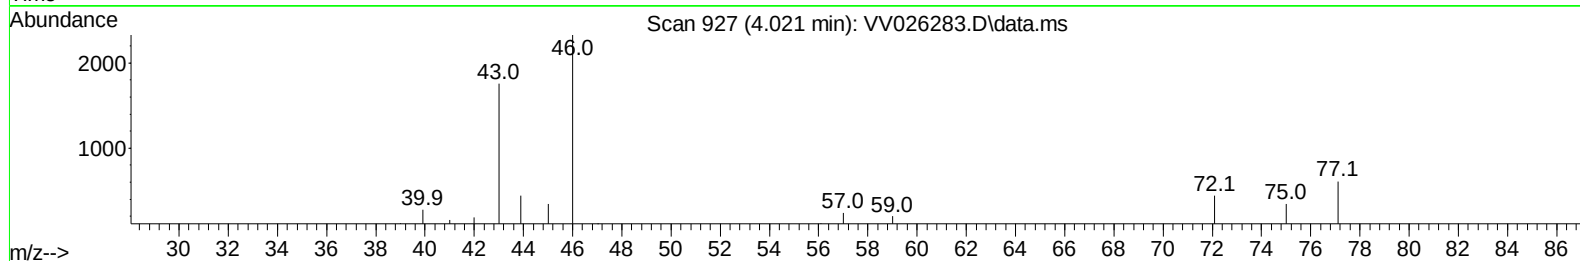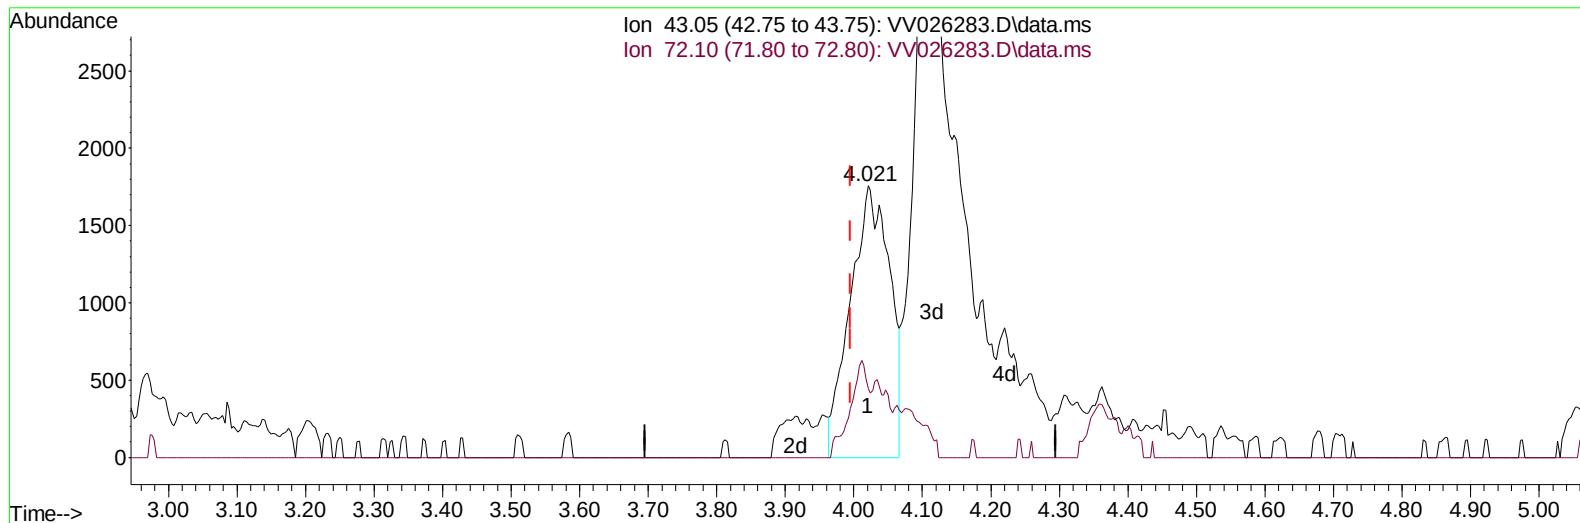

TIC: VV026283.D\data.ms

(21) 2-Butanone (T)

4.021min (+ 0.026) 4.43 ug/L m

response 6987

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	16.87
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026283.D
 Acq On : 15 Jun 2022 17:21
 Operator : SY/MD
 Sample : N3275-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD7

Manual IntegrationsAPPROVED

Quant Time: Jun 16 01:41:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 16 01:38:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/17/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	185657	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	176982	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	73204	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	75491	4.681	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	93.600%	
7) Chloroethane-d5	1.574	69	60569	4.777	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	95.600%	
11) 1,1-Dichloroethene-d2	2.114	63	101583	3.668	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	73.400%	
20) 2-Butanone-d5	3.905	46	83723	53.209	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	106.420%	
24) Chloroform-d	4.355	84	121460	5.139	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	102.800%	
26) 1,2-Dichloroethane-d4	5.040	65	49681	4.968	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	99.400%	
32) Benzene-d6	5.056	84	232243	4.908	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	98.200%	
36) 1,2-Dichloropropane-d6	6.076	67	70126	5.078	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	101.600%	
41) Toluene-d8	7.317	98	185529	4.300	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	86.000%	
43) trans-1,3-Dichloroprop...	7.629	79	18874	4.215	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	84.200%	
46) 2-Hexanone-d5	8.092	63	65445	48.382	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	96.760%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	42769	5.028	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	100.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	60352	5.352	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	107.000%	
Target Compounds						
9) Trichlorofluoromethane	1.761	101	50423	2.279	ug/L	99
13) Acetone	2.195	43	58626	48.078	ug/L	92
21) 2-Butanone	4.021	43	6987m	4.428	ug/L	
34) Trichloroethene	5.918	95	23690	1.912	ug/L	98
47) Tetrachloroethene	7.976	164	58454	6.371	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026283.D
Acq On : 15 Jun 2022 17:21
Operator : SY/MD
Sample : N3275-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD7

Manual IntegrationsAPPROVED

Quant Time: Jun 16 01:41:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 16 01:38:03 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
Supervised By :Mahesh Dadoda 06/17/2022

