

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026273.D
 Acq On : 15 Jun 2022 13:22
 Operator : SY/MD
 Sample : VV0615WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK373

Quant Time: Jun 16 01:38:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 16 01:38:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	198554	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	189271	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	79290	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	85435	4.954	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.000%
7) Chloroethane-d5	1.577	69	67001	4.941	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.800%
11) 1,1-Dichloroethene-d2	2.114	63	116149	3.922	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.400%
20) 2-Butanone-d5	3.912	46	85968	51.087	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.180%
24) Chloroform-d	4.355	84	124030	4.907	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
26) 1,2-Dichloroethane-d4	5.040	65	55194	5.161	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.200%
32) Benzene-d6	5.056	84	260592	5.150	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.000%
36) 1,2-Dichloropropane-d6	6.072	67	77990	5.281	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.600%
41) Toluene-d8	7.317	98	218389	4.733	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.600%
43) trans-1,3-Dichloroprop...	7.628	79	22189	4.633	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.600%
46) 2-Hexanone-d5	8.091	63	71140	49.177	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.360%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	44873	4.932	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	67773	5.549	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.000%
Target Compounds						Qvalue
16) Methylene chloride	2.516	84	4321	0.270	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026273.D
Acq On : 15 Jun 2022 13:22
Operator : SY/MD
Sample : VV0615WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK373

Quant Time: Jun 16 01:38:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 16 01:38:03 2022
Response via : Initial Calibration

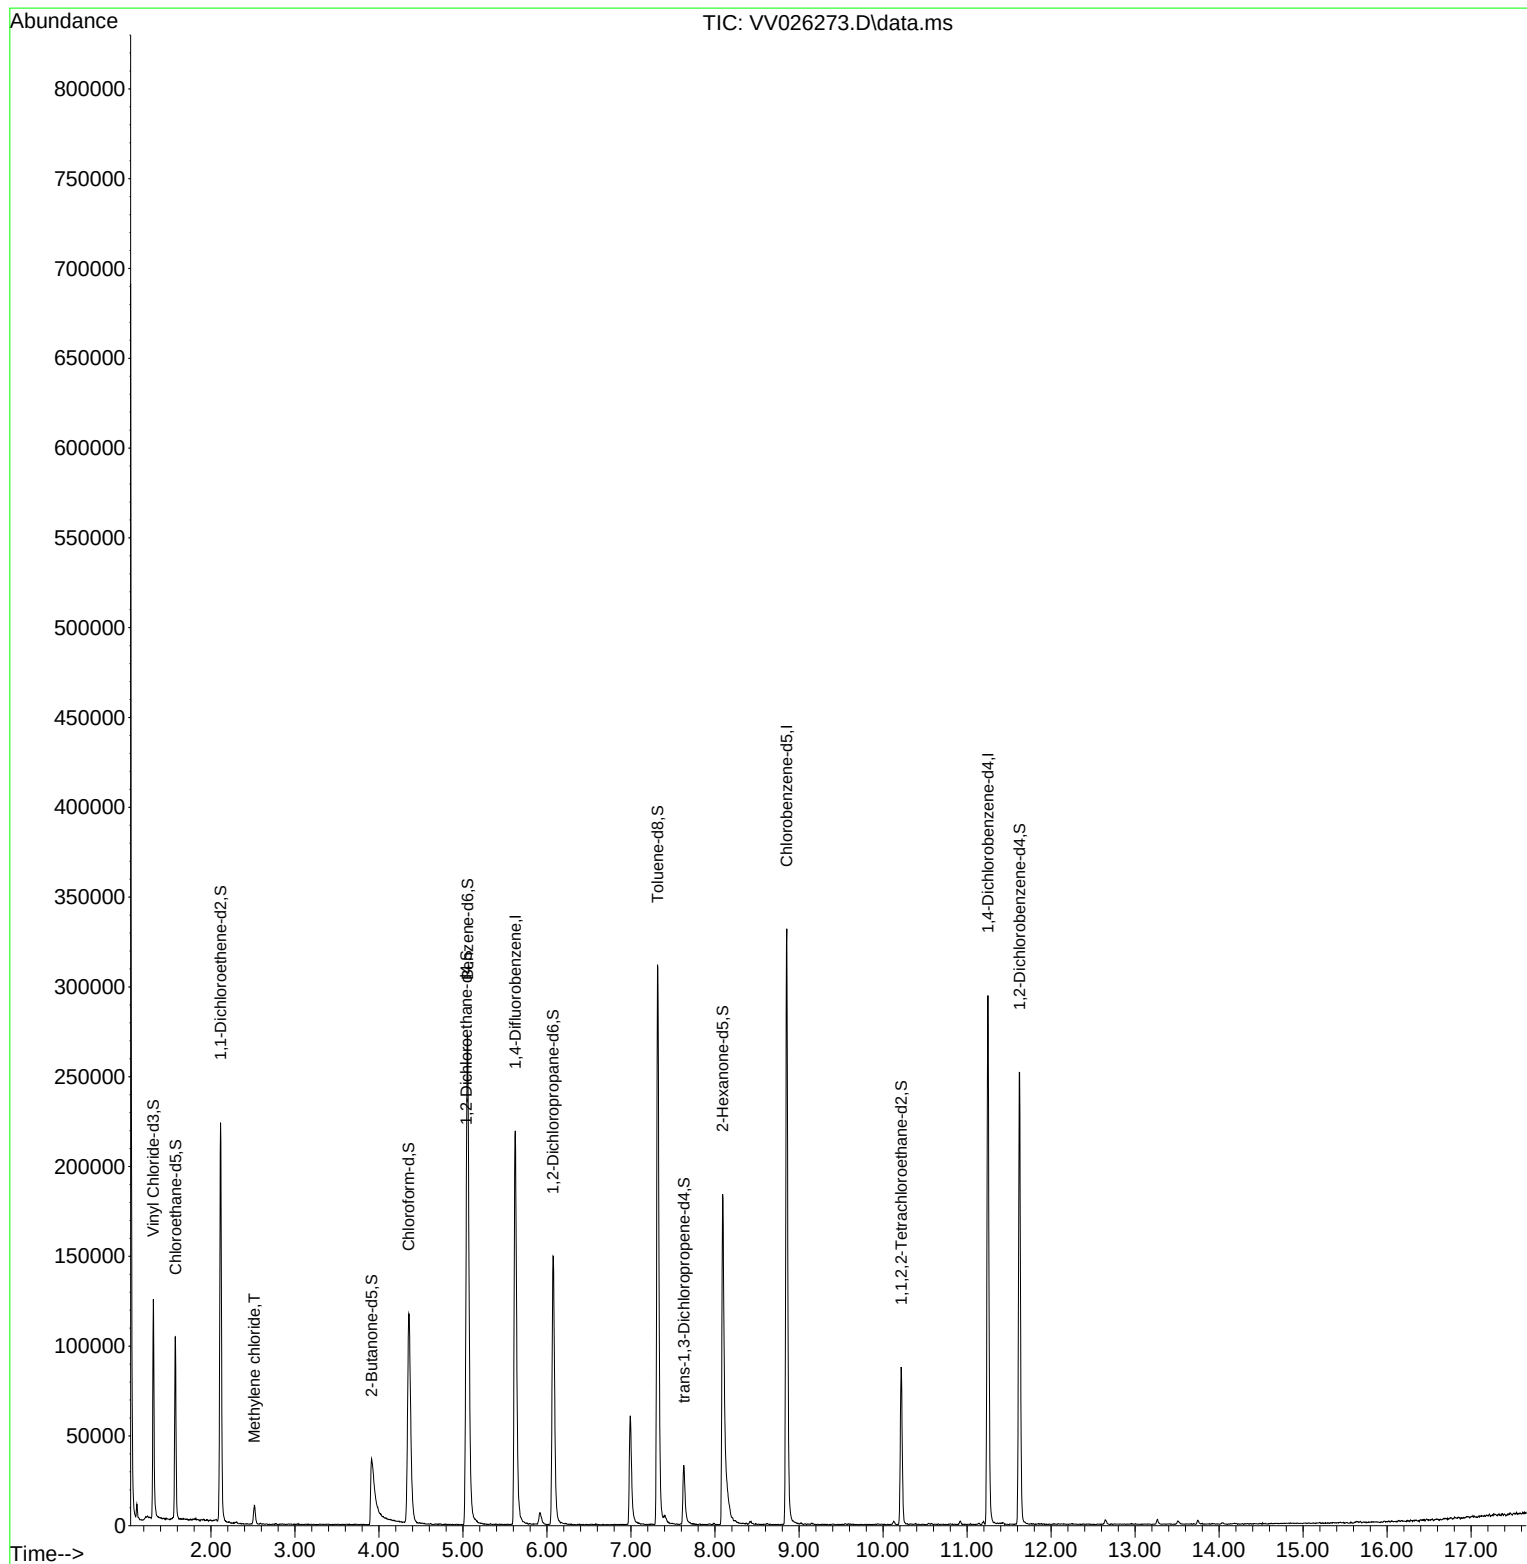

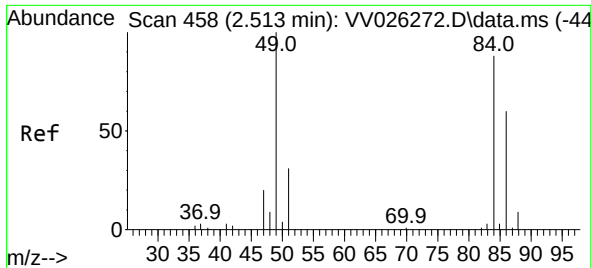

#16
Methylene chloride
Concen: 0.270 ug/L
RT: 2.516 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV026273.D
Acq: 15 Jun 2022 13:22

Instrument :
MSVOA_V
ClientSampleId :
VBLK373

Tgt Ion: 84 Resp: 4321

Ion	Ratio	Lower	Upper
84	100		
86	73.3	44.0	81.8
49	107.3	77.3	143.7

