

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026273.D
 Acq On : 15 Jun 2022 13:22
 Operator : SY/MD
 Sample : VV0615WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK373

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026273.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.314	78	85	110	rVB	121715	132285	19.79%	2.571%
2	1.577	159	167	179	rVB	101412	117358	17.55%	2.281%
3	2.114	322	334	351	rBV	221921	316924	47.41%	6.161%
4	2.516	450	459	473	rBV	10486	16778	2.51%	0.326%
5	3.912	884	893	926	rBV2	36656	134726	20.15%	2.619%
6	4.355	1015	1031	1061	rVB2	116448	299098	44.74%	5.814%
7	5.053	1233	1248	1276	rBV2	273021	668537	100.00%	12.996%
8	5.622	1413	1425	1455	rBV	219252	450189	67.34%	8.751%
9	5.915	1506	1516	1535	rBV5	6470	14139	2.11%	0.275%
10	6.072	1550	1565	1587	rBV	149542	309100	46.24%	6.009%
11	6.992	1840	1851	1874	rBV	60563	116399	17.41%	2.263%
12	7.317	1940	1952	1973	rBV	311722	556968	83.31%	10.827%
13	7.628	2040	2049	2070	rBV	32781	61410	9.19%	1.194%
14	8.091	2184	2193	2233	rBV2	183909	410402	61.39%	7.978%
15	8.853	2419	2430	2452	rBV	331559	538362	80.53%	10.465%
16	10.217	2843	2854	2870	rBV	87670	139987	20.94%	2.721%
17	11.249	3164	3175	3196	rBV	294405	460474	68.88%	8.951%
18	11.622	3280	3291	3309	rBV	251538	401153	60.00%	7.798%




Sum of corrected areas: 5144289

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026273.D
Acq On : 15 Jun 2022 13:22
Operator : SY/MD
Sample : VV0615WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK373

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

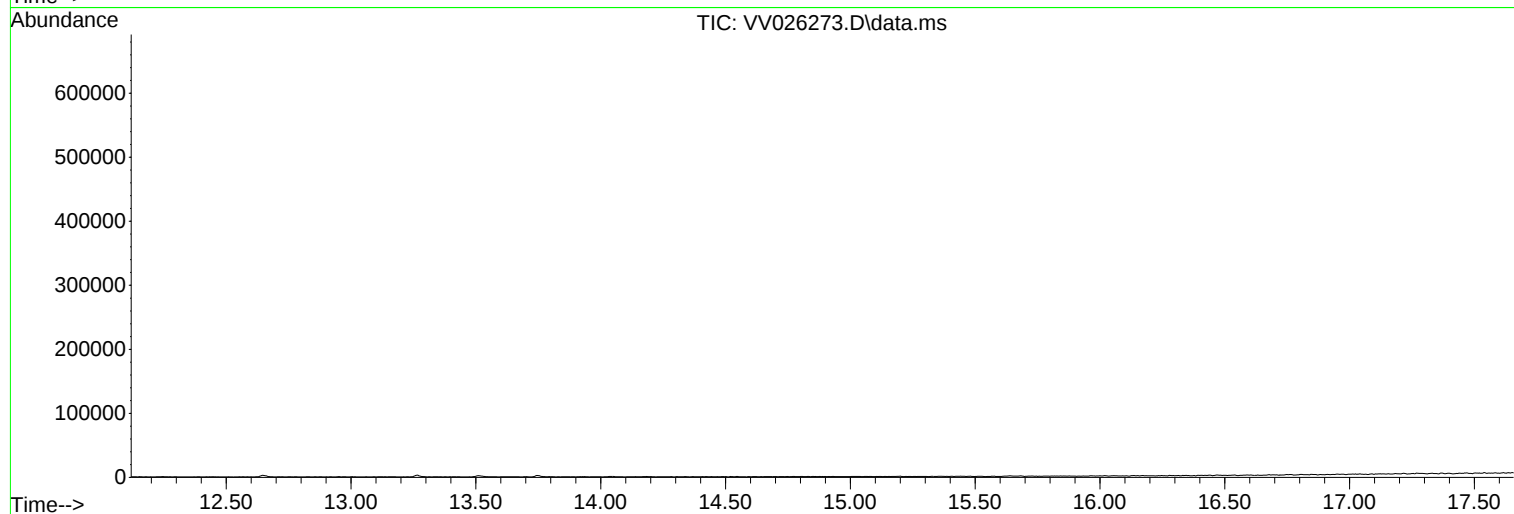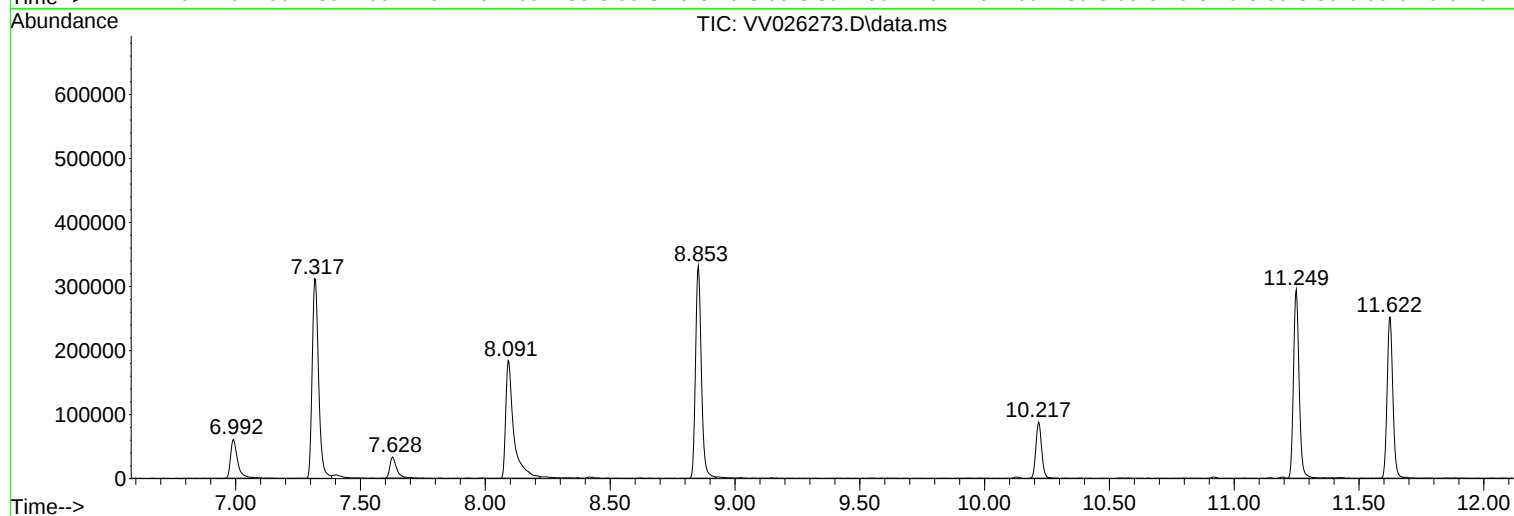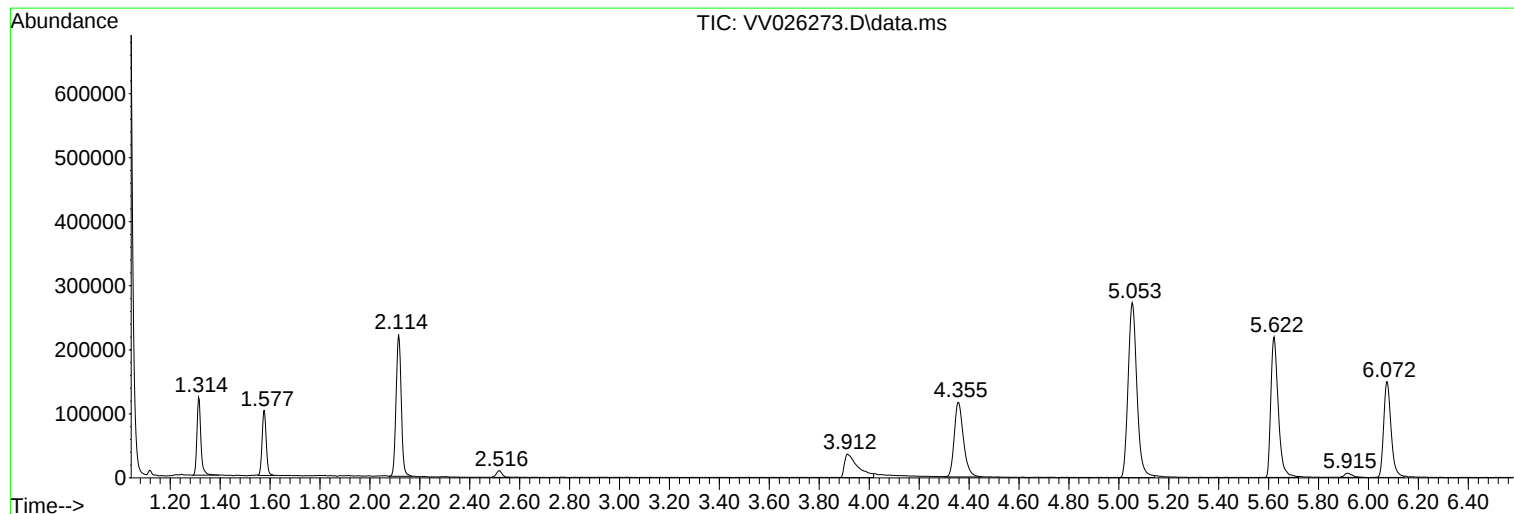

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026273.D
Acq On : 15 Jun 2022 13:22
Operator : SY/MD
Sample : VV0615WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK373

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026273.D
Acq On : 15 Jun 2022 13:22
Operator : SY/MD
Sample : VV0615WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK373

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc