

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026275.D
 Acq On : 15 Jun 2022 14:09
 Operator : SY/MD
 Sample : N3273-09DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B79DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026275.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	20	25	35	rVB3	8153	8870	1.06%	0.133%
2	1.317	78	86	105	rBV	128163	140805	16.78%	2.112%
3	1.577	158	167	182	rVB	125354	141368	16.85%	2.120%
4	1.761	215	224	234	rBV	38918	51648	6.16%	0.775%
5	2.117	324	335	351	rBV	230813	334117	39.83%	5.011%
6	2.516	449	459	476	rVB	26811	44931	5.36%	0.674%
7	3.915	876	894	922	rBV3	65012	244543	29.15%	3.668%
8	4.359	1015	1032	1055	rBV	140645	356447	42.49%	5.346%
9	5.053	1232	1248	1284	rBV2	317671	792506	94.47%	11.886%
10	5.622	1413	1425	1450	rBV	194136	400562	47.75%	6.008%
11	5.918	1506	1517	1538	rVB7	11742	27913	3.33%	0.419%
12	6.076	1551	1566	1589	rBV	183478	376391	44.87%	5.645%
13	6.992	1839	1851	1883	rBV2	64114	125446	14.95%	1.882%
14	7.320	1938	1953	1973	rBV	352067	618775	73.76%	9.281%
15	7.625	2039	2048	2071	rBV2	37461	71816	8.56%	1.077%
16	7.976	2145	2157	2181	rBV	503755	838883	100.00%	12.582%
17	8.092	2181	2193	2228	rBV2	258919	550279	65.60%	8.253%
18	8.854	2419	2430	2455	rBV	292086	486442	57.99%	7.296%
19	10.217	2843	2854	2872	rBV	111082	176663	21.06%	2.650%
20	11.249	3164	3175	3198	rBV	259448	405311	48.32%	6.079%
21	11.625	3280	3292	3312	rBV	299896	473609	56.46%	7.103%




Sum of corrected areas: 6667325

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026275.D
Acq On : 15 Jun 2022 14:09
Operator : SY/MD
Sample : N3273-09DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B79DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

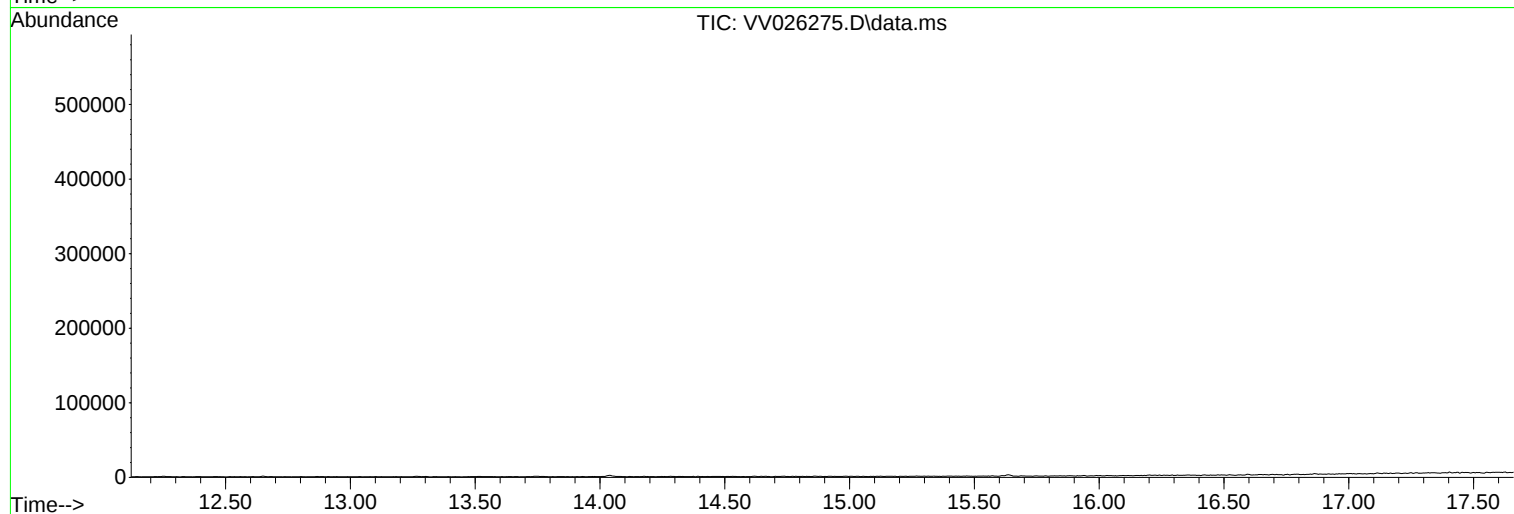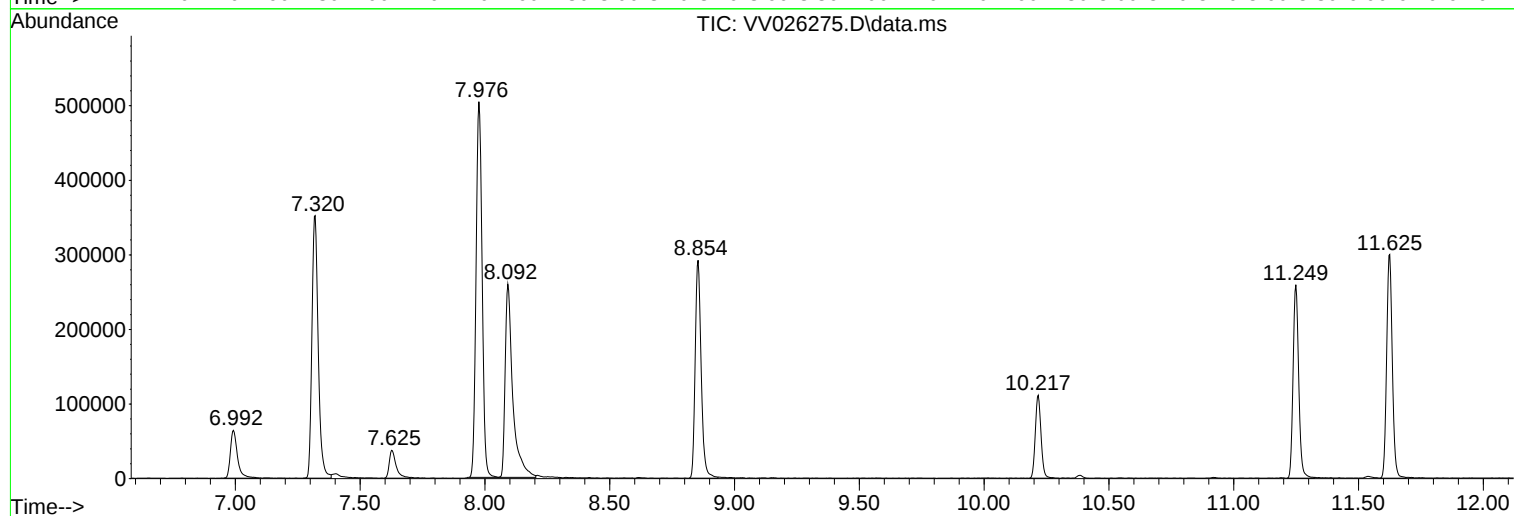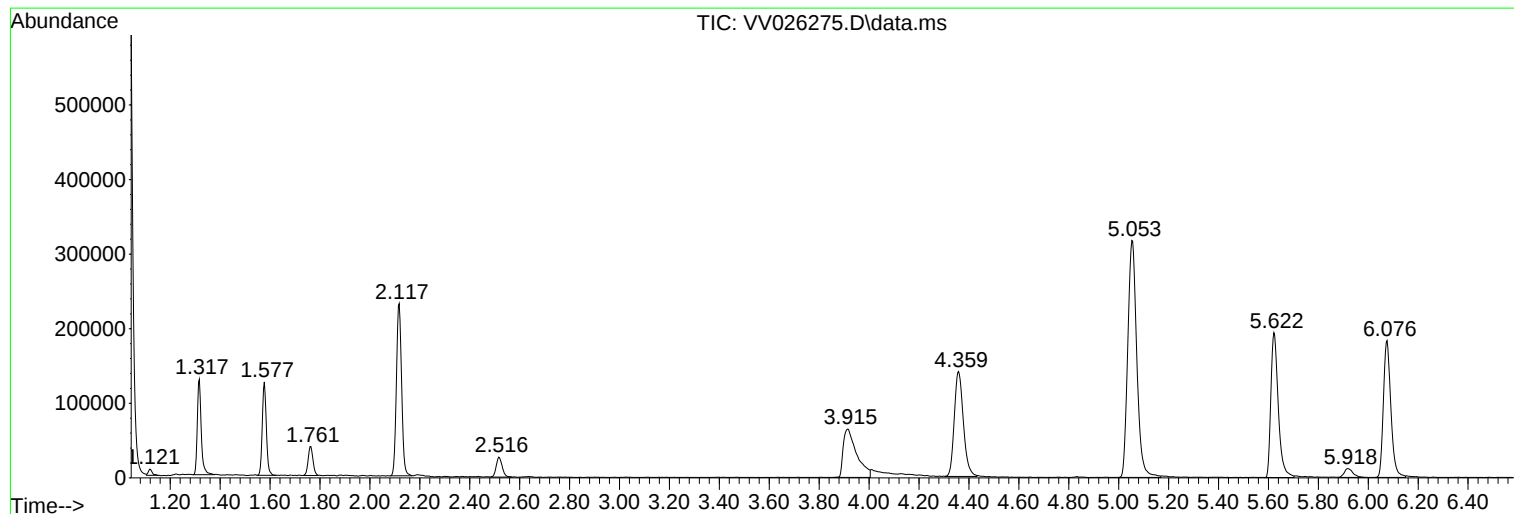

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026275.D
Acq On : 15 Jun 2022 14:09
Operator : SY/MD
Sample : N3273-09DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B79DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026275.D
Acq On : 15 Jun 2022 14:09
Operator : SY/MD
Sample : N3273-09DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B79DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc