

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026284.D
 Acq On : 15 Jun 2022 17:45
 Operator : SY/MD
 Sample : N3275-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026284.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	20	25	35	rVB4	9910	10818	1.69%	0.204%
2	1.220	50	56	62	rBV	7796	8451	1.32%	0.159%
3	1.317	79	86	100	rBV	118262	124523	19.50%	2.350%
4	1.577	160	167	183	rVB	100158	114850	17.99%	2.167%
5	1.761	218	224	232	rBV	5595	7490	1.17%	0.141%
6	2.117	325	335	348	rVB	206381	293804	46.02%	5.544%
7	2.211	354	364	382	rVB2	5911	16710	2.62%	0.315%
8	3.921	885	896	926	rBV2	41185	167182	26.18%	3.154%
9	4.359	1014	1032	1060	rBV2	120665	302174	47.33%	5.702%
10	5.056	1233	1249	1275	rBV2	259398	638492	100.00%	12.047%
11	5.622	1414	1425	1452	rBV	233040	473201	74.11%	8.929%
12	5.924	1507	1519	1537	rVB	9872	23652	3.70%	0.446%
13	6.075	1553	1566	1595	rBV	150834	309756	48.51%	5.845%
14	6.992	1841	1851	1870	rBV	54901	103580	16.22%	1.954%
15	7.320	1942	1953	1973	rBV	289379	513635	80.45%	9.691%
16	7.628	2039	2049	2069	rBV	31021	57177	8.96%	1.079%
17	7.940	2135	2146	2152	rBV3	8700	14756	2.31%	0.278%
18	7.982	2152	2159	2173	rVB3	11407	19816	3.10%	0.374%
19	8.091	2180	2193	2232	rBV	197414	419005	65.62%	7.906%
20	8.854	2419	2430	2456	rBV	350650	575955	90.21%	10.867%
21	10.217	2842	2854	2875	rBV	91599	145765	22.83%	2.750%
22	10.384	2896	2906	2917	rVB2	19562	31155	4.88%	0.588%
23	11.249	3164	3175	3196	rBV	314994	479503	75.10%	9.047%
24	11.529	3250	3262	3279	rBV2	17964	33655	5.27%	0.635%
25	11.622	3279	3291	3309	rVV	253071	402482	63.04%	7.594%
26	12.249	3477	3486	3497	rVB2	7297	12294	1.93%	0.232%




Sum of corrected areas: 5299881

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026284.D
Acq On : 15 Jun 2022 17:45
Operator : SY/MD
Sample : N3275-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

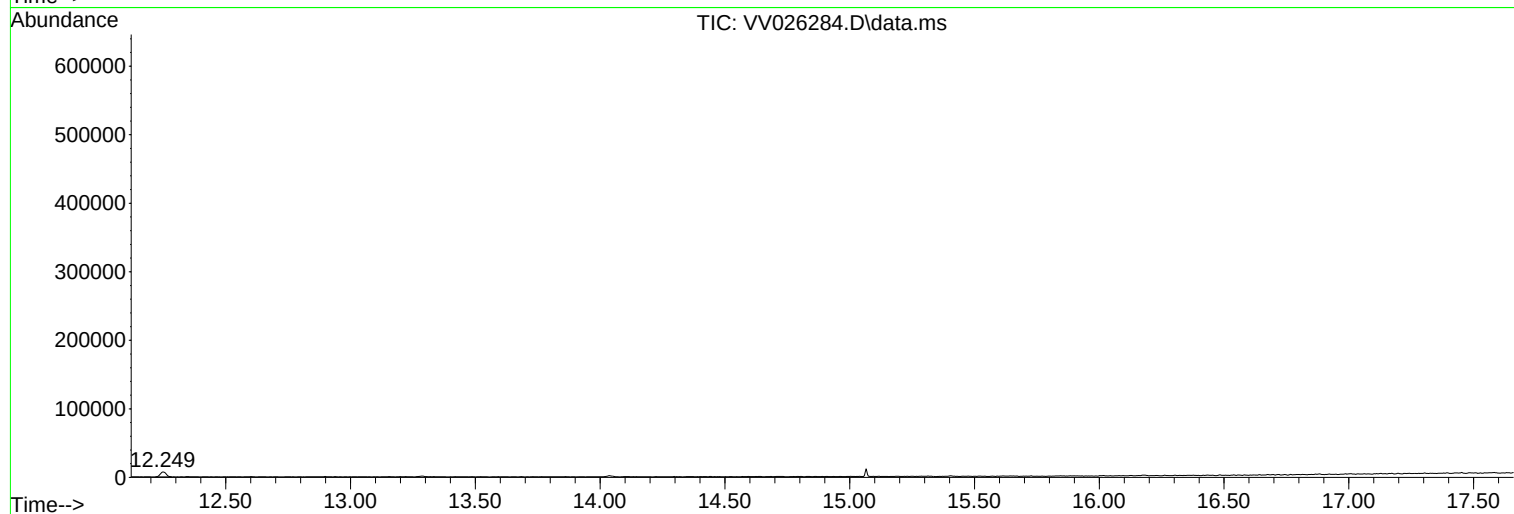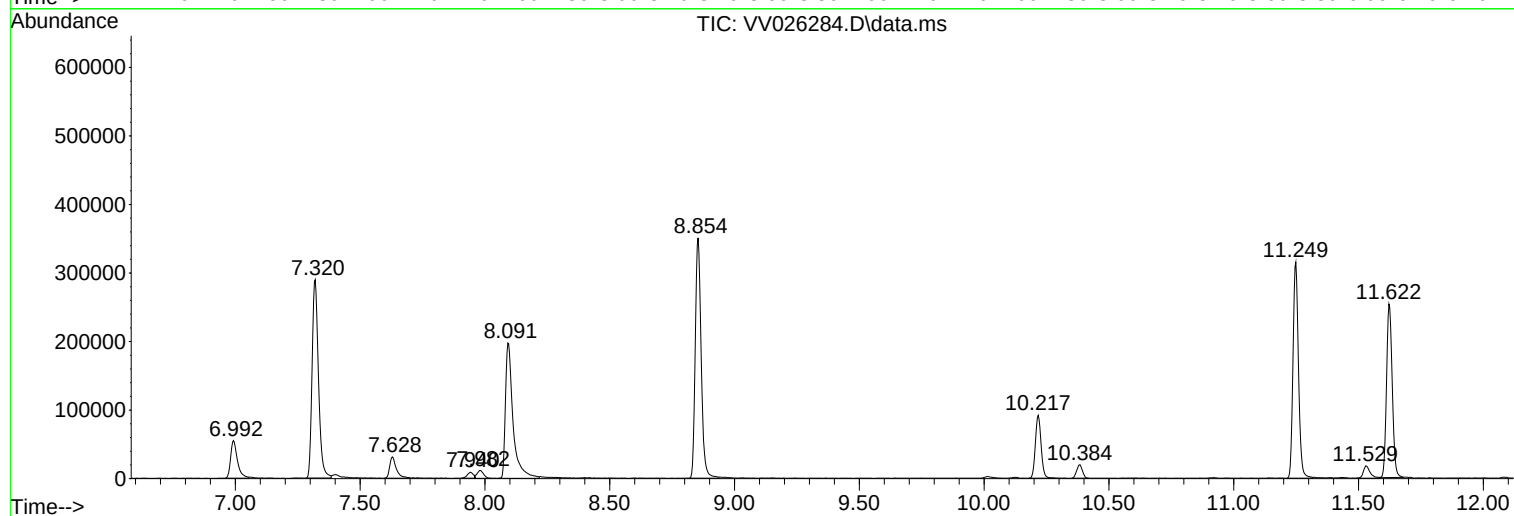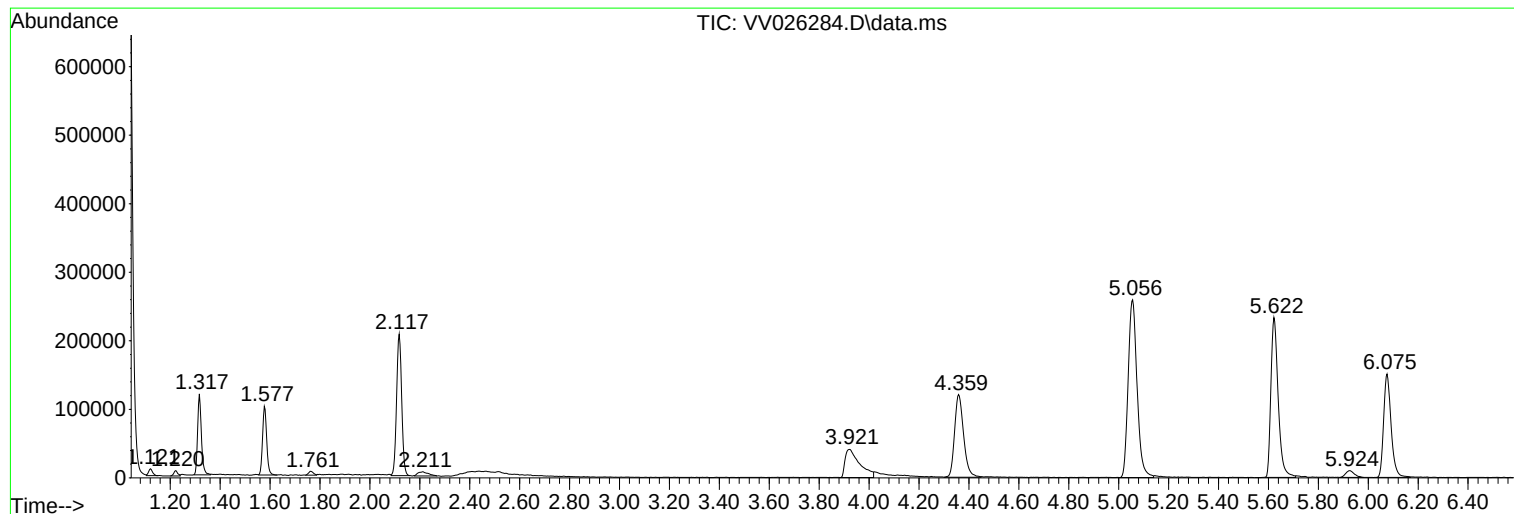

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026284.D
Acq On : 15 Jun 2022 17:45
Operator : SY/MD
Sample : N3275-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026284.D
Acq On : 15 Jun 2022 17:45
Operator : SY/MD
Sample : N3275-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc