

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026293.D
 Acq On : 15 Jun 2022 21:20
 Operator : SY/MD
 Sample : N3275-12DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026293.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	20	25	41	rVB3	8785	10976	1.62%	0.191%
2	1.317	79	86	103	rBV	110939	126978	18.74%	2.215%
3	1.581	160	168	184	rVB	90847	112849	16.65%	1.969%
4	2.114	323	334	350	rVB	215646	311030	45.90%	5.426%
5	2.516	451	459	468	rBV	10715	15736	2.32%	0.275%
6	2.629	487	494	517	rVB3	5566	12548	1.85%	0.219%
7	3.924	883	897	954	rBV2	47409	229713	33.90%	4.008%
8	4.355	1013	1031	1057	rBV	123596	310089	45.76%	5.410%
9	5.053	1233	1248	1284	rBV2	276676	677680	100.00%	11.823%
10	5.622	1413	1425	1456	rBV	230581	472296	69.69%	8.240%
11	5.918	1504	1517	1537	rBV	194620	393967	58.13%	6.873%
12	6.076	1553	1566	1591	rBV	156550	319594	47.16%	5.576%
13	6.992	1840	1851	1870	rBV2	57401	108840	16.06%	1.899%
14	7.317	1941	1952	1974	rBV	313728	554583	81.84%	9.675%
15	7.629	2040	2049	2078	rBV	30060	55971	8.26%	0.976%
16	7.982	2150	2159	2169	rVB4	9463	16157	2.38%	0.282%
17	8.095	2183	2194	2235	rBV	199085	426860	62.99%	7.447%
18	8.854	2416	2430	2456	rBV	342497	565494	83.45%	9.866%
19	10.217	2842	2854	2870	rBV	93704	149940	22.13%	2.616%
20	11.249	3162	3175	3196	rBV	305559	463664	68.42%	8.089%
21	11.625	3279	3292	3313	rBV	247601	397055	58.59%	6.927%




Sum of corrected areas: 5732020

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026293.D
Acq On : 15 Jun 2022 21:20
Operator : SY/MD
Sample : N3275-12DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

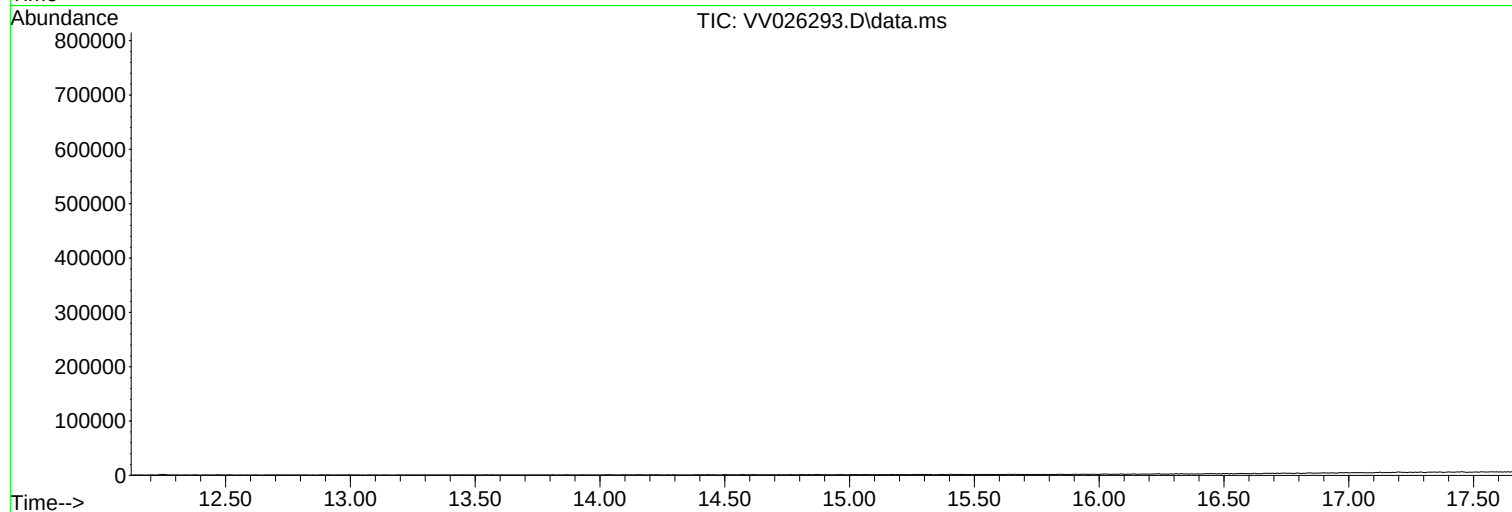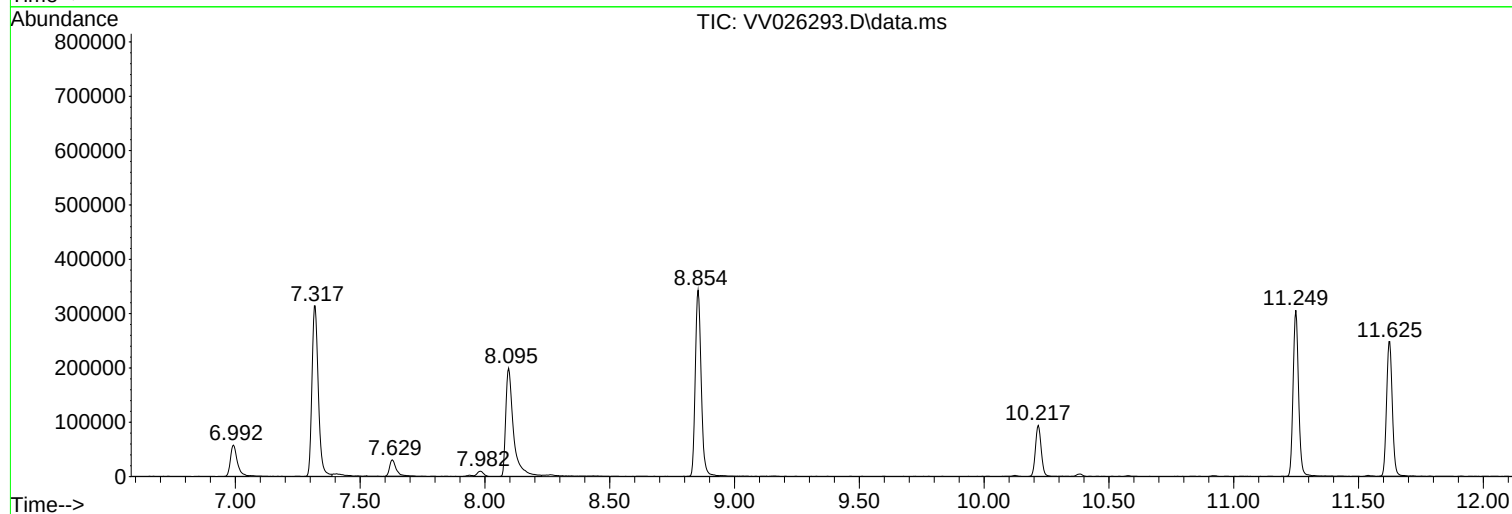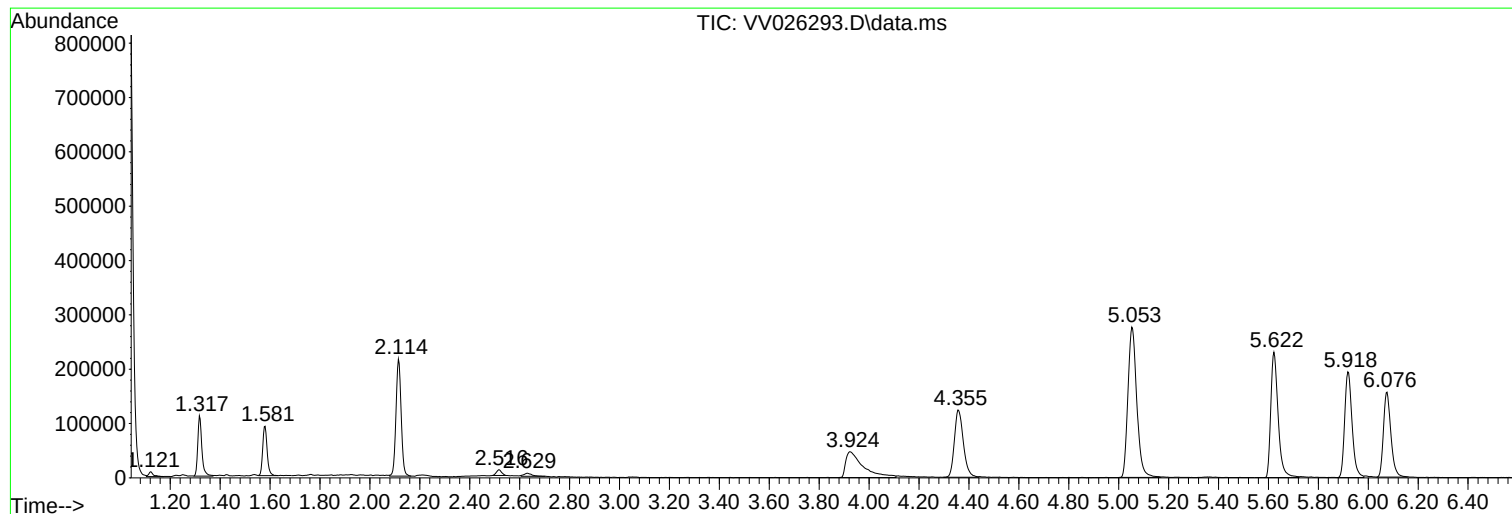

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026293.D
Acq On : 15 Jun 2022 21:20
Operator : SY/MD
Sample : N3275-12DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026293.D
Acq On : 15 Jun 2022 21:20
Operator : SY/MD
Sample : N3275-12DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc