

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026294.D
 Acq On : 15 Jun 2022 21:44
 Operator : SY/MD
 Sample : N3275-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026294.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	78	86	103	rVB	113196	119423	2.82%	1.221%
2	1.577	160	167	183	rVB	95478	110780	2.61%	1.132%
3	2.117	325	335	349	rVB	194884	278602	6.57%	2.847%
4	2.211	349	364	387	rBV2	21995	74648	1.76%	0.763%
5	2.433	396	433	493	rBV2	42308	487844	11.51%	4.986%
6	3.921	882	896	918	rBV3	49469	171809	4.05%	1.756%
7	4.359	1016	1032	1057	rBV	115002	291352	6.87%	2.978%
8	5.056	1233	1249	1277	rBV2	247525	610625	14.40%	6.241%
9	5.622	1413	1425	1448	rBV	213088	438383	10.34%	4.480%
10	5.918	1502	1517	1553	rBV	2203320	4239999	100.00%	43.334%
11	6.076	1553	1566	1596	rVB2	143207	303689	7.16%	3.104%
12	6.992	1841	1851	1873	rBV	52008	99737	2.35%	1.019%
13	7.320	1942	1953	1972	rBV	278222	497028	11.72%	5.080%
14	7.629	2040	2049	2070	rBV2	29205	55270	1.30%	0.565%
15	7.979	2147	2158	2174	rVB	72919	125263	2.95%	1.280%
16	8.092	2183	2193	2223	rBV2	186361	391442	9.23%	4.001%
17	8.854	2416	2430	2451	rBV	322808	534479	12.61%	5.463%
18	10.217	2843	2854	2871	rBV	88288	140199	3.31%	1.433%
19	11.249	3162	3175	3198	rBV	281765	442575	10.44%	4.523%
20	11.625	3280	3292	3309	rBV	234240	371274	8.76%	3.795%




Sum of corrected areas: 9784421

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026294.D
Acq On : 15 Jun 2022 21:44
Operator : SY/MD
Sample : N3275-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

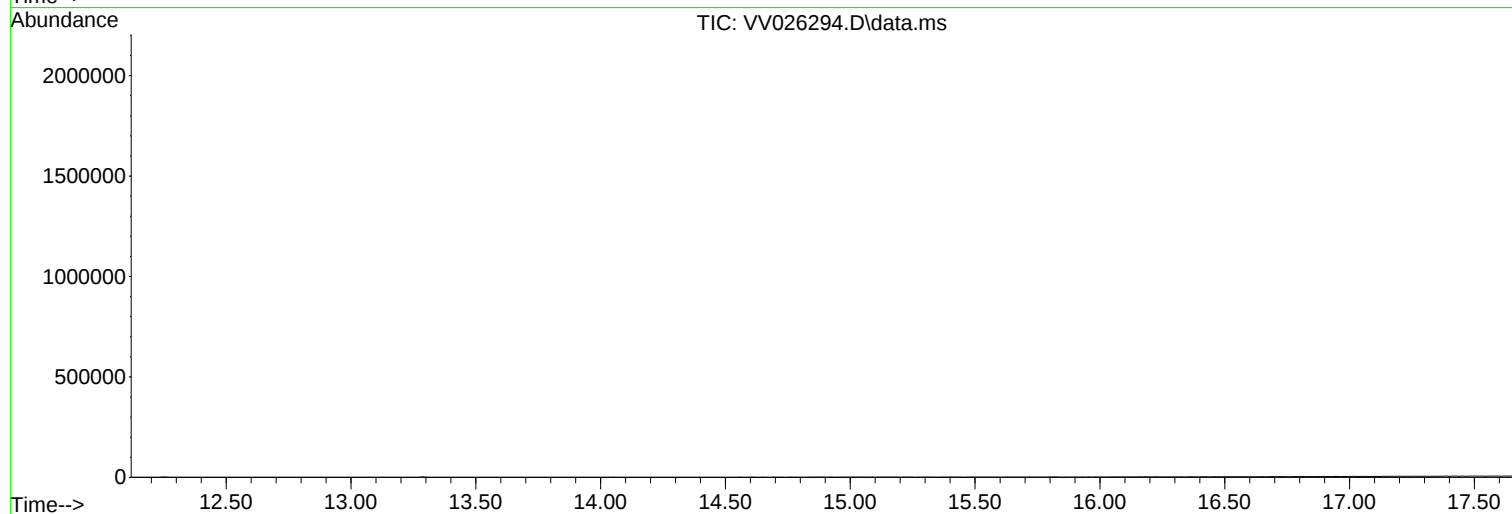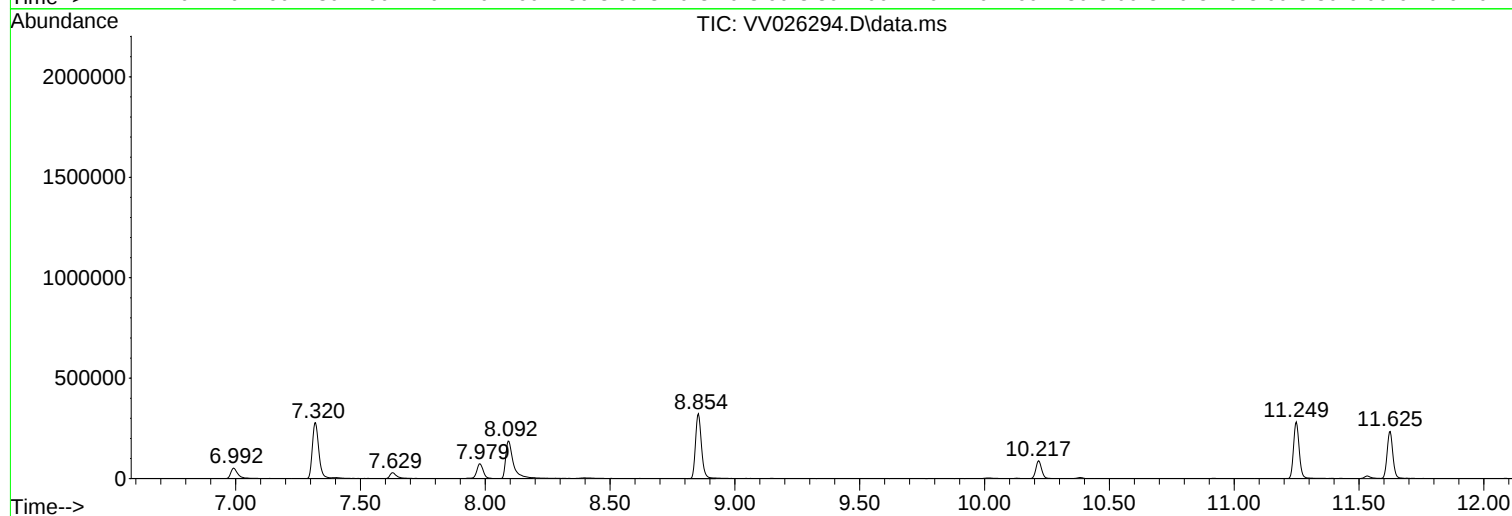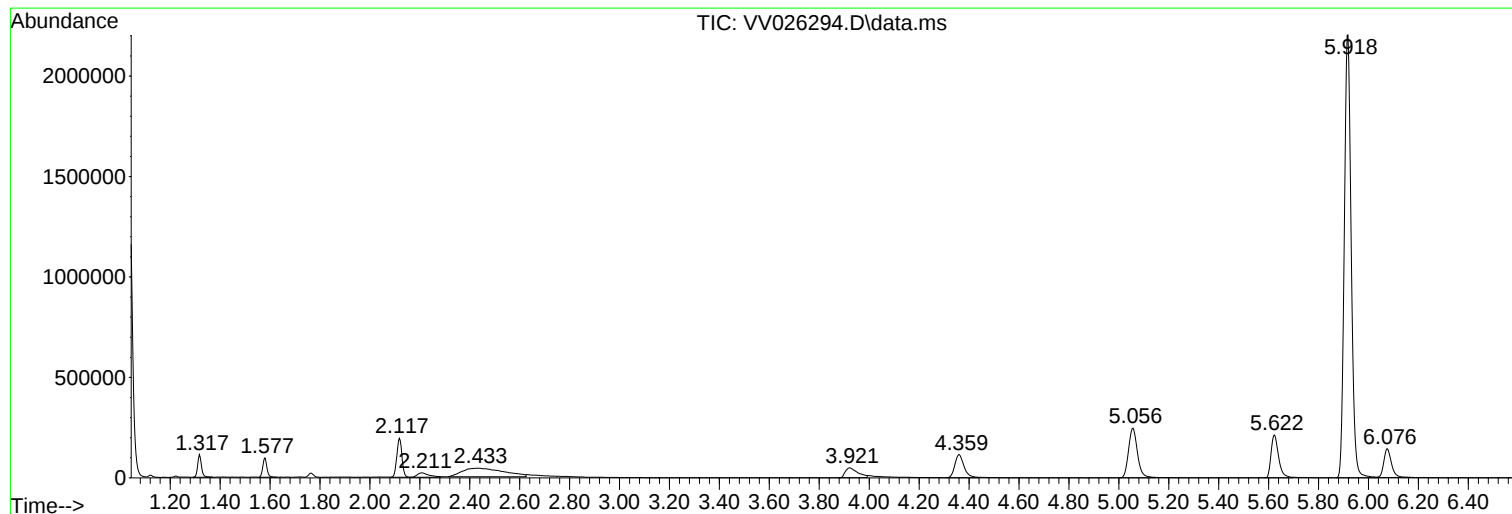

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026294.D
Acq On : 15 Jun 2022 21:44
Operator : SY/MD
Sample : N3275-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE4










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.433	5.56 ug/L	487844	1,4-Difluorobenzene	5.622

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
5			Methyltartronic acid	134	C4H6O5	000595-98-2	9

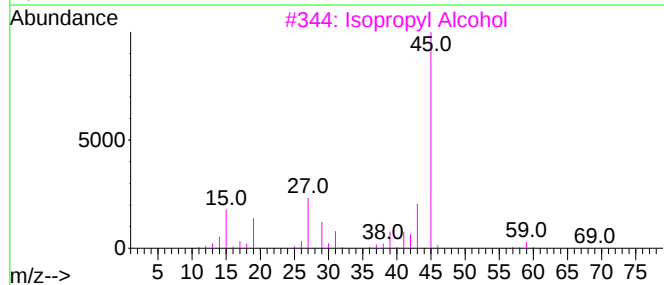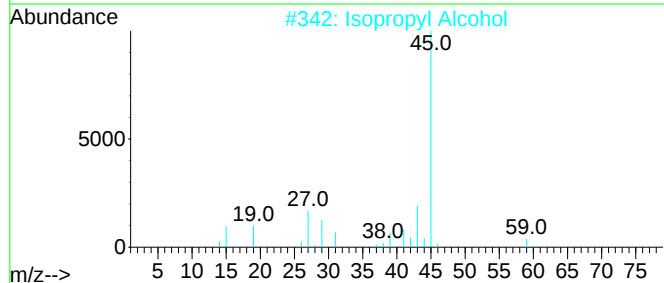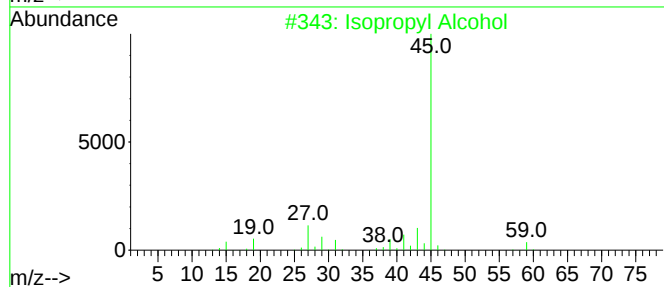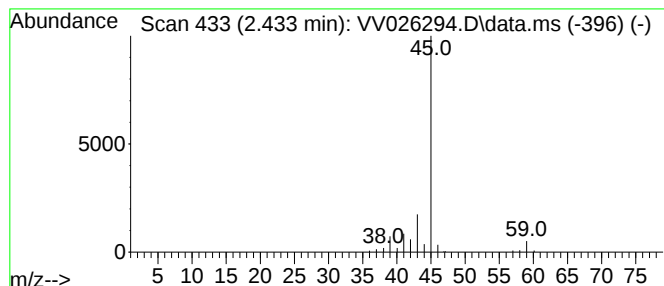

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026294.D
Acq On : 15 Jun 2022 21:44
Operator : SY/MD
Sample : N3275-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.433	5.6	ug/L	487844	1	5.622	438383	5.0