

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026299.D
 Acq On : 16 Jun 2022 00:08
 Operator : SY/MD
 Sample : N3273-15DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B90DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026299.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	21	26	39	rVB3	9653	11563	1.44%	0.174%
2	1.320	78	87	100	rBV	131508	145724	18.14%	2.193%
3	1.580	160	168	185	rVB	125799	142768	17.77%	2.148%
4	1.722	201	212	219	rBV	41724	52012	6.47%	0.783%
5	1.767	219	226	238	rVB	35571	47765	5.95%	0.719%
6	2.121	325	336	353	rVB	230552	336468	41.88%	5.063%
7	2.519	449	460	474	rBV	33705	57084	7.10%	0.859%
8	3.924	882	897	936	rBV3	63672	282241	35.13%	4.247%
9	4.362	1016	1033	1064	rVB	149626	379229	47.20%	5.707%
10	5.056	1233	1249	1283	rBV2	323127	803444	100.00%	12.090%
11	5.622	1414	1425	1457	rBV	241209	493998	61.49%	7.434%
12	5.927	1507	1520	1535	rBV7	17994	42071	5.24%	0.633%
13	6.075	1553	1566	1594	rBV	186929	384421	47.85%	5.785%
14	6.992	1837	1851	1873	rBV	61993	115758	14.41%	1.742%
15	7.320	1941	1953	1973	rBV	342641	596689	74.27%	8.979%
16	7.628	2039	2049	2073	rBV2	35515	67512	8.40%	1.016%
17	7.976	2138	2157	2175	rBV	254291	433680	53.98%	6.526%
18	8.091	2183	2193	2226	rBV2	275812	566341	70.49%	8.522%
19	8.853	2419	2430	2451	rBV	361142	587117	73.08%	8.835%
20	10.217	2842	2854	2875	rBV	120419	188947	23.52%	2.843%
21	11.249	3162	3175	3200	rBV	295304	459892	57.24%	6.920%
22	11.622	3279	3291	3310	rBV	283327	450694	56.10%	6.782%




Sum of corrected areas: 6645418

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026299.D
Acq On : 16 Jun 2022 00:08
Operator : SY/MD
Sample : N3273-15DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B90DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

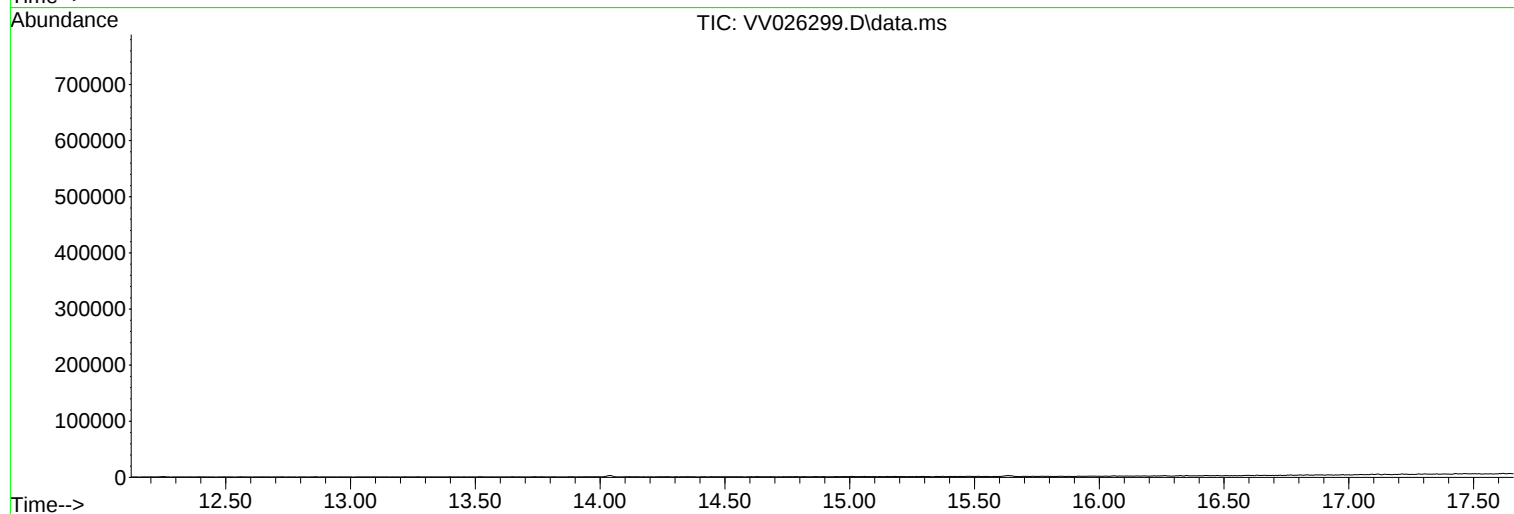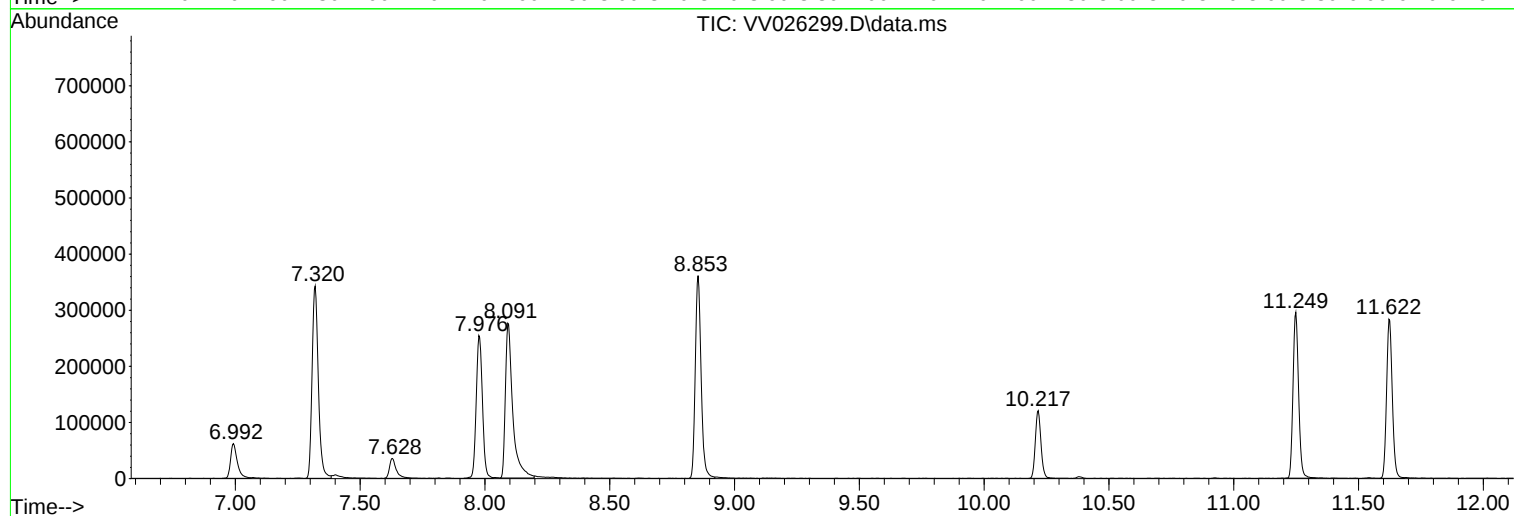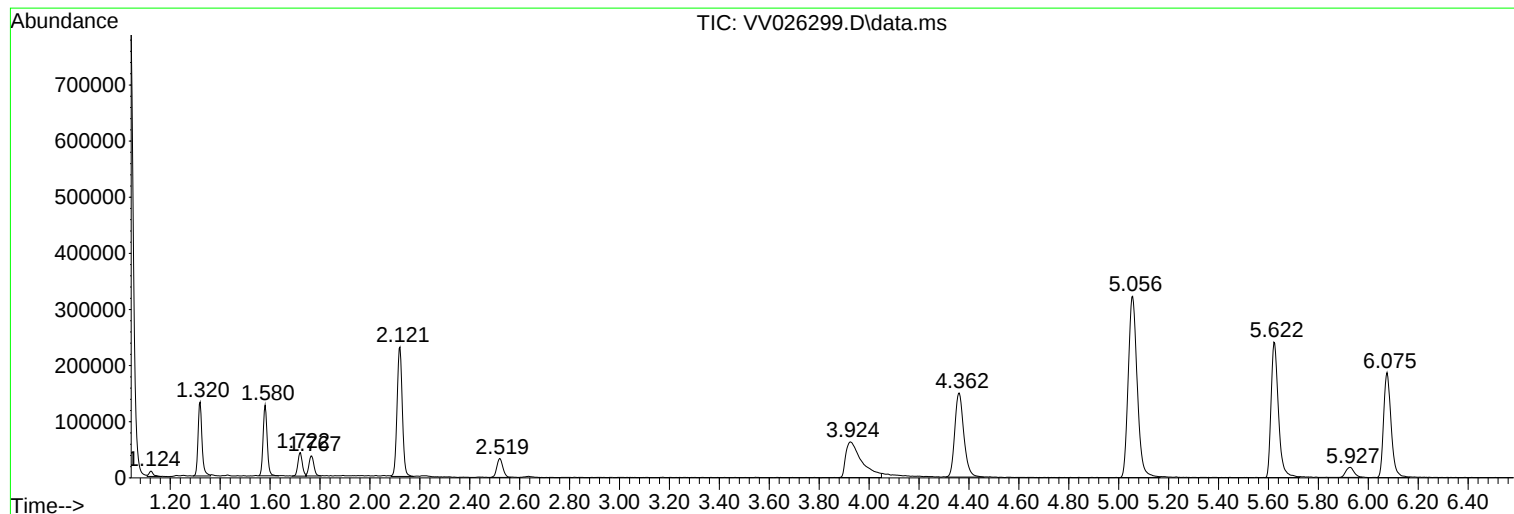

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026299.D
Acq On : 16 Jun 2022 00:08
Operator : SY/MD
Sample : N3273-15DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B90DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026299.D
Acq On : 16 Jun 2022 00:08
Operator : SY/MD
Sample : N3273-15DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B90DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc