

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026304.D
 Acq On : 16 Jun 2022 02:08
 Operator : SY/MD
 Sample : N3274-11DL 2500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BA1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026304.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	101	rBV	117727	124575	18.81%	2.216%
2	1.580	160	168	180	rBV	102933	117337	17.72%	2.087%
3	2.121	325	336	354	rVB	207250	298579	45.09%	5.311%
4	3.924	881	897	925	rBV2	44523	183868	27.77%	3.270%
5	4.362	1016	1033	1057	rBV2	122275	306445	46.28%	5.450%
6	5.056	1233	1249	1284	rBV2	270038	662164	100.00%	11.777%
7	5.625	1413	1426	1461	rBV	220103	455317	68.76%	8.098%
8	5.921	1505	1518	1549	rBV	254691	509784	76.99%	9.067%
9	6.075	1553	1566	1596	rVB	152335	315797	47.69%	5.617%
10	6.992	1841	1851	1875	rBV	53879	105889	15.99%	1.883%
11	7.320	1941	1953	1973	rBV	304089	531462	80.26%	9.453%
12	7.628	2040	2049	2066	rBV2	30566	55927	8.45%	0.995%
13	7.982	2150	2159	2170	rVB3	10909	19214	2.90%	0.342%
14	8.091	2184	2193	2229	rBV	194474	406788	61.43%	7.235%
15	8.853	2418	2430	2455	rBV	333875	546336	82.51%	9.717%
16	10.217	2841	2854	2871	rBV	92296	148263	22.39%	2.637%
17	11.246	3164	3174	3203	rBV	285099	445377	67.26%	7.921%
18	11.622	3280	3291	3309	rBV	247280	389295	58.79%	6.924%




Sum of corrected areas: 5622417

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026304.D
Acq On : 16 Jun 2022 02:08
Operator : SY/MD
Sample : N3274-11DL 2500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

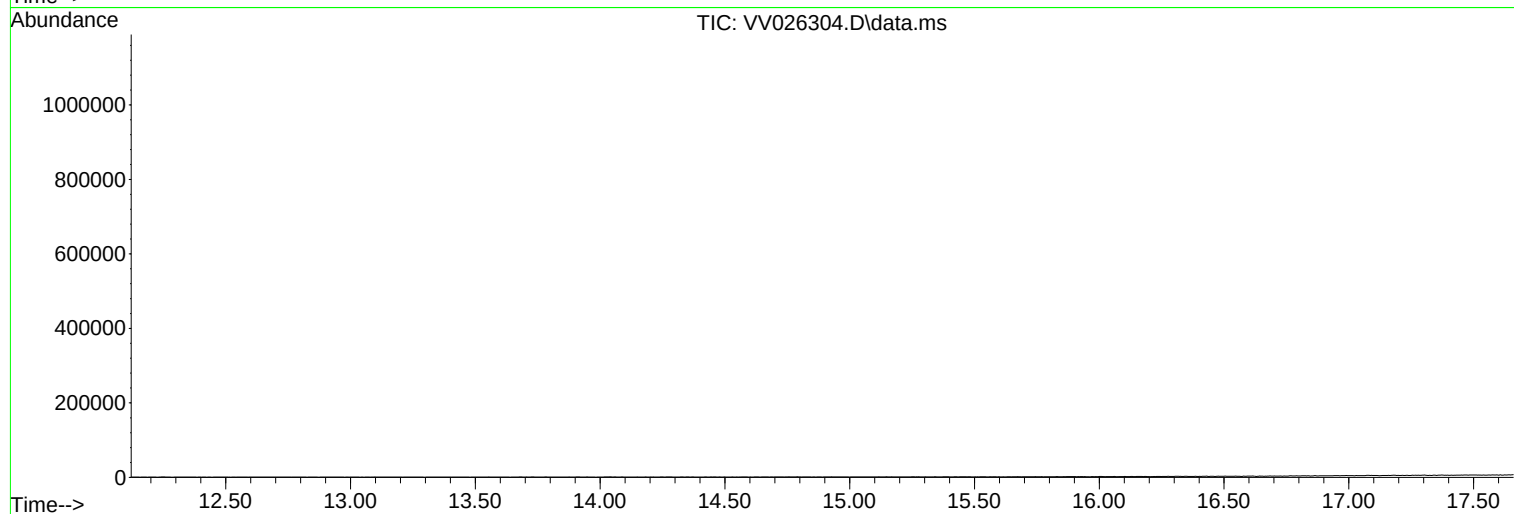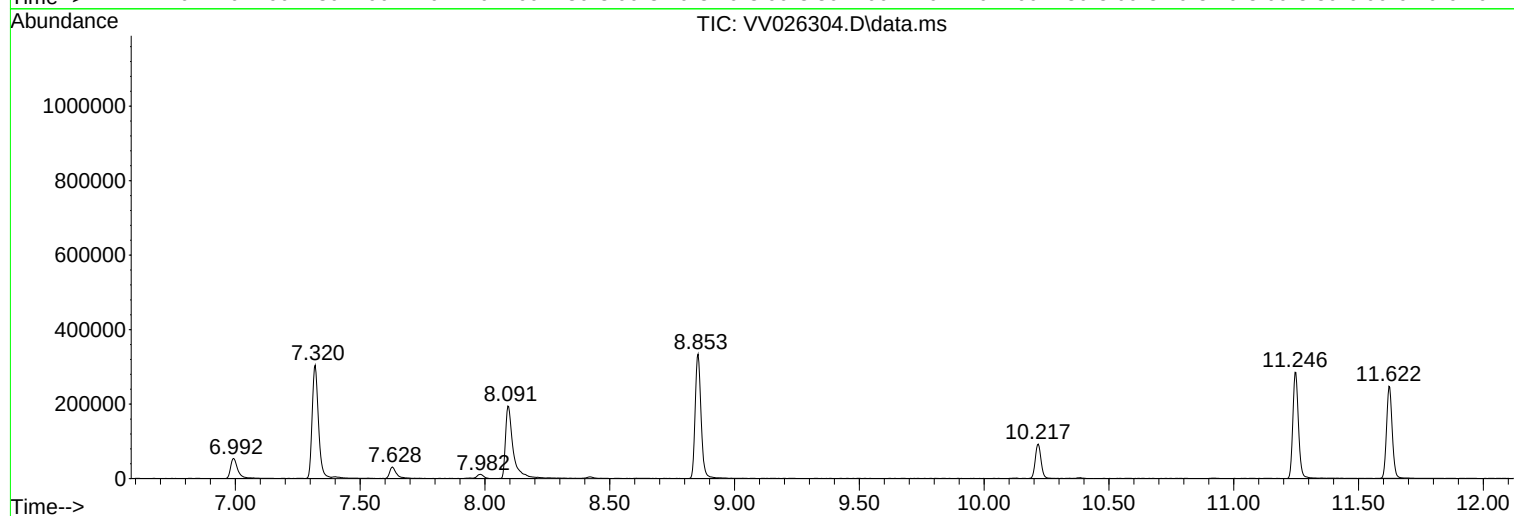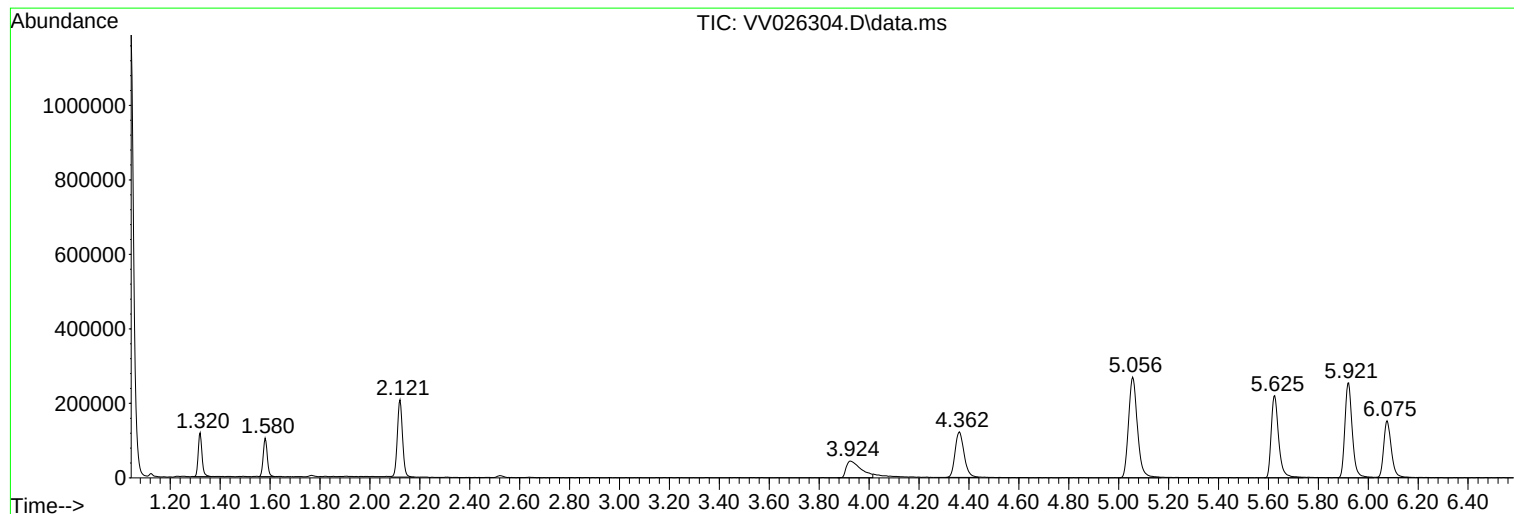

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026304.D
Acq On : 16 Jun 2022 02:08
Operator : SY/MD
Sample : N3274-11DL 2500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026304.D
Acq On : 16 Jun 2022 02:08
Operator : SY/MD
Sample : N3274-11DL 2500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc