

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026306.D
 Acq On : 16 Jun 2022 02:55
 Operator : SY/MD
 Sample : N3274-05DL 1000X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B95DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026306.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	102	rBV	117413	123868	16.39%	2.081%
2	1.580	159	168	184	rBV	100495	117321	15.53%	1.971%
3	2.121	325	336	355	rVB	201441	292630	38.73%	4.916%
4	2.523	450	461	475	rBV3	6928	11902	1.58%	0.200%
5	3.928	881	898	949	rBV3	54757	264483	35.01%	4.443%
6	4.362	1017	1033	1063	rBV2	120931	304303	40.28%	5.112%
7	5.056	1232	1249	1281	rBV2	259432	648011	85.77%	10.886%
8	5.625	1413	1426	1453	rBV	217637	449694	59.52%	7.554%
9	5.918	1504	1517	1552	rBV	379621	755556	100.00%	12.693%
10	6.075	1553	1566	1589	rVV	152049	308290	40.80%	5.179%
11	6.992	1841	1851	1881	rBV2	52855	103584	13.71%	1.740%
12	7.320	1942	1953	1975	rBV	294322	523125	69.24%	8.788%
13	7.628	2039	2049	2064	rBV	30558	55380	7.33%	0.930%
14	7.979	2148	2158	2174	rVB2	32332	56966	7.54%	0.957%
15	8.091	2183	2193	2240	rBV2	188981	405839	53.71%	6.818%
16	8.419	2284	2295	2312	rBV4	13896	24615	3.26%	0.414%
17	8.853	2416	2430	2456	rBV	332738	541986	71.73%	9.105%
18	10.217	2842	2854	2869	rBV	94168	147077	19.47%	2.471%
19	11.249	3164	3175	3199	rBV	275815	437477	57.90%	7.349%
20	11.622	3277	3291	3314	rBV	237423	380568	50.37%	6.393%




Sum of corrected areas: 5952675

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026306.D
Acq On : 16 Jun 2022 02:55
Operator : SY/MD
Sample : N3274-05DL 1000X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B95DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

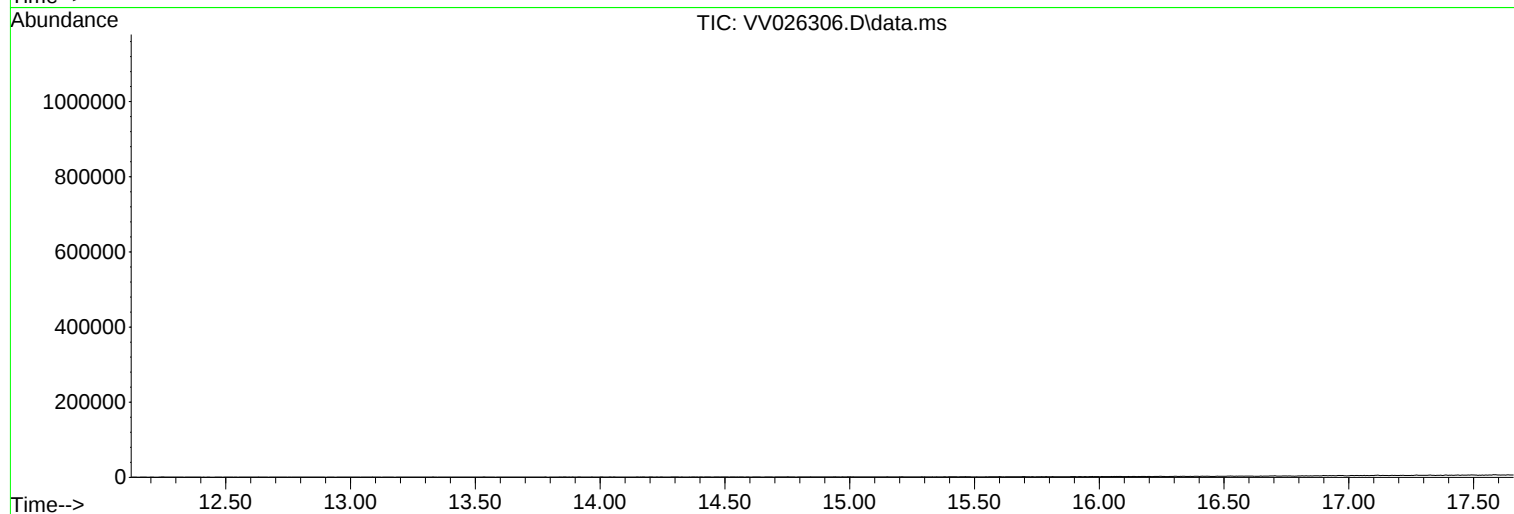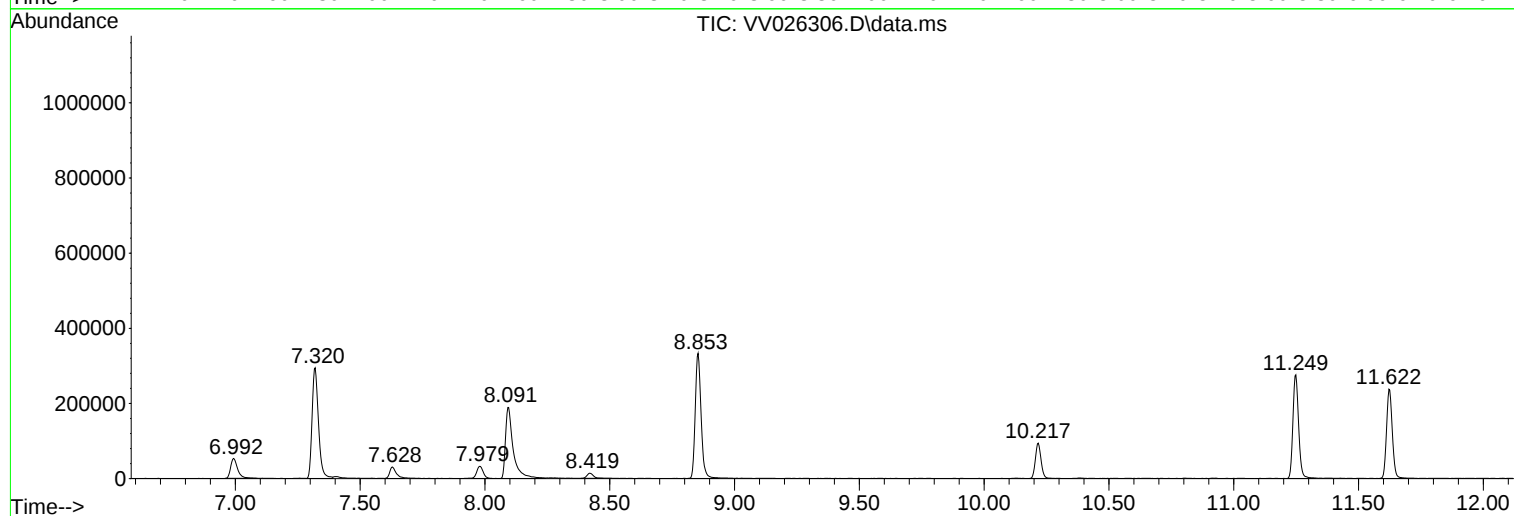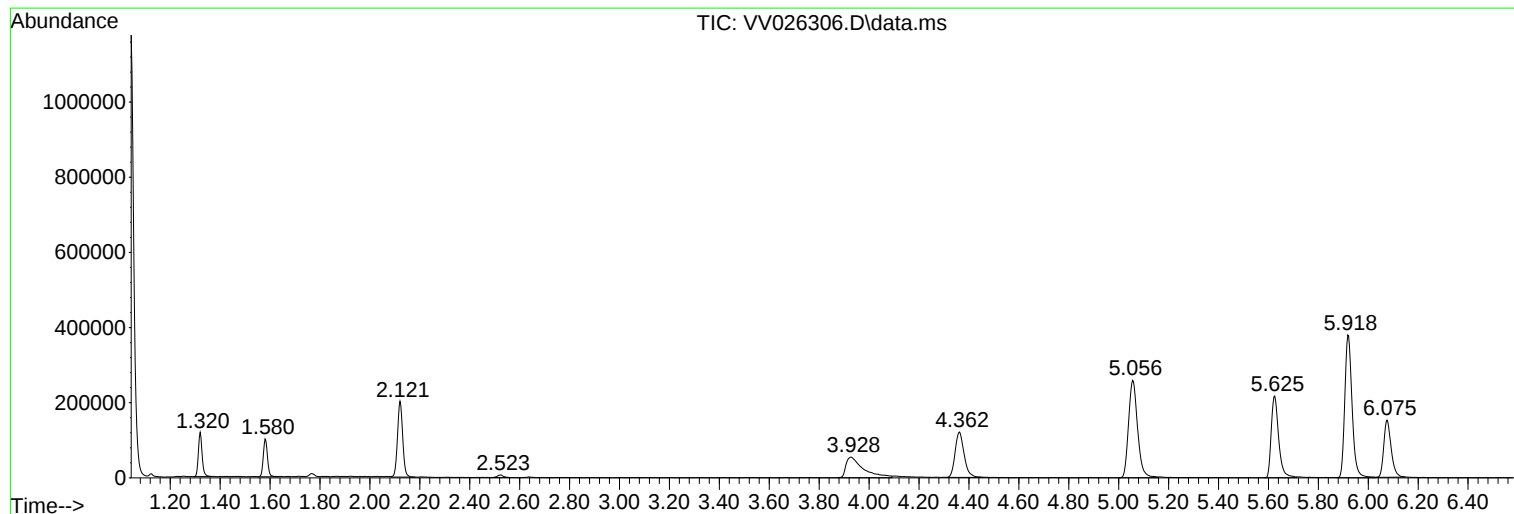

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026306.D
Acq On : 16 Jun 2022 02:55
Operator : SY/MD
Sample : N3274-05DL 1000X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B95DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026306.D
Acq On : 16 Jun 2022 02:55
Operator : SY/MD
Sample : N3274-05DL 1000X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B95DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc