

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026307.D
 Acq On : 16 Jun 2022 03:19
 Operator : SY/MD
 Sample : N3274-12 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BA2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026307.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	103	rBV	104122	119596	11.02%	1.846%
2	1.580	160	168	182	rBV	89518	107440	9.90%	1.658%
3	1.764	216	225	236	rBV	136011	173960	16.03%	2.685%
4	2.117	324	335	351	rVB	204450	300102	27.66%	4.632%
5	2.519	449	460	473	rBV	15401	26057	2.40%	0.402%
6	2.629	486	494	509	rVB2	8270	16690	1.54%	0.258%
7	3.928	883	898	943	rBV3	45203	217402	20.03%	3.355%
8	4.359	1016	1032	1061	rBV	118933	303003	27.92%	4.676%
9	5.056	1234	1249	1276	rBV2	266795	653256	60.20%	10.082%
10	5.622	1411	1425	1450	rBV	235821	483959	44.60%	7.469%
11	5.924	1504	1519	1537	rBV6	15066	34137	3.15%	0.527%
12	6.075	1553	1566	1592	rBV	148663	307487	28.34%	4.746%
13	6.992	1838	1851	1874	rBV	53211	103045	9.50%	1.590%
14	7.320	1941	1953	1973	rBV	296837	524158	48.30%	8.090%
15	7.628	2039	2049	2064	rBV2	29341	52899	4.87%	0.816%
16	7.976	2142	2157	2178	rBV	648071	1085112	100.00%	16.747%
17	8.095	2184	2194	2221	rBV	187681	404465	37.27%	6.242%
18	8.854	2418	2430	2452	rBV	350679	570730	52.60%	8.809%
19	10.217	2842	2854	2870	rBV	91974	144717	13.34%	2.234%
20	11.249	3164	3175	3195	rBV	303255	466266	42.97%	7.196%
21	11.625	3280	3292	3308	rBV	243731	384798	35.46%	5.939%




Sum of corrected areas: 6479279

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026307.D
Acq On : 16 Jun 2022 03:19
Operator : SY/MD
Sample : N3274-12 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

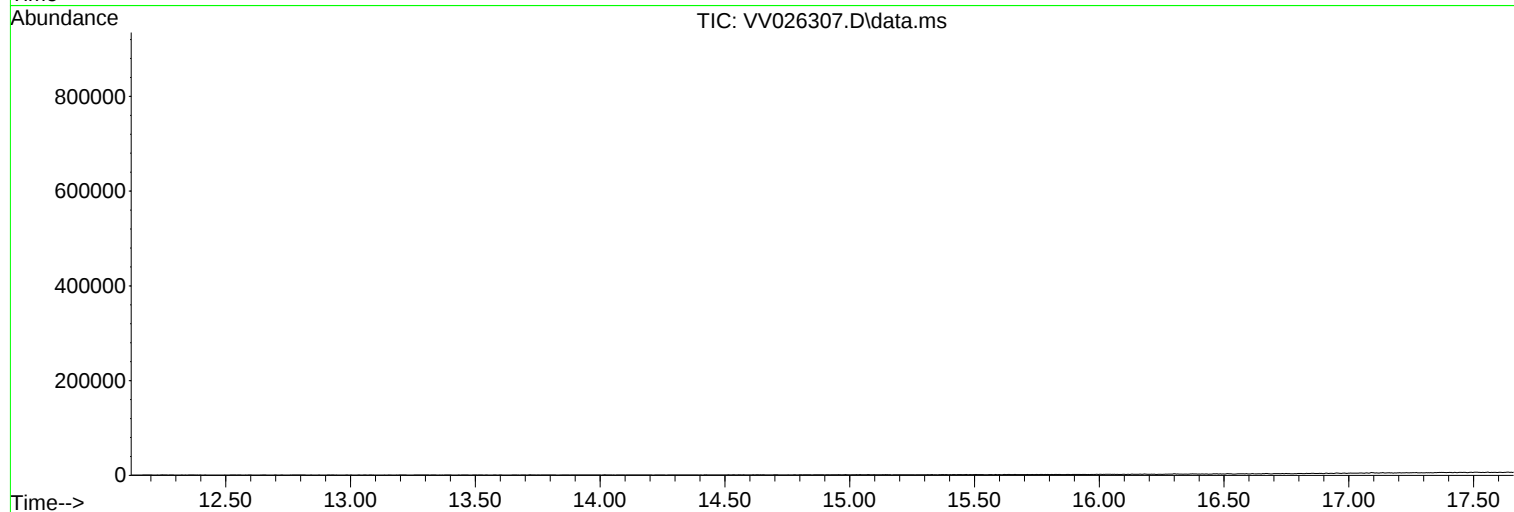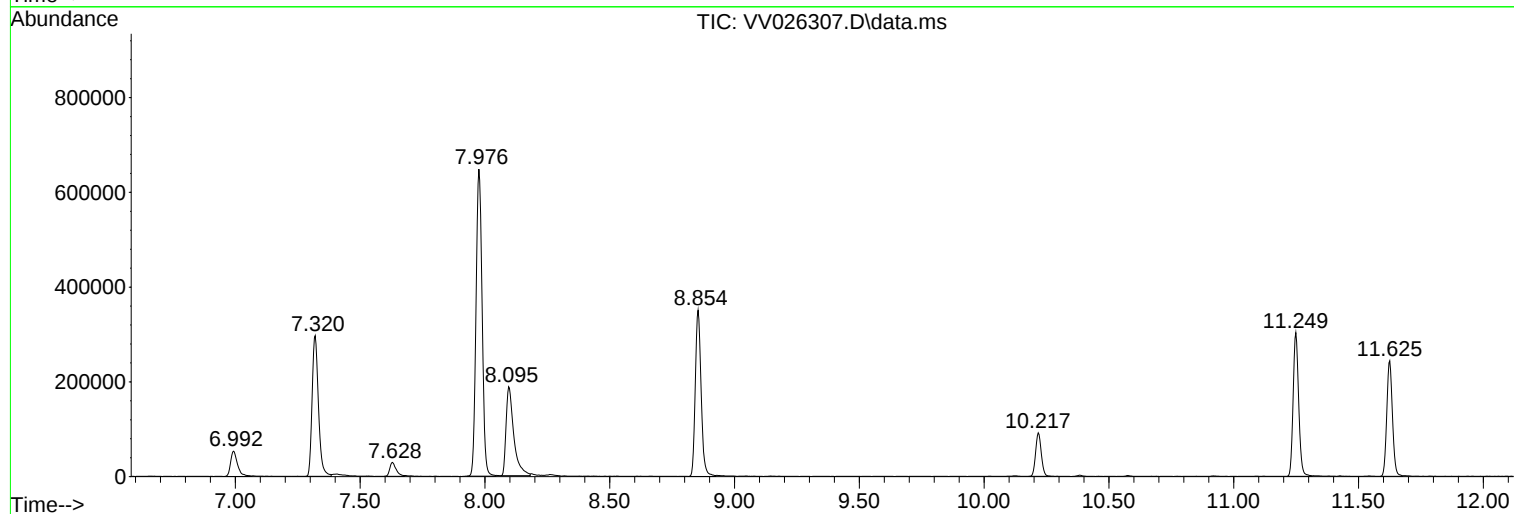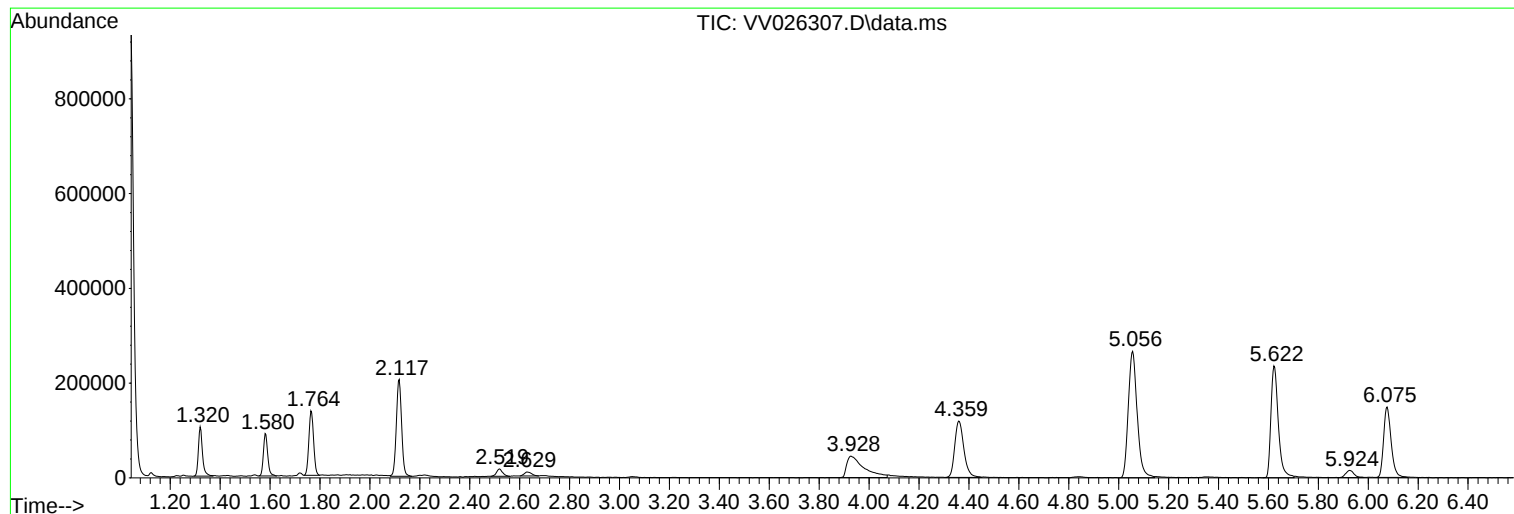

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026307.D
Acq On : 16 Jun 2022 03:19
Operator : SY/MD
Sample : N3274-12 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026307.D
Acq On : 16 Jun 2022 03:19
Operator : SY/MD
Sample : N3274-12 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
