

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026308.D
 Acq On : 16 Jun 2022 03:43
 Operator : SY/MD
 Sample : N3274-13 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BA3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026308.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	21	26	39	rVB3	11061	12940	2.03%	0.223%
2	1.320	77	87	108	rBV	116895	127100	19.91%	2.190%
3	1.580	160	168	183	rVB	98653	112177	17.57%	1.933%
4	1.719	204	211	218	rBV	24427	29286	4.59%	0.505%
5	1.767	218	226	239	rVB	50200	66363	10.40%	1.143%
6	2.121	324	336	350	rBV	198848	283978	44.49%	4.893%
7	2.519	452	460	474	rVB2	6776	12844	2.01%	0.221%
8	3.928	881	898	947	rBV2	47626	231405	36.25%	3.987%
9	4.362	1017	1033	1058	rBV	117356	297737	46.65%	5.130%
10	5.056	1233	1249	1278	rBV2	259069	638278	100.00%	10.998%
11	5.625	1414	1426	1453	rBV	222992	460931	72.21%	7.942%
12	5.924	1508	1519	1534	rBV8	13573	30603	4.79%	0.527%
13	6.075	1553	1566	1591	rBV	147990	305873	47.92%	5.270%
14	6.992	1841	1851	1873	rBV	52900	99691	15.62%	1.718%
15	7.320	1941	1953	1973	rBV	283636	506762	79.40%	8.732%
16	7.628	2039	2049	2076	rBV	28762	54529	8.54%	0.940%
17	7.976	2144	2157	2181	rBV	372139	625849	98.05%	10.784%
18	8.095	2184	2194	2224	rBV2	188580	391446	61.33%	6.745%
19	8.853	2418	2430	2465	rBV	338302	554376	86.85%	9.552%
20	10.217	2842	2854	2880	rBV	91153	144333	22.61%	2.487%
21	11.249	3164	3175	3204	rBV	288656	445672	69.82%	7.679%
22	11.622	3280	3291	3311	rBV	239898	371326	58.18%	6.398%




Sum of corrected areas: 5803499

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026308.D
Acq On : 16 Jun 2022 03:43
Operator : SY/MD
Sample : N3274-13 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

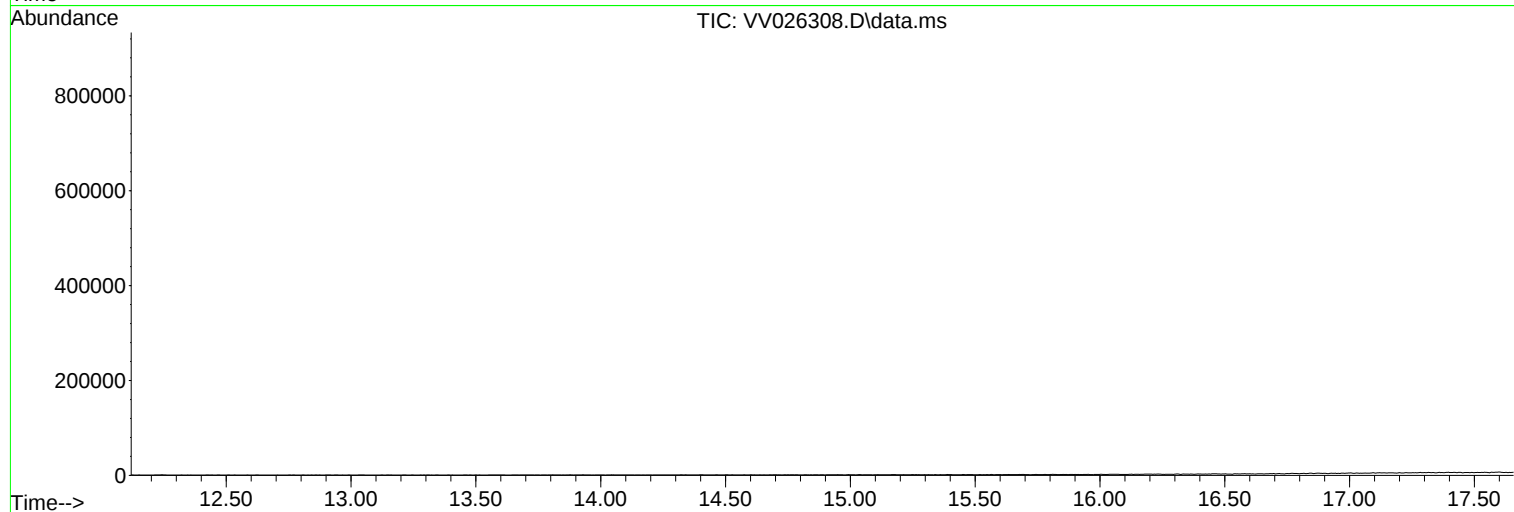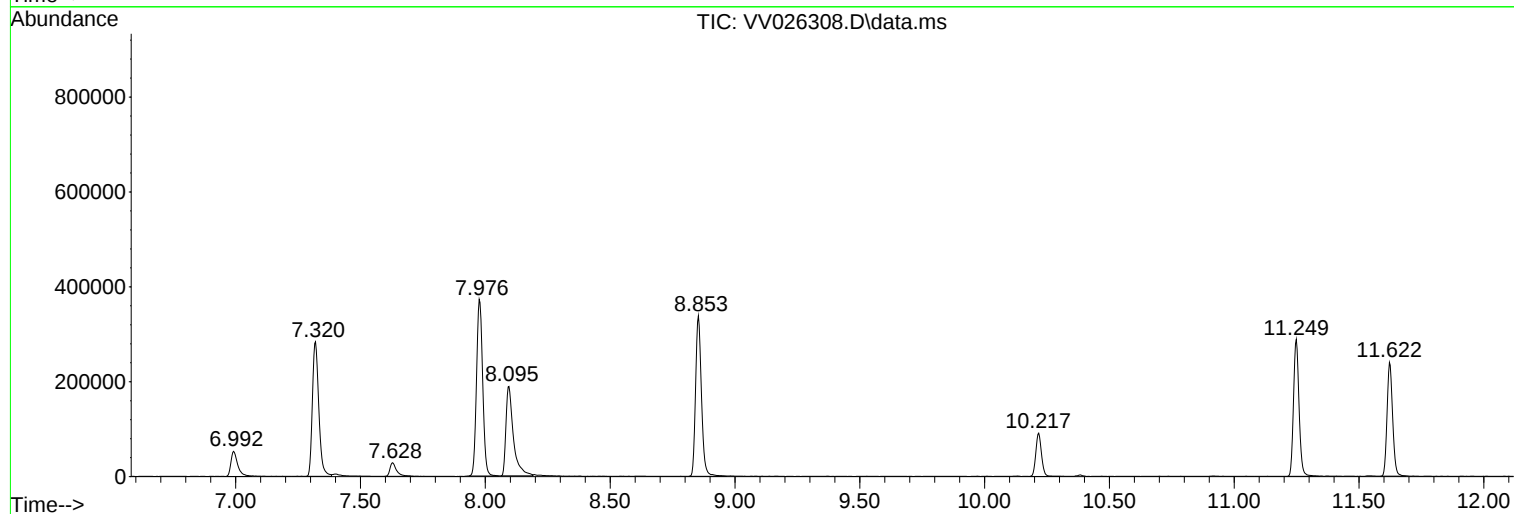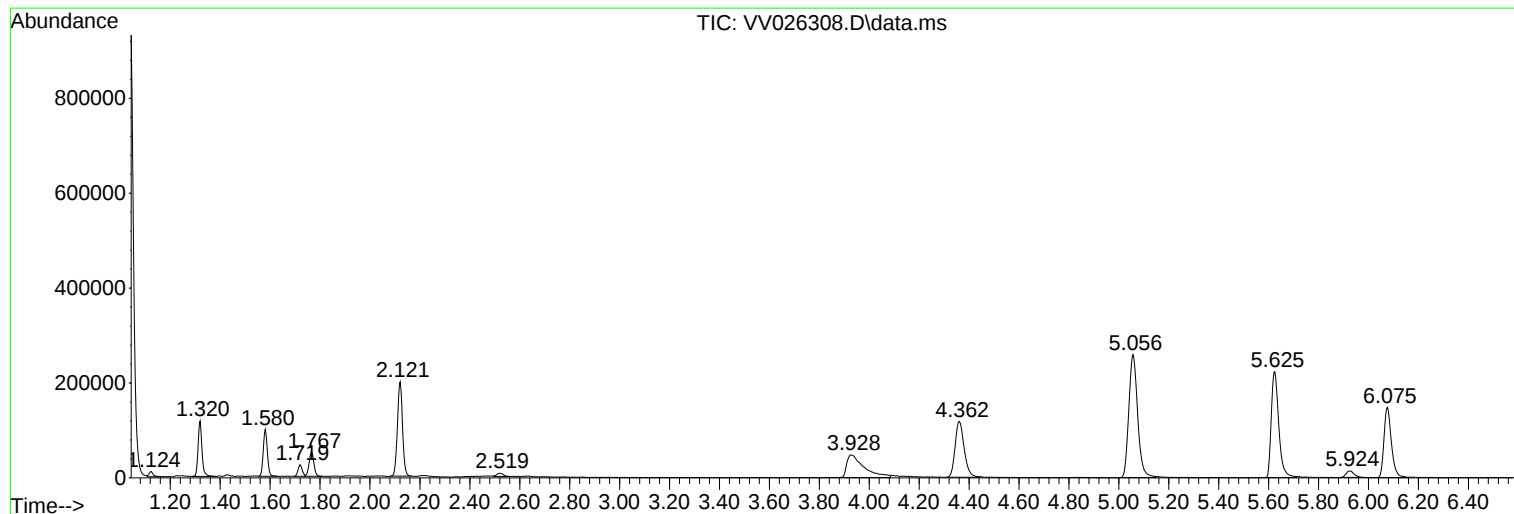

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026308.D
Acq On : 16 Jun 2022 03:43
Operator : SY/MD
Sample : N3274-13 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026308.D
Acq On : 16 Jun 2022 03:43
Operator : SY/MD
Sample : N3274-13 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
