

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026309.D
 Acq On : 16 Jun 2022 04:07
 Operator : SY/MD
 Sample : N3274-14 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BB7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026309.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	99	rBV	114969	120676	15.13%	1.824%
2	1.581	161	168	182	rBV	99638	113554	14.23%	1.716%
3	1.767	217	226	238	rVB	108127	141444	17.73%	2.138%
4	2.121	324	336	353	rVB	202528	292202	36.63%	4.417%
5	3.925	883	897	935	rBV3	42232	185488	23.25%	2.804%
6	4.362	1018	1033	1065	rBV2	118331	299334	37.52%	4.525%
7	5.056	1233	1249	1277	rBV2	256989	638253	80.01%	9.648%
8	5.622	1413	1425	1455	rBV	222756	468989	58.79%	7.089%
9	5.918	1504	1517	1544	rBV	300543	601288	75.37%	9.089%
10	6.076	1551	1566	1601	rVB	147866	306574	38.43%	4.634%
11	6.992	1840	1851	1878	rBV2	52904	103630	12.99%	1.566%
12	7.320	1941	1953	1971	rBV	290174	511831	64.16%	7.737%
13	7.629	2037	2049	2071	rBV	29341	54299	6.81%	0.821%
14	7.976	2145	2157	2184	rBV	484098	797729	100.00%	12.058%
15	8.095	2184	2194	2226	rBV2	187569	391299	49.05%	5.915%
16	8.854	2418	2430	2455	rBV	344836	566404	71.00%	8.561%
17	10.217	2842	2854	2872	rBV	87589	140589	17.62%	2.125%
18	10.998	3088	3097	3108	rBV2	20552	33404	4.19%	0.505%
19	11.249	3160	3175	3196	rBV	300211	469067	58.80%	7.090%
20	11.622	3279	3291	3309	rBV	238585	379668	47.59%	5.739%




Sum of corrected areas: 6615722

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026309.D
Acq On : 16 Jun 2022 04:07
Operator : SY/MD
Sample : N3274-14 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

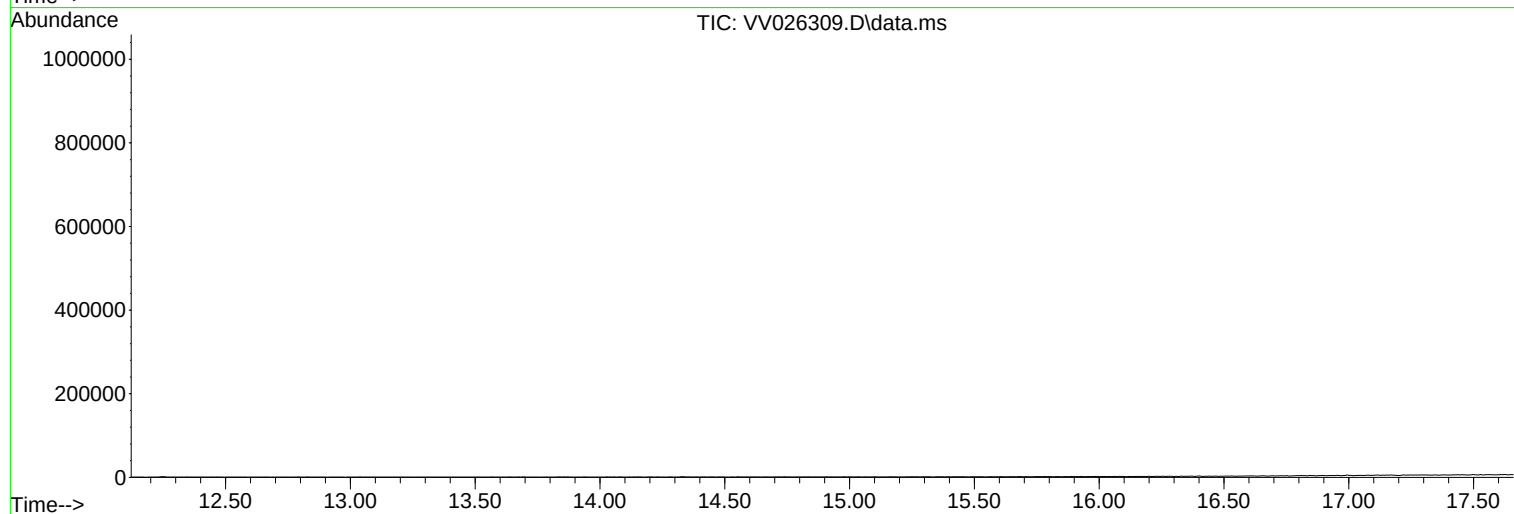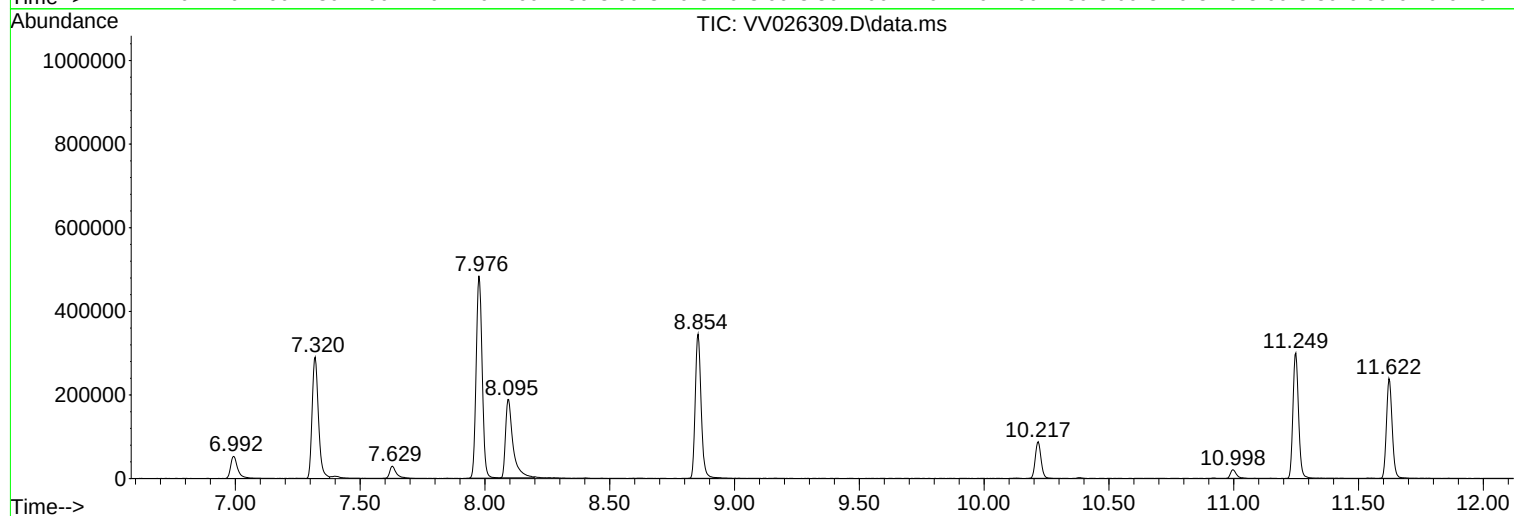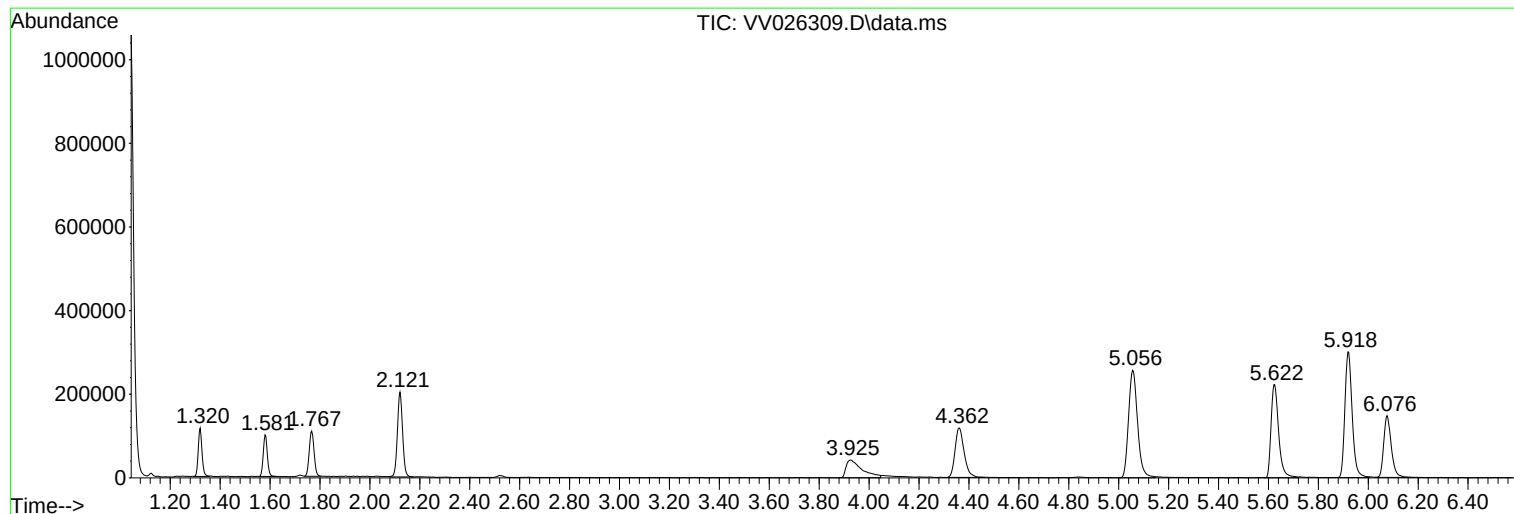

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026309.D
Acq On : 16 Jun 2022 04:07
Operator : SY/MD
Sample : N3274-14 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026309.D
Acq On : 16 Jun 2022 04:07
Operator : SY/MD
Sample : N3274-14 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc