

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026315.D
 Acq On : 16 Jun 2022 06:30
 Operator : SY/MD
 Sample : N3274-03DL 40000X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B93DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026315.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	80	87	100	rVB	112158	117451	12.79%	2.008%
2	1.581	160	168	179	rBV	95451	109915	11.97%	1.880%
3	2.121	325	336	358	rVB	193584	282663	30.79%	4.834%
4	3.931	881	899	953	rBV3	51182	247342	26.94%	4.230%
5	4.362	1016	1033	1057	rBV	115409	288261	31.40%	4.929%
6	5.056	1233	1249	1279	rBV2	250002	618901	67.41%	10.583%
7	5.625	1414	1426	1454	rBV	214486	447456	48.74%	7.652%
8	5.918	1505	1517	1552	rBV2	459572	918047	100.00%	15.699%
9	6.076	1552	1566	1598	rVB	146392	306253	33.36%	5.237%
10	6.992	1840	1851	1879	rBV	51284	98730	10.75%	1.688%
11	7.320	1941	1953	1972	rBV	287086	497116	54.15%	8.501%
12	7.629	2040	2049	2077	rVB2	27288	51879	5.65%	0.887%
13	8.095	2184	2194	2222	rBV2	176621	373059	40.64%	6.379%
14	8.420	2286	2295	2309	rVB3	9168	15541	1.69%	0.266%
15	8.854	2418	2430	2451	rBV	325279	537908	58.59%	9.198%
16	10.217	2839	2854	2875	rBV	89109	139799	15.23%	2.391%
17	11.249	3164	3175	3195	rBV	278062	433822	47.25%	7.418%
18	11.622	3280	3291	3313	rBV	230909	363742	39.62%	6.220%




Sum of corrected areas: 5847885

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026315.D
Acq On : 16 Jun 2022 06:30
Operator : SY/MD
Sample : N3274-03DL 40000X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B93DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

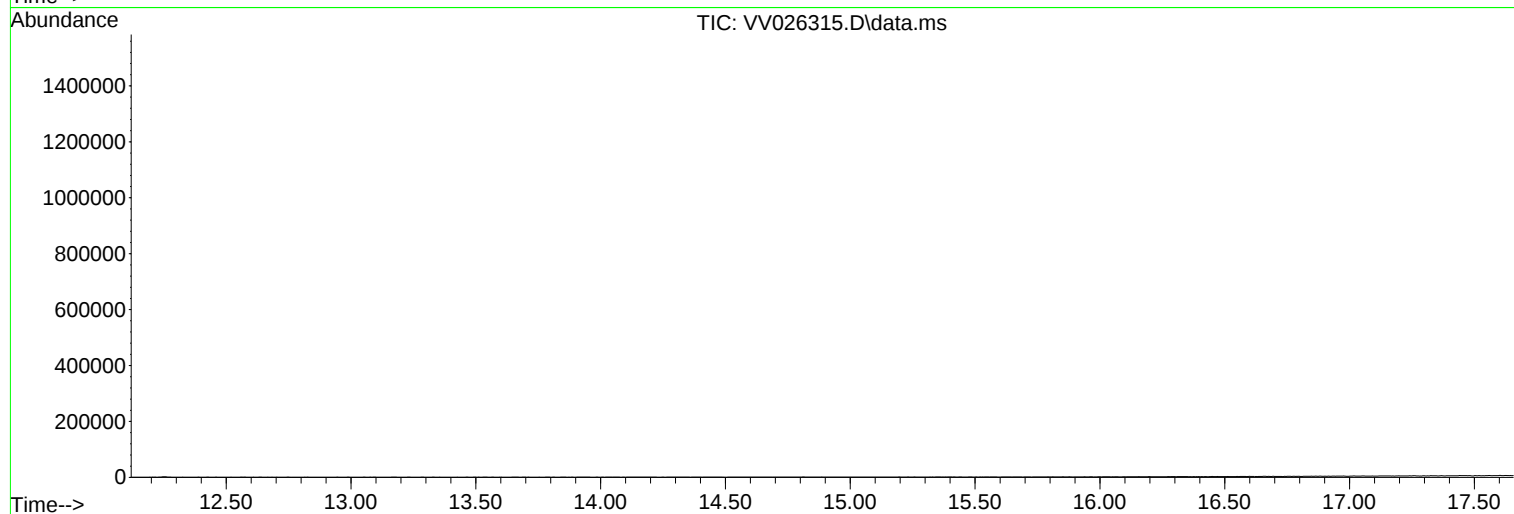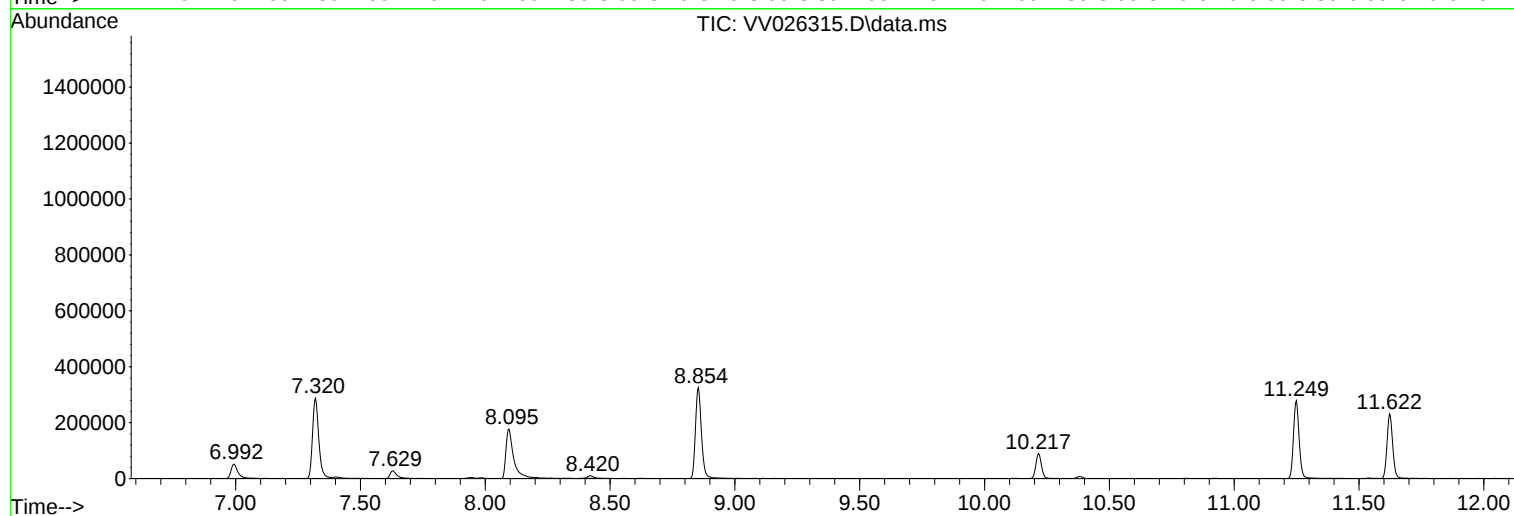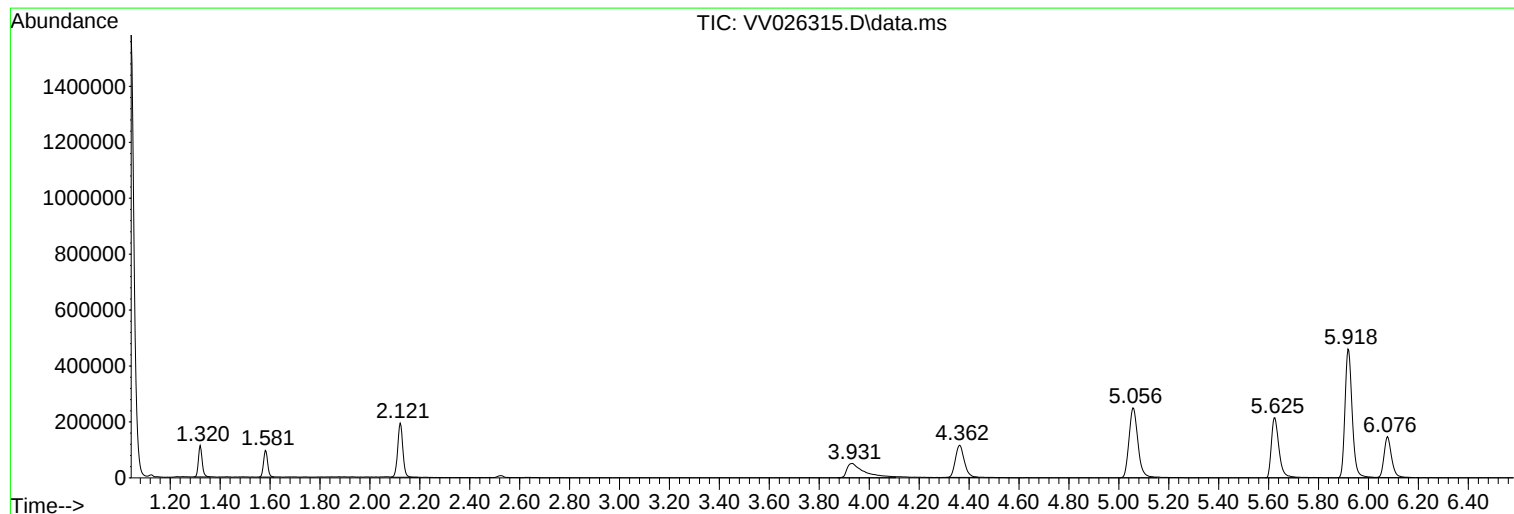

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026315.D
Acq On : 16 Jun 2022 06:30
Operator : SY/MD
Sample : N3274-03DL 40000X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B93DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026315.D
Acq On : 16 Jun 2022 06:30
Operator : SY/MD
Sample : N3274-03DL 40000X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B93DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
