
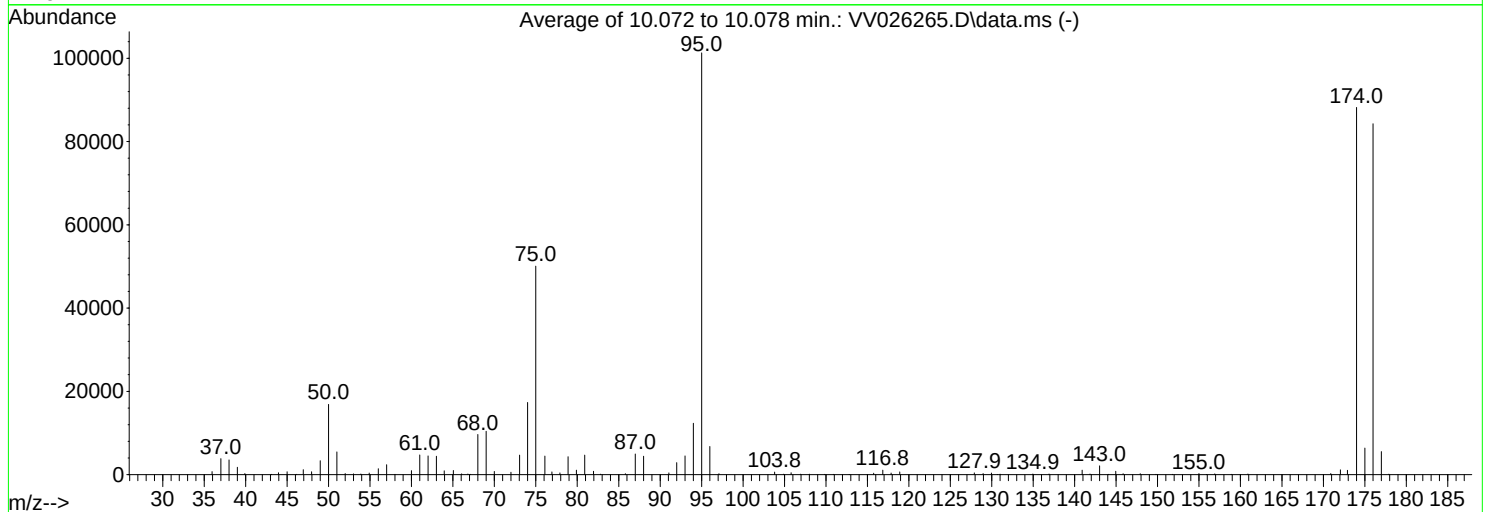


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026265.D
Acq On : 15 Jun 2022 09:16
Operator : SY/MD
Sample : BFB329
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB329

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jun 17 06:57:04 2022

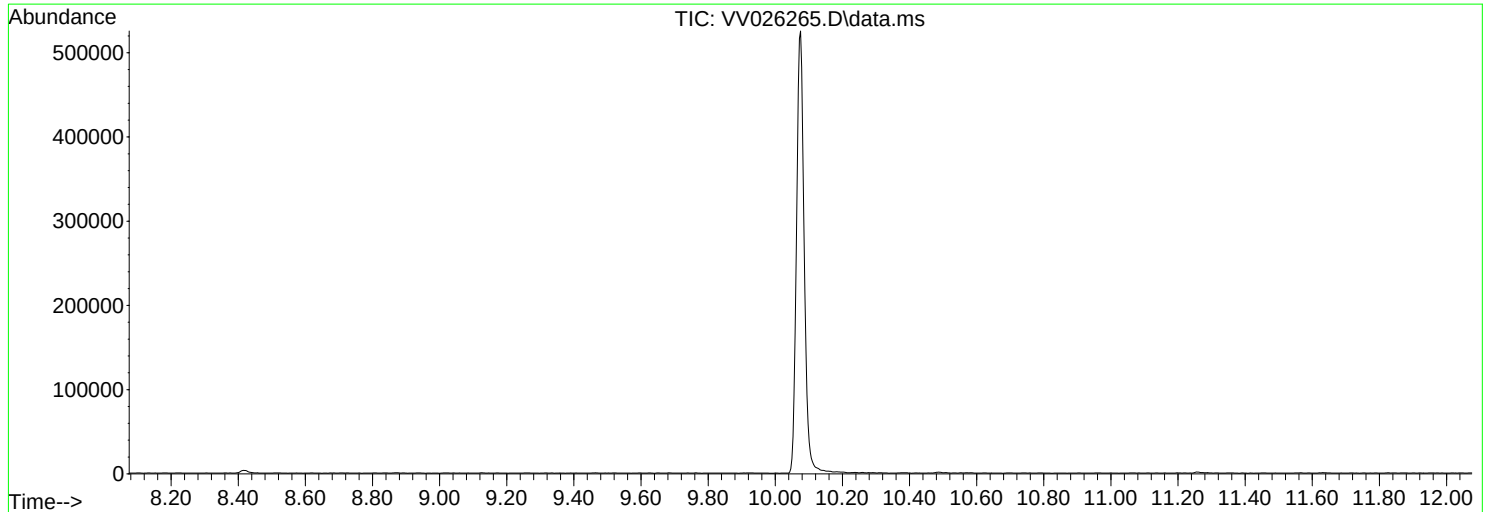

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	16890	PASS
75	95	30	80	49.4	50069	PASS
95	95	100	100	100.0	101304	PASS
96	95	5	9	6.7	6755	PASS
173	174	0.00	2	1.2	1024	PASS
174	95	50	120	87.0	88176	PASS
175	174	5	9	7.3	6395	PASS
176	174	95	105	95.6	84259	PASS
177	176	5	10	6.6	5545	PASS

m/z	Abundance
39.90	624.0
44.00	285.0

Instrument :
MSVOA_V
ClientSampleId :
BFB329

m/z	Abundance
35.90	788.0
37.00	4102.0
38.00	3650.0
39.00	1728.0
40.00	900.0
43.10	110.0
43.90	783.0
45.00	732.0
46.10	164.0
47.00	1258.0
48.00	725.0
49.00	3511.0
50.00	17424.0
51.00	5548.0
52.00	295.0
53.00	161.0
53.90	158.0
54.90	408.0
56.00	1370.0
57.00	2549.0
58.00	132.0
60.00	916.0
61.00	4779.0
62.00	4590.0
63.00	4520.0
64.00	893.0
65.10	1043.0
66.10	209.0
66.80	281.0
68.00	9858.0
69.00	10707.0
70.00	777.0
72.00	578.0
73.10	4804.0
74.00	17696.0
75.00	51664.0
76.10	4735.0
77.00	572.0
77.90	455.0
78.90	4493.0
79.90	1125.0
80.90	4819.0
81.90	731.0
82.90	111.0
85.80	267.0
87.00	5092.0
88.00	4665.0
91.10	421.0
92.00	2907.0
93.00	4609.0
94.00	12423.0
95.00	103592.0
96.00	7048.0
97.10	273.0
103.80	582.0
104.90	125.0
105.80	459.0
107.00	116.0
109.80	126.0
112.80	113.0
115.70	336.0
116.80	1023.0
117.80	377.0
118.90	648.0
127.90	405.0
128.90	233.0
130.00	374.0
130.70	152.0
131.00	123.0
135.00	172.0
137.00	164.0
140.90	1113.0
141.80	138.0
143.00	2074.0
144.10	124.0
144.90	839.0
145.90	274.0
148.00	259.0
149.80	139.0
151.80	122.0
155.00	289.0
155.90	101.0
156.90	170.0
160.90	183.0
170.90	266.0
172.10	1158.0
172.90	997.0
174.00	88752.0
175.00	6599.0
176.00	83928.0
177.00	5443.0
177.90	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB329

m/z	Abundance
35.90	754.0
37.00	3988.0
38.00	3643.0
39.00	1861.0
39.90	923.0
43.10	104.0
43.90	743.0
45.00	694.0
46.10	128.0
47.00	1253.0
47.90	745.0
49.00	3443.0
50.00	17456.0
51.00	5634.0
52.00	277.0
53.00	187.0
53.90	172.0
54.90	385.0
56.00	1465.0
57.00	2449.0
58.00	112.0
60.00	1026.0
61.00	4925.0
62.00	4677.0
63.00	4598.0
64.00	998.0
65.00	1031.0
66.00	213.0
66.80	238.0
68.00	10072.0
69.00	10770.0
70.00	764.0
72.00	618.0
73.10	4841.0
74.00	17872.0
75.00	51808.0
76.10	4615.0
76.90	684.0
77.90	434.0
78.90	4453.0
79.90	1100.0
80.90	4907.0
82.00	857.0
82.80	108.0
85.80	264.0
87.00	5090.0
88.00	4573.0
91.00	433.0
92.00	3039.0
93.00	4648.0
94.00	12816.0
95.00	104848.0
96.00	6983.0
97.10	240.0
103.80	645.0
104.90	121.0
105.80	470.0
107.00	125.0
108.00	125.0
109.90	111.0
110.90	115.0
115.80	372.0
116.90	1106.0
117.90	377.0
118.90	670.0
127.90	453.0
129.00	296.0
129.90	379.0
131.00	132.0
134.90	161.0
136.90	168.0
140.90	1143.0
141.80	146.0
143.00	2236.0
144.10	115.0
145.00	813.0
145.90	270.0
147.90	238.0
149.80	120.0
151.80	103.0
155.00	296.0
156.90	223.0
158.90	115.0
160.90	146.0
170.90	255.0
172.10	1218.0
172.90	1070.0
174.00	91024.0
175.00	6651.0
176.00	86912.0
177.00	5776.0
177.90	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB329

m/z	Abundance
35.90	754.0
37.00	3988.0
38.00	3643.0
39.00	1861.0
39.90	923.0
43.10	104.0
43.90	743.0
45.00	694.0
46.10	128.0
47.00	1253.0
47.90	745.0
49.00	3443.0
50.00	17456.0
51.00	5634.0
52.00	277.0
53.00	187.0
53.90	172.0
54.90	385.0
56.00	1465.0
57.00	2449.0
58.00	112.0
60.00	1026.0
61.00	4925.0
62.00	4677.0
63.00	4598.0
64.00	998.0
65.00	1031.0
66.00	213.0
66.80	238.0
68.00	10072.0
69.00	10770.0
70.00	764.0
72.00	618.0
73.10	4841.0
74.00	17872.0
75.00	51808.0
76.10	4615.0
76.90	684.0
77.90	434.0
78.90	4453.0
79.90	1100.0
80.90	4907.0
82.00	857.0
82.80	108.0
85.80	264.0
87.00	5090.0
88.00	4573.0
91.00	433.0
92.00	3039.0
93.00	4648.0
94.00	12816.0
95.00	104848.0
96.00	6983.0
97.10	240.0
103.80	645.0
104.90	121.0
105.80	470.0
107.00	125.0
108.00	125.0
109.90	111.0
110.90	115.0
115.80	372.0
116.90	1106.0
117.90	377.0
118.90	670.0
127.90	453.0
129.00	296.0
129.90	379.0
131.00	132.0
134.90	161.0
136.90	168.0
140.90	1143.0
141.80	146.0
143.00	2236.0
144.10	115.0
145.00	813.0
145.90	270.0
147.90	238.0
149.80	120.0
151.80	103.0
155.00	296.0
156.90	223.0
158.90	115.0
160.90	146.0
170.90	255.0
172.10	1218.0
172.90	1070.0
174.00	91024.0
175.00	6651.0
176.00	86912.0
177.00	5776.0
177.90	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB329

m/z	Abundance
36.00	680.0
37.00	3407.0
38.00	3320.0
39.00	1747.0
39.90	898.0
44.00	772.0
45.00	601.0
46.90	1086.0
47.90	614.0
49.00	3034.0
50.00	15789.0
51.00	5220.0
52.00	271.0
53.00	214.0
53.90	149.0
54.90	321.0
56.00	1398.0
57.00	2119.0
60.00	964.0
61.00	4538.0
62.00	4215.0
63.00	4133.0
63.90	926.0
65.00	911.0
66.00	149.0
67.10	229.0
68.00	9033.0
69.00	9712.0
70.00	733.0
72.00	554.0
73.00	4376.0
74.00	16480.0
75.00	46736.0
76.10	4088.0
76.90	730.0
77.90	392.0
78.90	3981.0
79.90	979.0
80.90	4385.0
82.00	883.0
82.70	127.0
85.80	218.0
87.00	4704.0
88.00	4072.0
91.00	380.0
92.00	2757.0
93.00	4239.0
94.00	11782.0
95.00	95472.0
96.00	6233.0
97.10	149.0
103.80	610.0
104.90	116.0
105.80	470.0
106.90	125.0
108.00	174.0
110.90	118.0
115.00	101.0
115.80	328.0
116.90	1089.0
117.90	417.0
118.90	656.0
127.90	422.0
129.00	319.0
129.90	367.0
131.00	147.0
134.90	154.0
136.80	183.0
140.90	1008.0
141.90	141.0
143.00	2046.0
145.00	746.0
145.80	205.0
147.80	217.0
155.00	252.0
156.90	234.0
158.90	143.0
160.80	101.0
170.90	239.0
172.00	1129.0
172.90	1004.0
174.00	84752.0
175.00	5935.0
176.00	81936.0
177.00	5417.0
177.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB329