

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061618\
 Data File : VV006330.D
 Acq On : 16 Jun 2018 19:31
 Operator : SY/MD
 Sample : J3549-20
 Misc : 25 mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWG2

Quant Time: Jun 18 01:19:19 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 18 01:15:51 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	306150	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	274408	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	121449	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	69384	4.15	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.00%
7) Chloroethane-d5	1.58	69	60323	4.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.20%
11) 1,1-Dichloroethene-d2	2.13	63	97820	3.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.20%
20) 2-Butanone-d5	3.96	46	202478	57.03	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.06%
24) Chloroform-d	4.41	84	152535	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
26) 1,2-Dichloroethane-d4	5.09	65	73445	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.80%
32) Benzene-d6	5.11	84	293472	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.00%
36) 1,2-Dichloropropane-d6	6.12	67	92687	4.68	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.60%
41) Toluene-d8	7.37	98	262634	4.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.60%
43) trans-1,3-Dichloropropene-	7.67	79	29523	3.33	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	66.60%
46) 2-Hexanone-d5	8.14	63	152127	39.72	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.44%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	59619	4.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	104467	4.96	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.20%

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	2.21	43	15314	7.960	ug/L	93
15) Methyl Acetate	2.38	43	4315	0.754	ug/L #	48
21) 2-Butanone	4.04	43	54078	15.451	ug/L	93
25) Chloroform	4.44	83	283076	8.502	ug/L	97
35) Methylcyclohexane	6.12	83	22843	0.644	ug/L #	20
37) 1,2-Dichloropropane	6.12	63	9773	0.539	ug/L #	85
38) Bromodichloromethane	6.56	83	42806	1.773	ug/L	98
40) 4-Methyl-2-pentanone	7.29	43	2621	0.280	ug/L #	80
42) Toluene	7.44	91	28225	0.338	ug/L	99
48) 2-Hexanone	8.19	43	24873	3.775	ug/L #	86
49) Dibromochloromethane	8.30	129	6786	0.420	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061618\
Data File : VV006330.D
Acq On : 16 Jun 2018 19:31
Operator : SY/MD
Sample : J3549-20
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWG2

Quant Time: Jun 18 01:19:19 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 18 01:15:51 2018
Response via : Initial Calibration

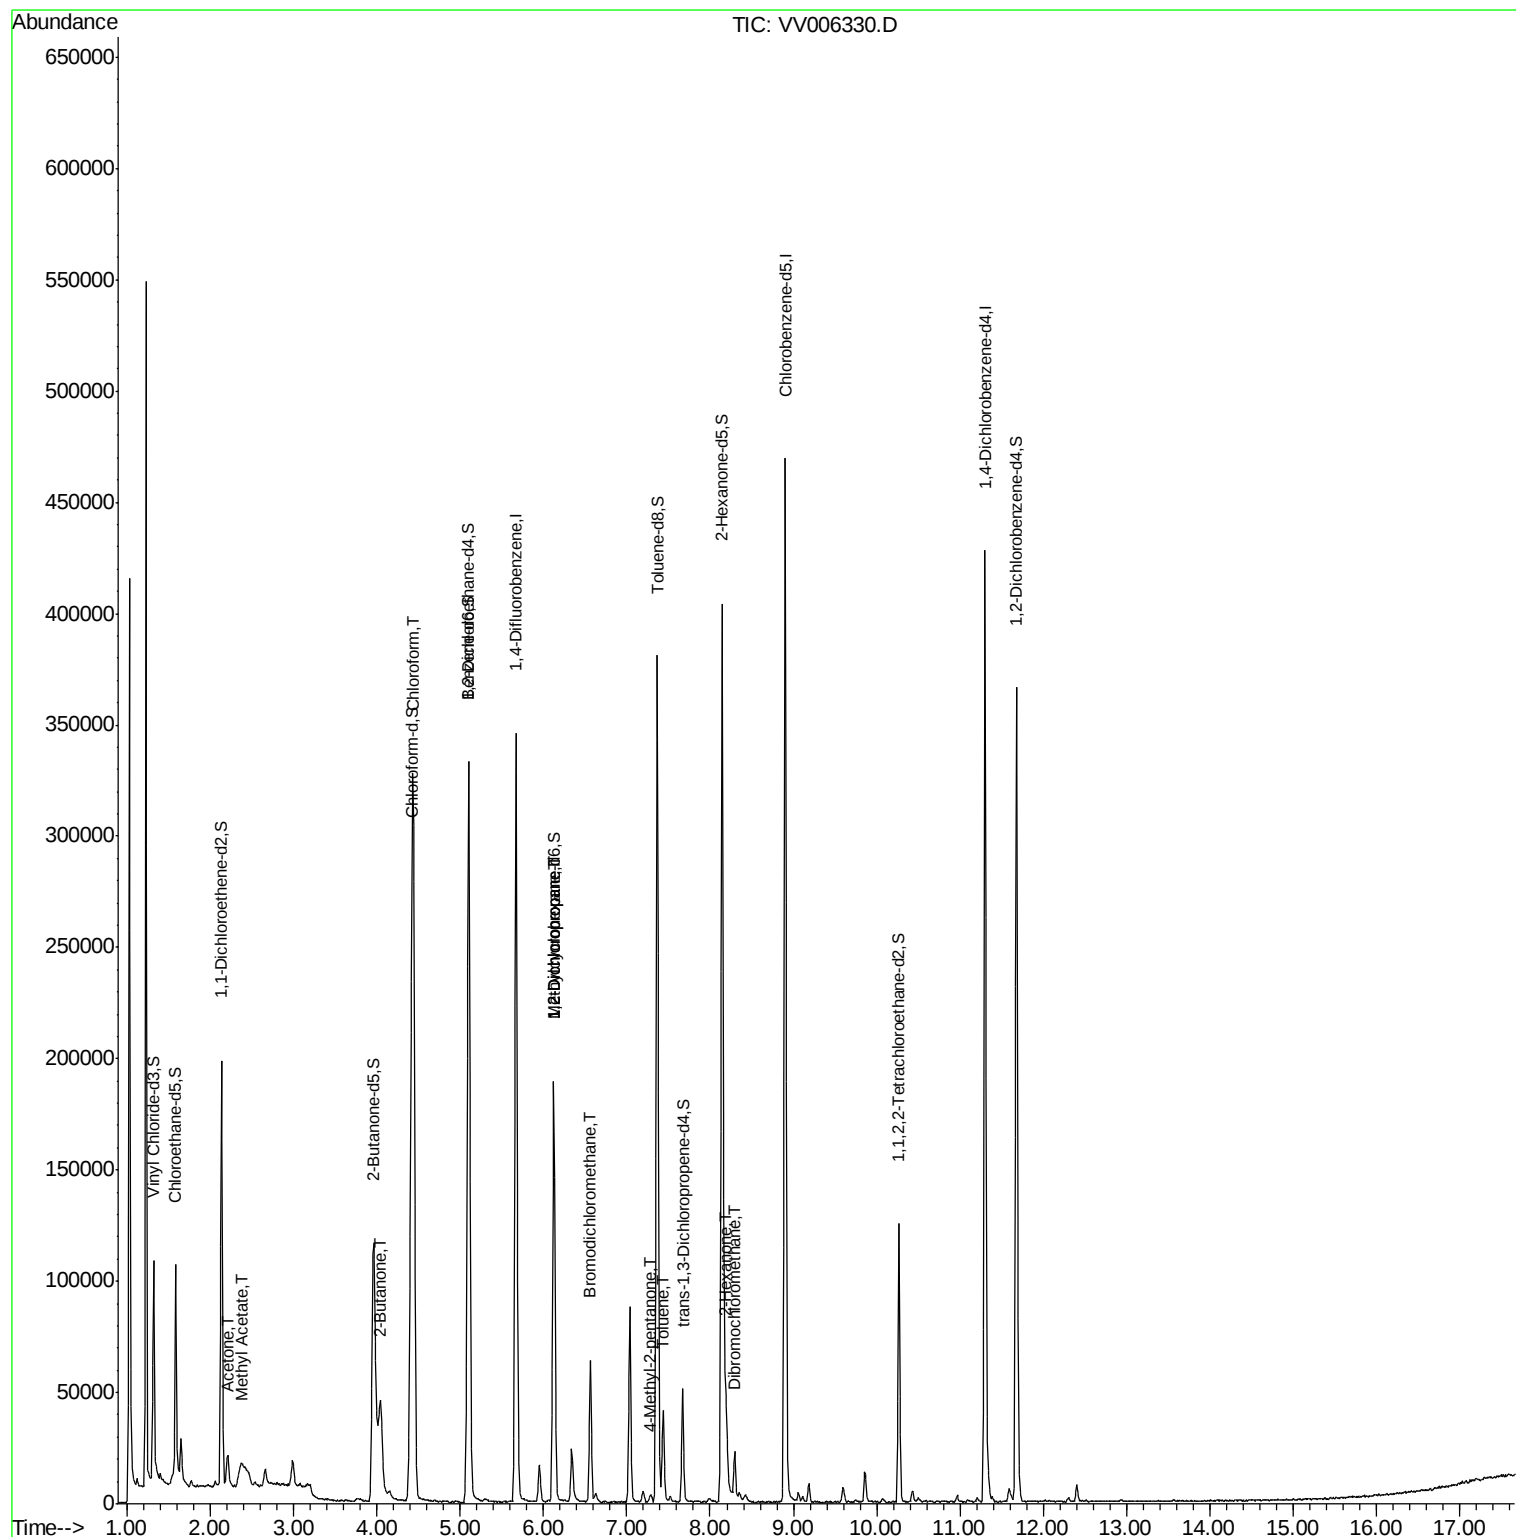

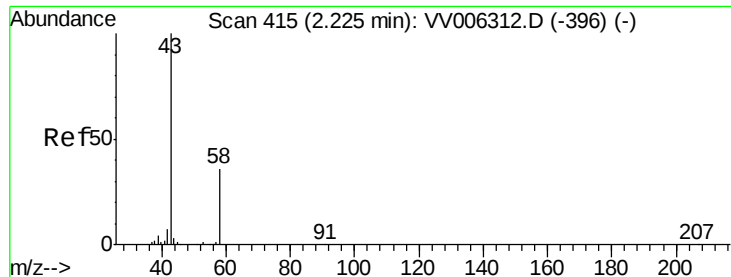

#13

Acetone

Concen: 7.960 ug/L

RT: 2.21 min Scan# 410

Delta R.T. -0.02 min

Lab File: VV006330.D

Acq: 16 Jun 2018 19:31

Instrument :

MSVOA_V

ClientSampleId :





ESWG2

Tgt Ion: 43 Resp: 15314

Ion Ratio Lower Upper

43 100

58 37.8 0.0 67.4

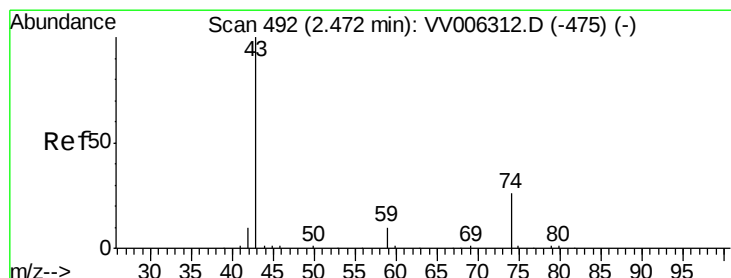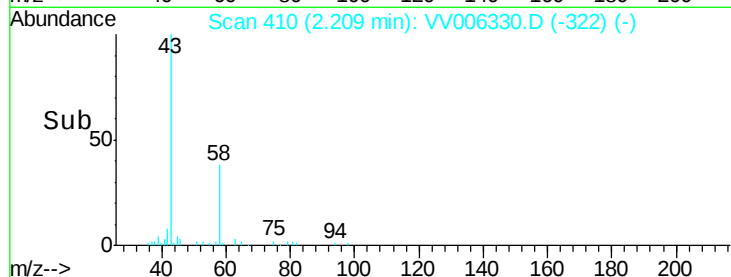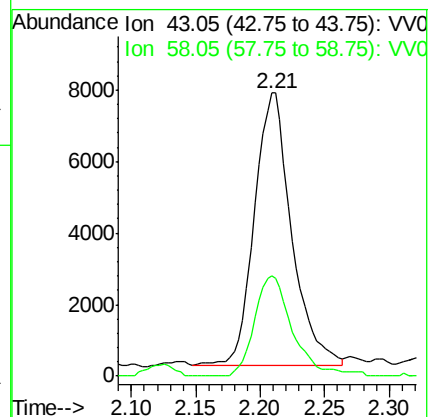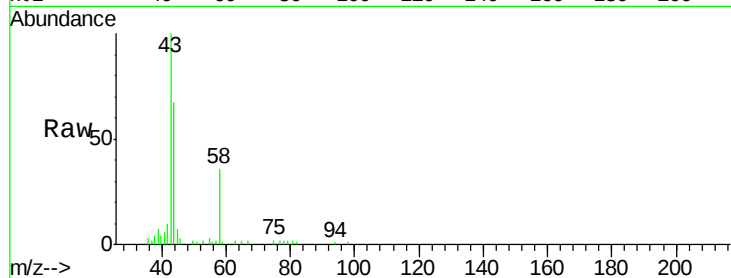

#15

Methyl Acetate

Concen: 0.754 ug/L

RT: 2.38 min Scan# 462

Delta R.T. -0.10 min

Lab File: VV006330.D




Acq: 16 Jun 2018 19:31


Tgt Ion: 43 Resp: 4315

Ion Ratio Lower Upper

43 100

74 1.6 23.4 35.0#

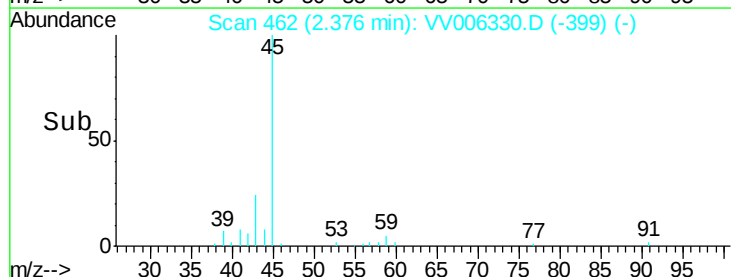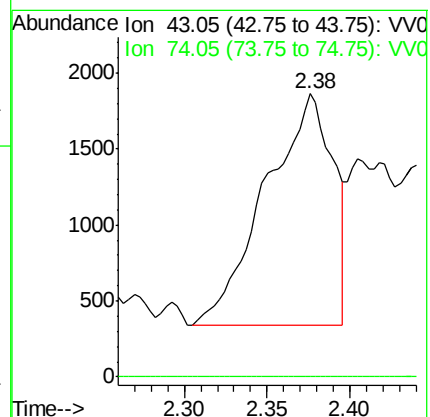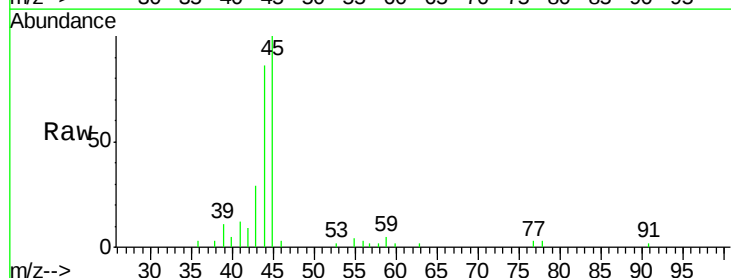

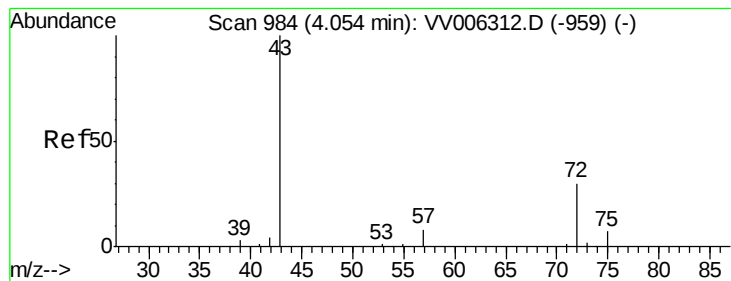

#21

2-Butanone

Concen: 15.451 ug/L

RT: 4.04 min Scan# 981

Delta R.T. -0.01 min

Lab File: VV006330.D

Acq: 16 Jun 2018 19:31

Instrument :

MSVOA_V

ClientSampled :


ESWG2

Tgt Ion: 43 Resp: 54078




Ion Ratio Lower Upper

43 100

72 31.0 13.8 41.3

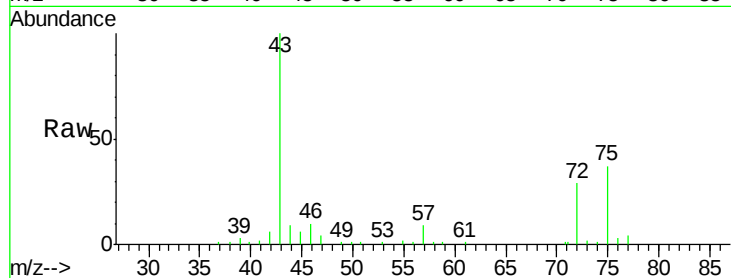

Abundance Ion 43.05 (42.75 to 43.75): VV006330.D (-891) (-)

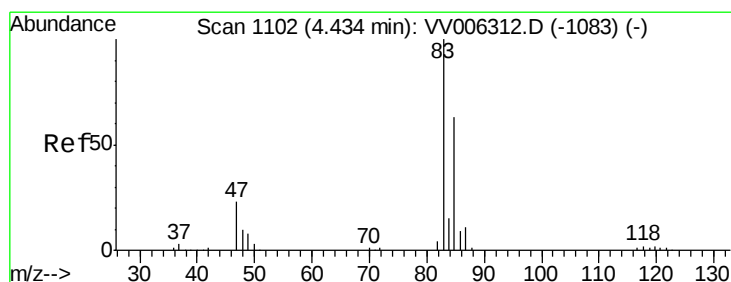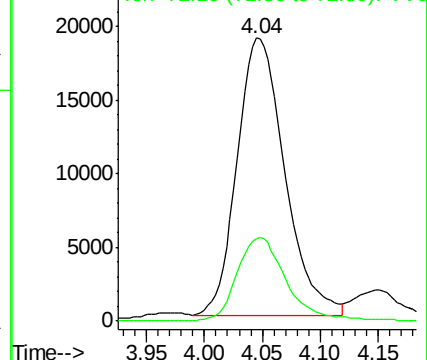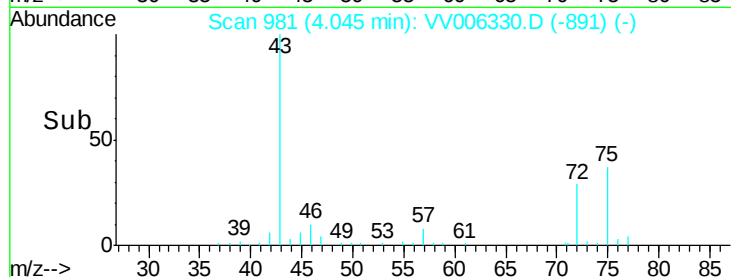

#25

Chloroform

Concen: 8.502 ug/L

RT: 4.44 min Scan# 1103

Delta R.T. 0.00 min

Lab File: VV006330.D


Acq: 16 Jun 2018 19:31

Tgt Ion: 83 Resp: 283076



Ion Ratio Lower Upper


83 100

85 63.9 46.2 85.8

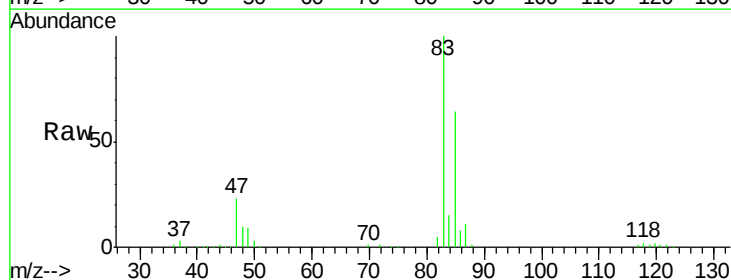

Abundance Ion 83.05 (82.75 to 83.75): VV006330.D (-1009) (-)



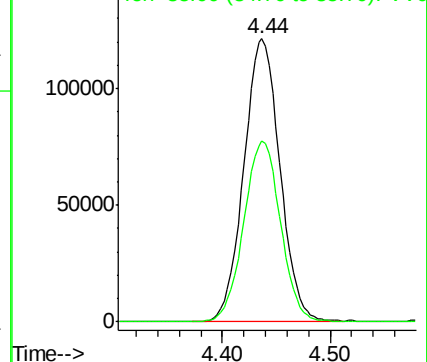
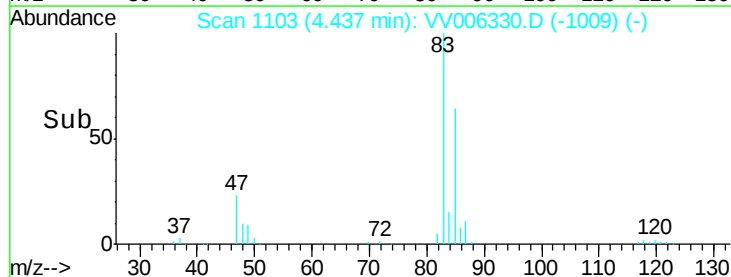


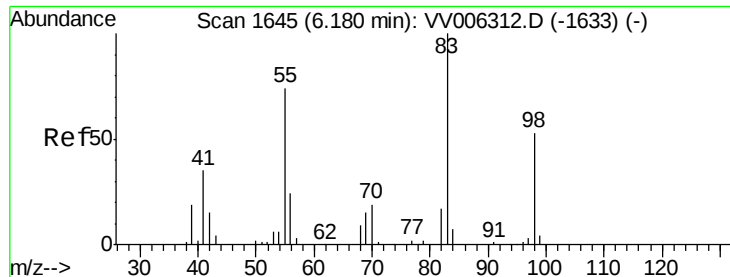

#35
Methylcyclohexane
Concen: 0.644 ug/L
RT: 6.12 min Scan# 1628
Delta R.T. -0.05 min
Lab File: VV006330.D
Acq: 16 Jun 2018 19:31




Instrument :
MSVOA_V
ClientSampleId :
ESWG2


Tgt Ion: 83 Resp: 22843
Ion Ratio Lower Upper
83 100
55 0.3 57.5 86.3#
98 1.1 39.8 59.8#

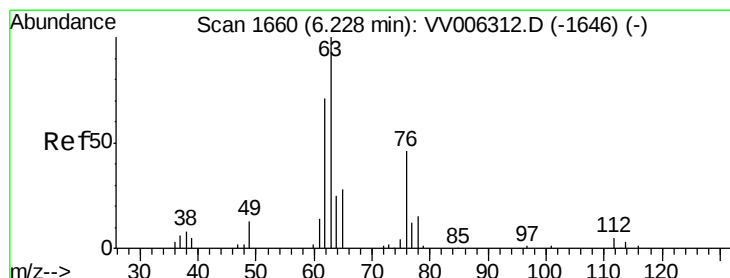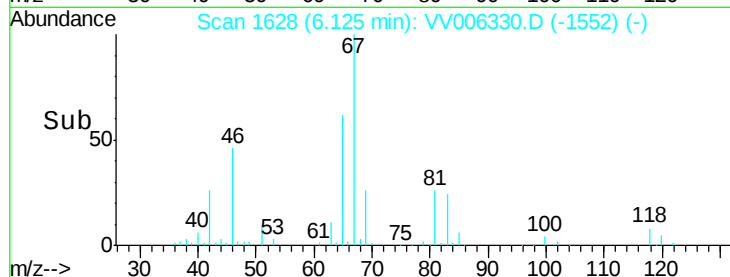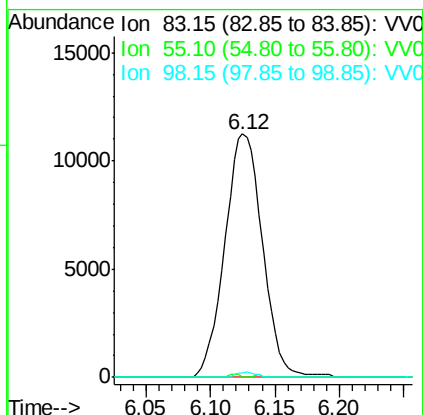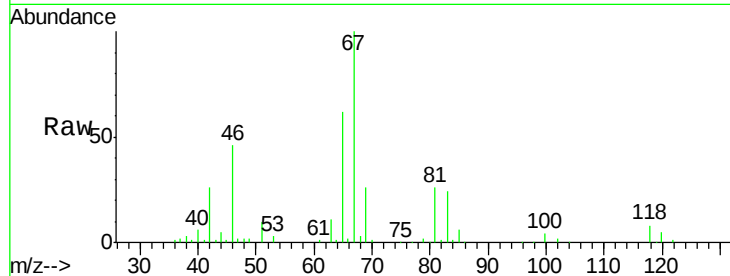

#37
1,2-Dichloropropane
Concen: 0.539 ug/L
RT: 6.12 min Scan# 1628
Delta R.T. -0.10 min
Lab File: VV006330.D
Acq: 16 Jun 2018 19:31

Tgt Ion: 63 Resp: 9773
Ion Ratio Lower Upper
63 100
112 0.0 4.1 6.1#


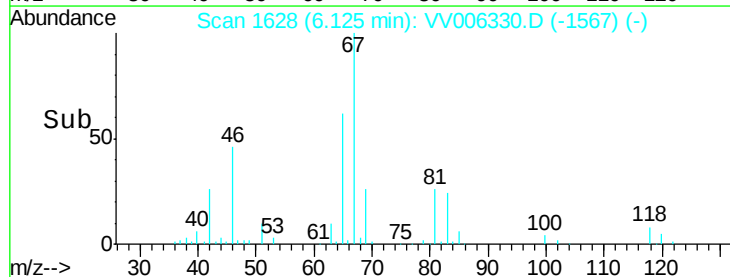
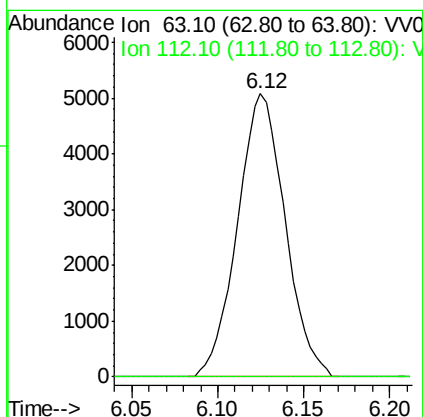
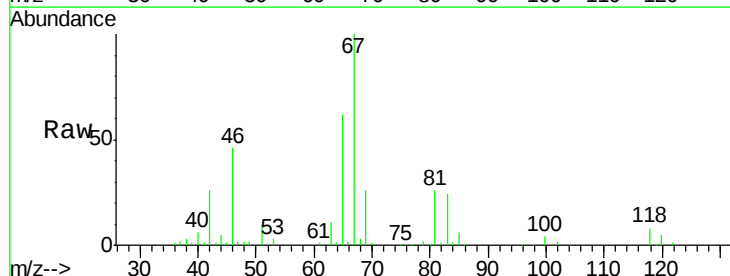


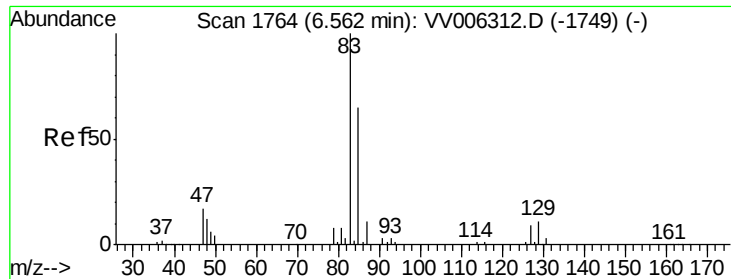

#38
 Bromodichloromethane
 Concen: 1.773 ug/L
 RT: 6.56 min Scan# 1764
 Delta R.T. 0.00 min
 Lab File: VV006330.D
 Acq: 16 Jun 2018 19:31




Instrument :
 MSVOA_V
 ClientSampleId :
 ESGW2


Tgt Ion: 83 Resp: 42806
 Ion Ratio Lower Upper
 83 100
 85 65.8 44.9 83.5
 127 9.8 7.0 10.4

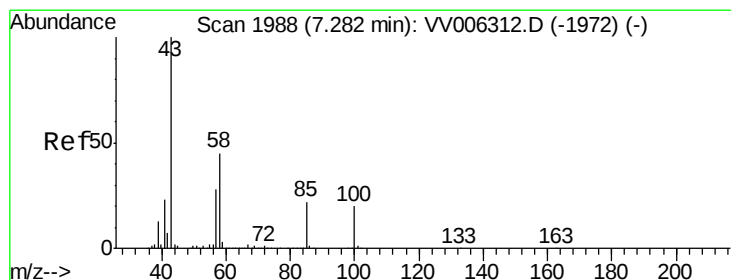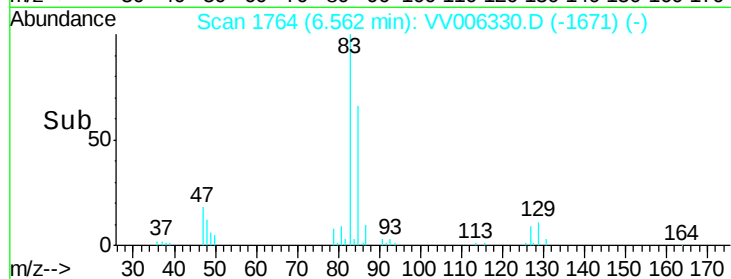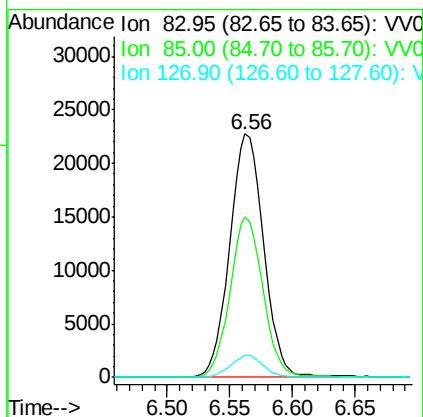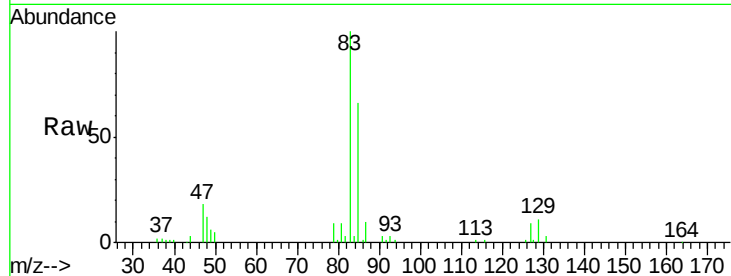

#40
 4-Methyl-2-pentanone
 Concen: 0.280 ug/L
 RT: 7.29 min Scan# 1989
 Delta R.T. 0.00 min
 Lab File: VV006330.D
 Acq: 16 Jun 2018 19:31

Tgt Ion: 43 Resp: 2621
 Ion Ratio Lower Upper
 43 100
 58 38.1 36.0 54.0
 100 0.0 15.4 23.2#

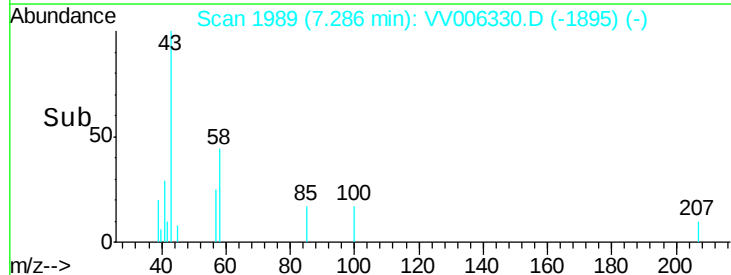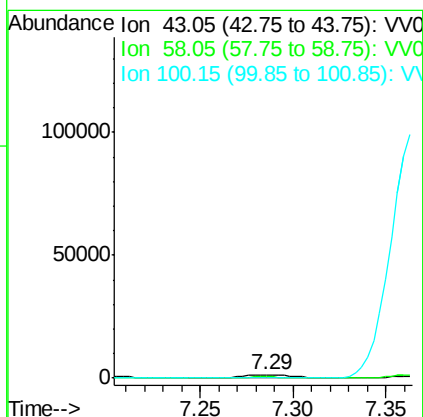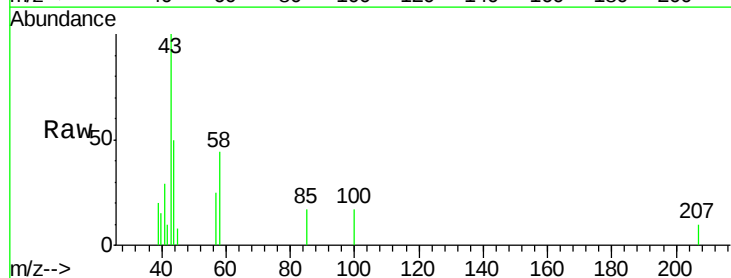

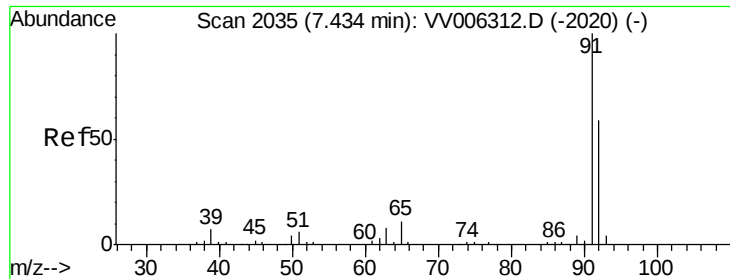

#42

Toluene

Concen: 0.338 ug/L

RT: 7.44 min Scan# 2036

Delta R.T. 0.00 min

Lab File: VV006330.D

Acq: 16 Jun 2018 19:31

Instrument :

MSVOA_V

ClientSampleId :


ESWG2

Tgt Ion: 91 Resp: 28225

Ion Ratio Lower Upper


91 100

92 57.6 41.1 76.3


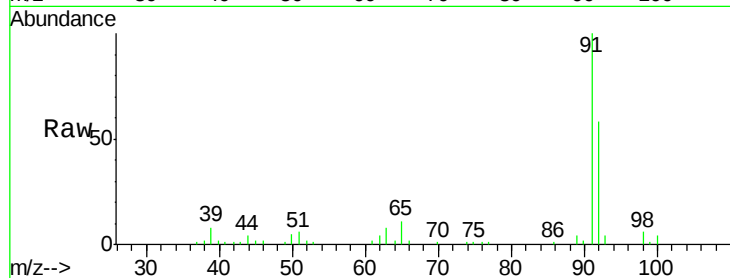


Abundance Ion 91.15 (90.85 to 91.85): VV006330.D (-2178) (-)

Ion 92.15 (91.85 to 92.85): VV006330.D (-2178) (-)

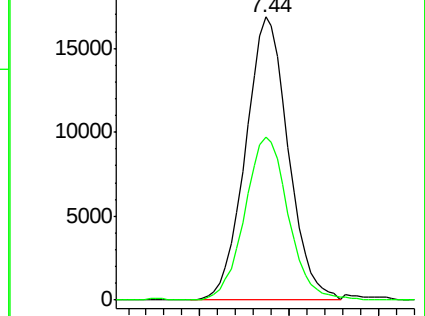

Time-->

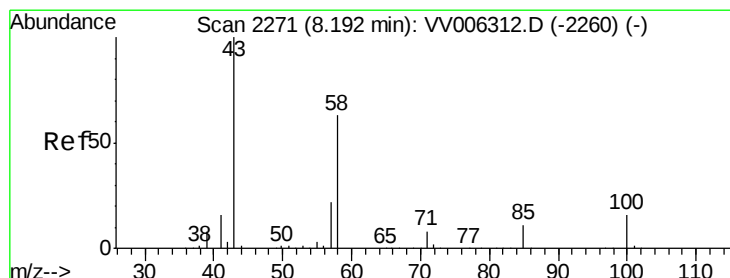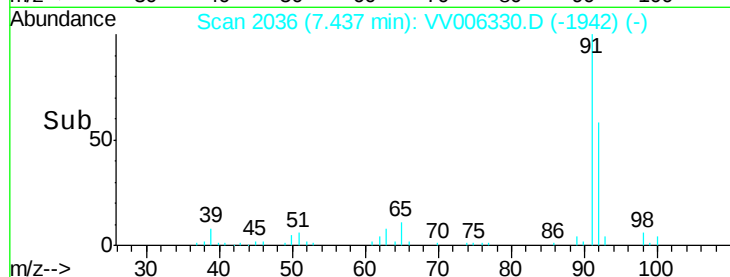

#48

2-Hexanone

Concen: 3.775 ug/L

RT: 8.19 min Scan# 2271

Delta R.T. 0.00 min

Lab File: VV006330.D

Acq: 16 Jun 2018 19:31

Tgt Ion: 43 Resp: 24873


Ion Ratio Lower Upper

43 100

58 49.6 48.6 72.8

57 16.8 17.5 26.3#

100 9.5 12.6 18.8#

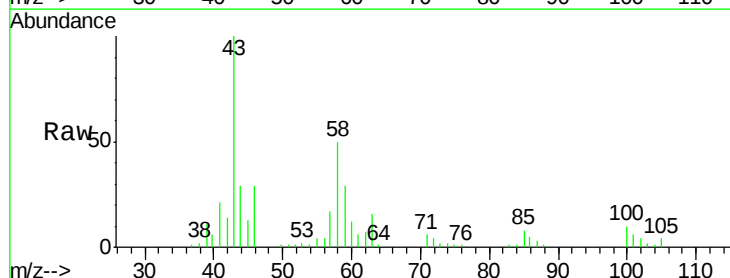


Abundance Ion 43.05 (42.75 to 43.75): VV006330.D (-2178) (-)


Ion 58.05 (57.75 to 58.75): VV006330.D (-2178) (-)


Ion 57.20 (56.90 to 57.90): VV006330.D (-2178) (-)

Ion 100.15 (99.85 to 100.85): VV006330.D (-2178) (-)

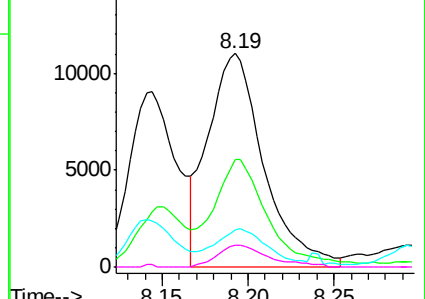

Time-->

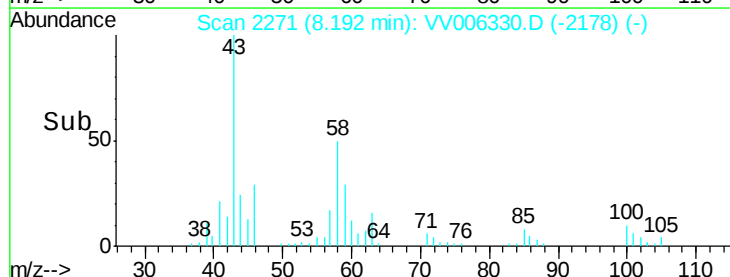

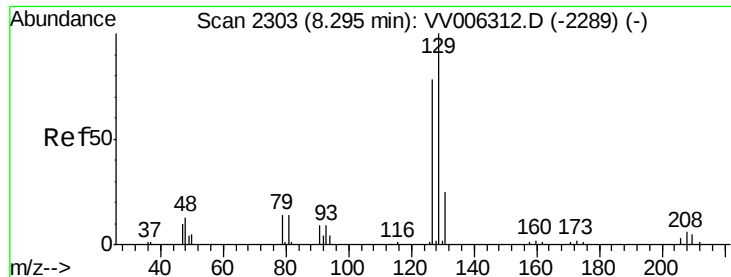

#49

Dibromochloromethane

Concen: 0.420 ug/L

RT: 8.30 min Scan# 2304

Delta R.T. 0.00 min

Lab File: VV006330.D

Acq: 16 Jun 2018 19:31

Instrument :

MSVOA_V

ClientSampleId :


ESWG2

Tgt Ion:129 Resp: 6786

Ion Ratio Lower Upper

129 100

127 80.7 55.2 102.4

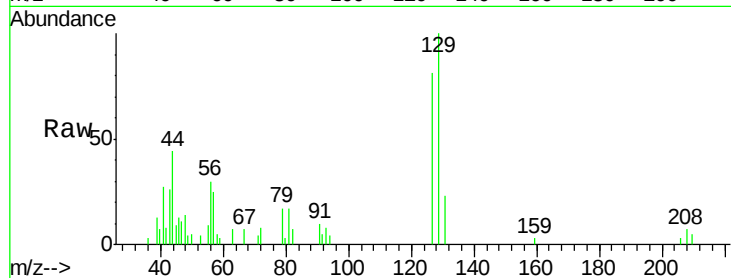

Abundance Ion 128.95 (128.65 to 129.65): V

Ion 126.90 (126.60 to 127.60): V

