

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061618\
 Data File : VV006314.D
 Acq On : 16 Jun 2018 12:18
 Operator : SY/MD
 Sample : J3549-01
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWD6

Quant Time: Jun 18 01:29:58 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 18 01:15:51 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	354658	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	320499	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	144510	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	72698	3.75	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.00%
7) Chloroethane-d5	1.58	69	61607	3.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.40%
11) 1,1-Dichloroethene-d2	2.13	63	101456	2.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	53.80%#
20) 2-Butanone-d5	3.95	46	189328	46.03	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.06%
24) Chloroform-d	4.41	84	139388	3.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	74.40%
26) 1,2-Dichloroethane-d4	5.09	65	71235	3.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.60%
32) Benzene-d6	5.10	84	291642	3.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.80%
36) 1,2-Dichloropropane-d6	6.12	67	90283	3.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	78.00%
41) Toluene-d8	7.36	98	267129	3.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.80%
43) trans-1,3-Dichloropropene-	7.67	79	29434	2.84	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	56.80%
46) 2-Hexanone-d5	8.14	63	152861	34.17	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	68.34%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	60327	3.60	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	72.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	102711	4.10	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	82.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	13631	6.116 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061618\
Data File : VV006314.D
Acq On : 16 Jun 2018 12:18
Operator : SY/MD
Sample : J3549-01
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWD6

Quant Time: Jun 18 01:29:58 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 18 01:15:51 2018
Response via : Initial Calibration

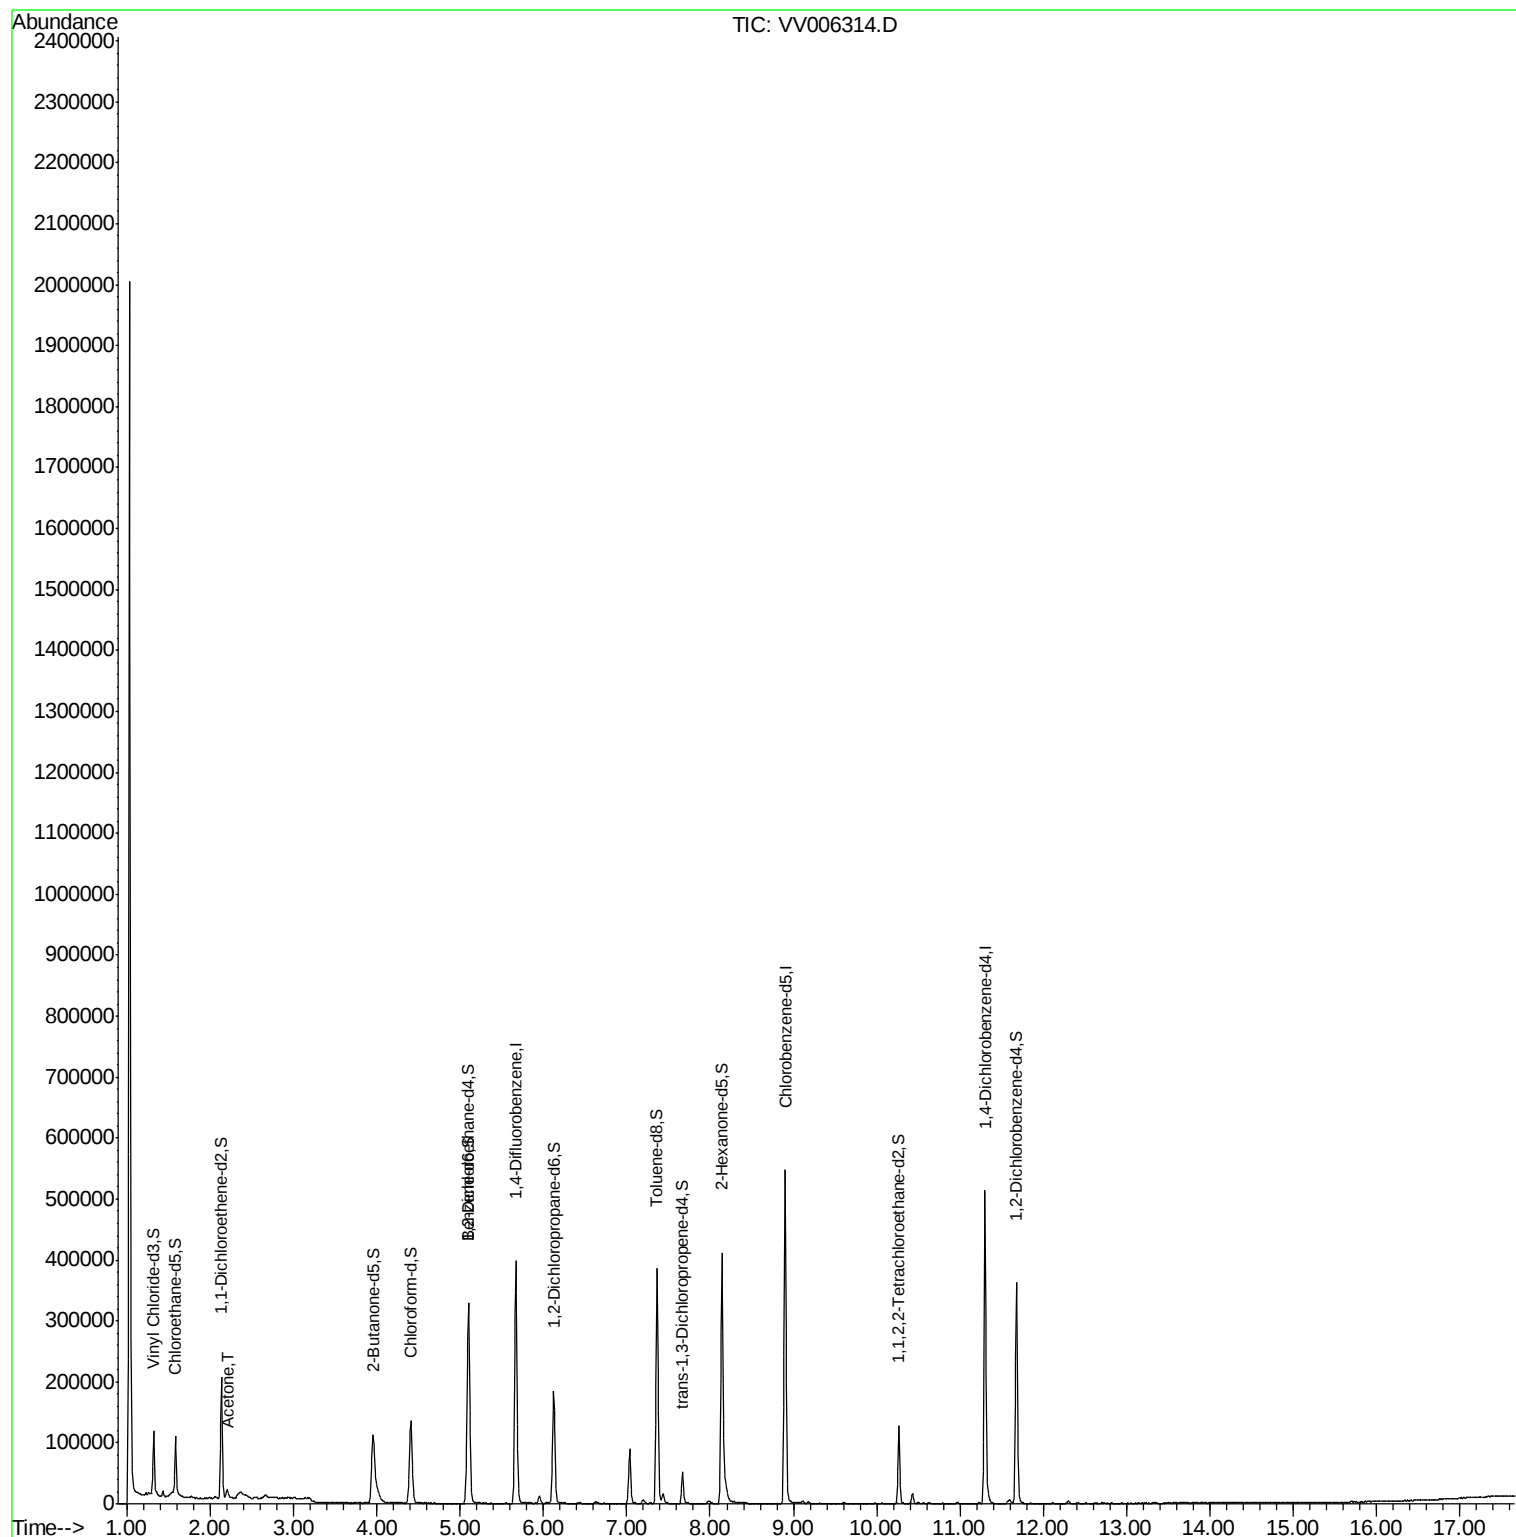

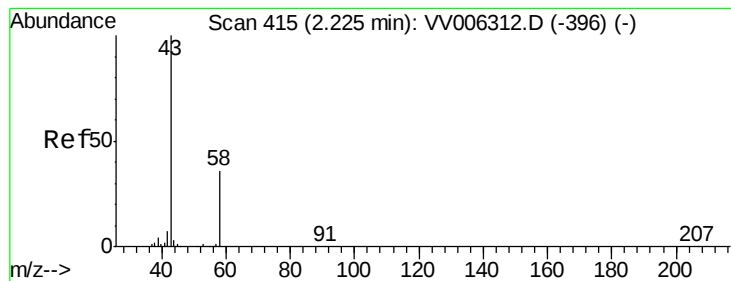

#13

Acetone

Concen: 6.116 ug/L

RT: 2.21 min Scan# 409

Delta R.T. -0.02 min

Lab File: VV006314.D

Acq: 16 Jun 2018 12:18

Instrument :
MSVOA_V
ClientSampleId :
ESWD6

Tot Ion: 43 Resp: 13631

Ion Ratio Lower Upper

43 100

58 37.7 0.0 67.4

