

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061618\
 Data File : VV006315.D
 Acq On : 16 Jun 2018 12:45
 Operator : SY/MD
 Sample : J3549-02
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWD7

Quant Time: Jun 18 01:31:16 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 18 01:15:51 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	319338	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	286322	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	130913	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	69795	4.00	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.00%
7) Chloroethane-d5	1.58	69	60547	4.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.80%
11) 1,1-Dichloroethene-d2	2.13	63	97069	2.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.20%#
20) 2-Butanone-d5	3.95	46	188199	50.82	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.64%
24) Chloroform-d	4.41	84	135767	4.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.40%
26) 1,2-Dichloroethane-d4	5.09	65	69722	4.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.40%
32) Benzene-d6	5.11	84	279608	4.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.20%
36) 1,2-Dichloropropane-d6	6.12	67	86977	4.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.00%
41) Toluene-d8	7.37	98	254606	3.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.60%
43) trans-1,3-Dichloropropene-	7.67	79	29018	3.13	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	62.60%
46) 2-Hexanone-d5	8.14	63	152032	38.04	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.08%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	60434	4.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	100589	4.43	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.60%


Target Compounds					Ovalue
13) Acetone	2.20	43	13230	6.593 ug/L	93
34) Trichloroethene	5.96	95	123352	5.725 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061618\
Data File : VV006315.D
Acq On : 16 Jun 2018 12:45
Operator : SY/MD
Sample : J3549-02
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWD7

Quant Time: Jun 18 01:31:16 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 18 01:15:51 2018
Response via : Initial Calibration

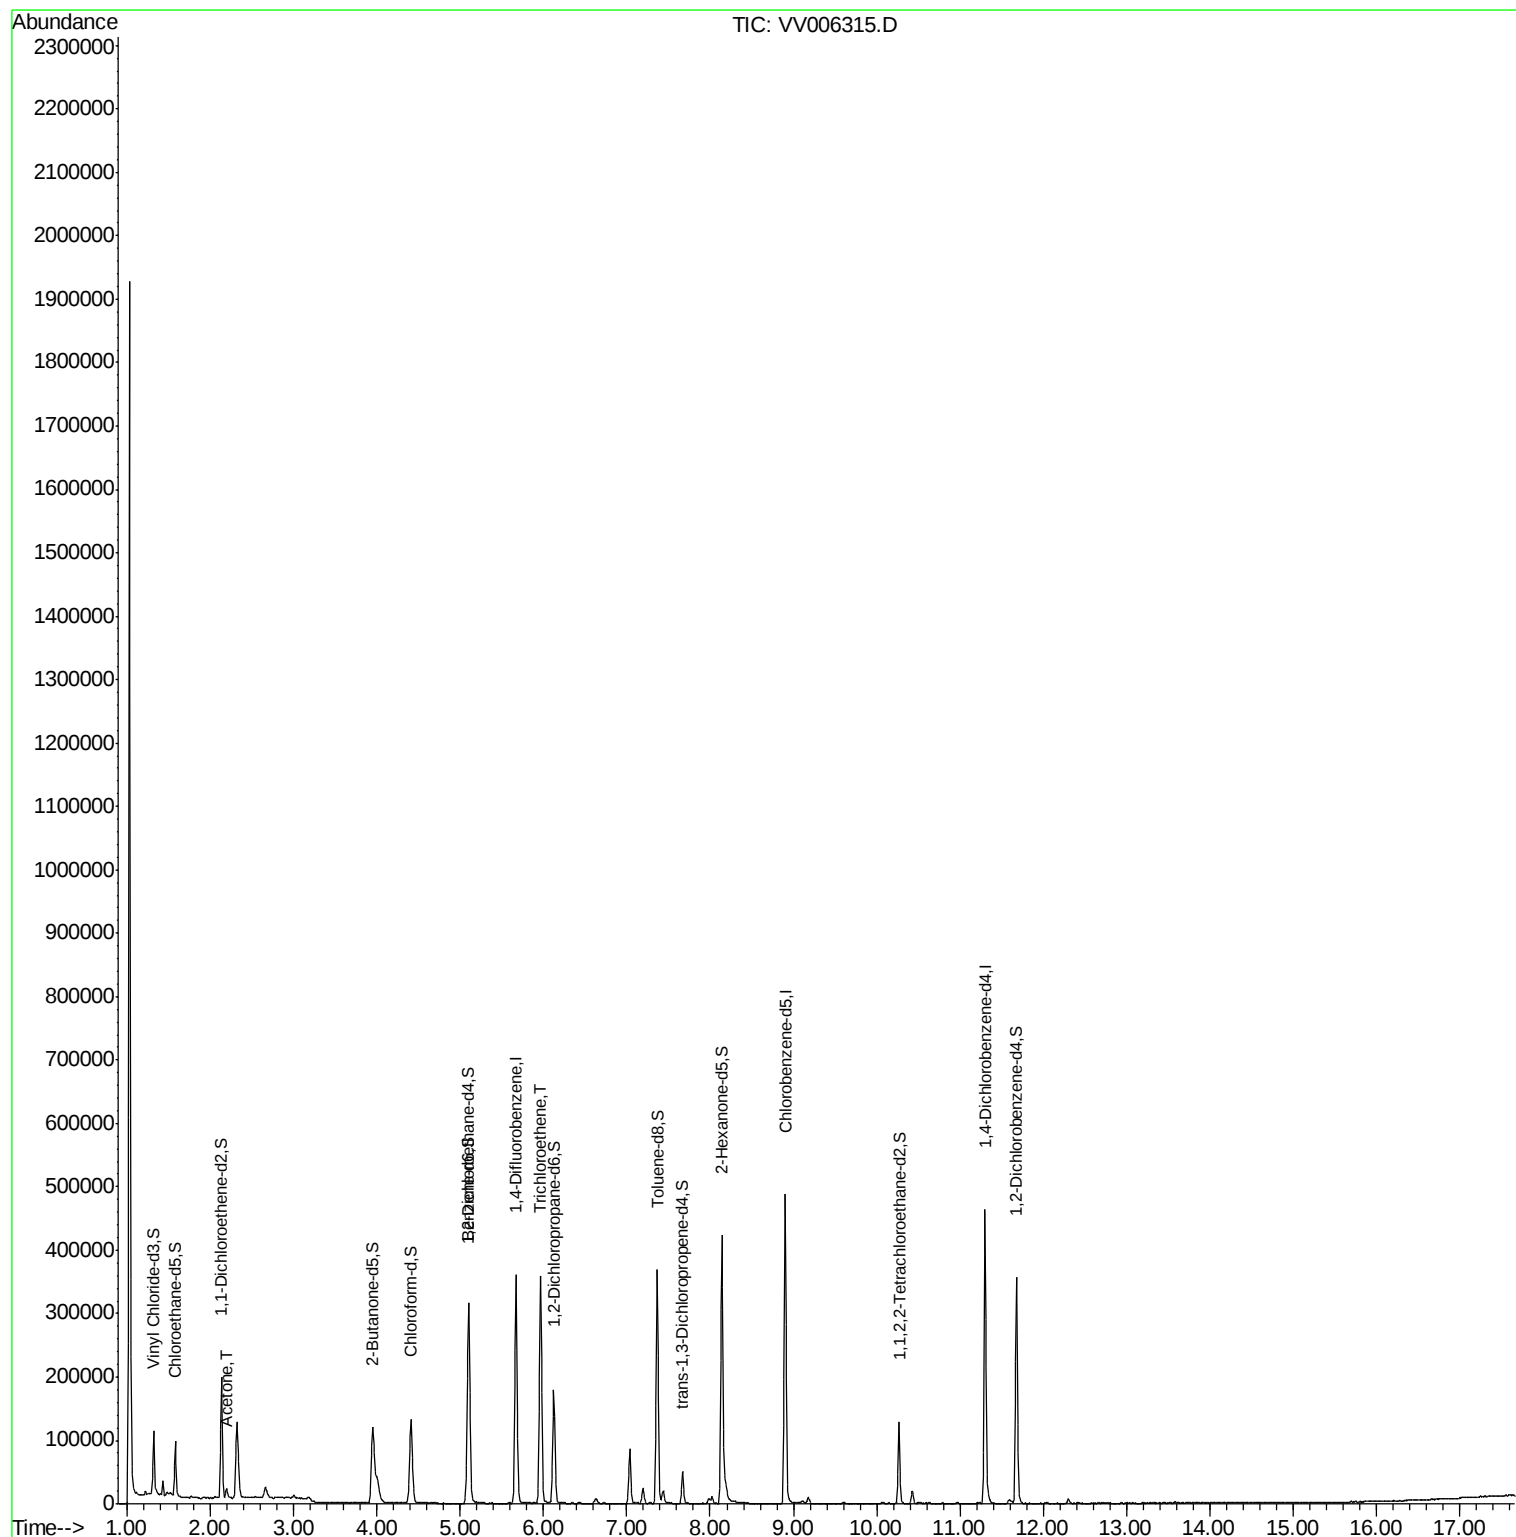

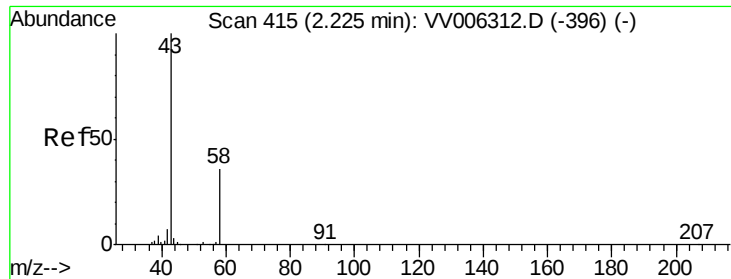

#13

Acetone

Concen: 6.593 ug/L

RT: 2.20 min Scan# 406

Delta R.T. -0.03 min

Lab File: VV006315.D

Acq: 16 Jun 2018 12:45





Instrument :
MSVOA_V
ClientSampleId :
ESWD7

Tot Ion: 43 Resp: 13230

Ion Ratio Lower Upper

43 100

58 37.5 0.0 67.4

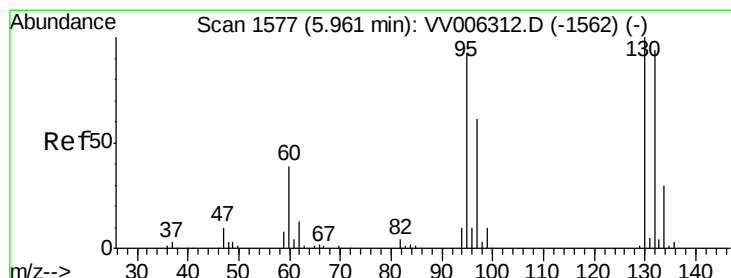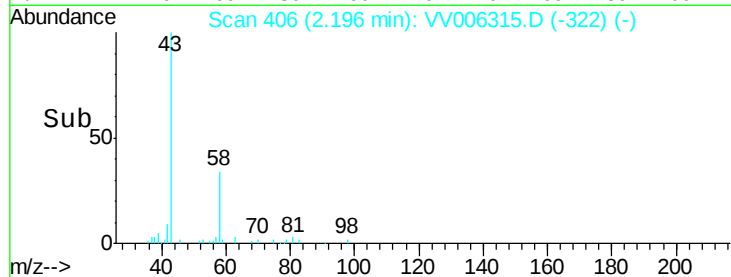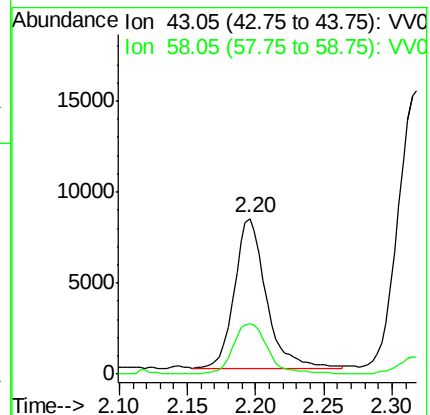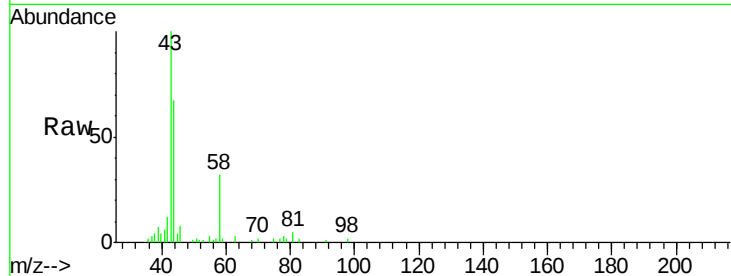

#34

Trichloroethene

Concen: 5.725 ug/L

RT: 5.96 min Scan# 1578

Delta R.T. 0.00 min

Lab File: VV006315.D

Acq: 16 Jun 2018 12:45

Tgt Ion: 95 Resp: 123352

Ion Ratio Lower Upper

95 100

97 64.4 45.1 83.9

132 101.4 69.0 128.1

130 105.4 72.8 135.2

