

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061618\
 Data File : VV006317.D
 Acq On : 16 Jun 2018 13:39
 Operator : SY/MD
 Sample : J3549-11
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWE6

Quant Time: Jun 18 01:34:37 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 18 01:15:51 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	335152	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	299364	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	135297	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	98202	5.37	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.40%
7) Chloroethane-d5	1.58	69	76547	5.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.40%
11) 1,1-Dichloroethene-d2	2.13	63	134912	3.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.80%
20) 2-Butanone-d5	3.95	46	180531	46.45	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.90%
24) Chloroform-d	4.41	84	154910	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.40%
26) 1,2-Dichloroethane-d4	5.09	65	78204	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
32) Benzene-d6	5.11	84	343888	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
36) 1,2-Dichloropropane-d6	6.12	67	99443	4.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.00%
41) Toluene-d8	7.37	98	322293	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.00%
43) trans-1,3-Dichloropropene-	7.67	79	33141	3.42	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.40%
46) 2-Hexanone-d5	8.14	63	148026	35.43	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	70.86%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	61752	3.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	78.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	113707	4.85	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.00%


Target Compounds					Ovalue
13) Acetone	2.20	43	29631	14.069 ug/L	92
42) Toluene	7.44	91	62905	0.690 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061618\
Data File : VV006317.D
Acq On : 16 Jun 2018 13:39
Operator : SY/MD
Sample : J3549-11
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWE6

Quant Time: Jun 18 01:34:37 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 18 01:15:51 2018
Response via : Initial Calibration

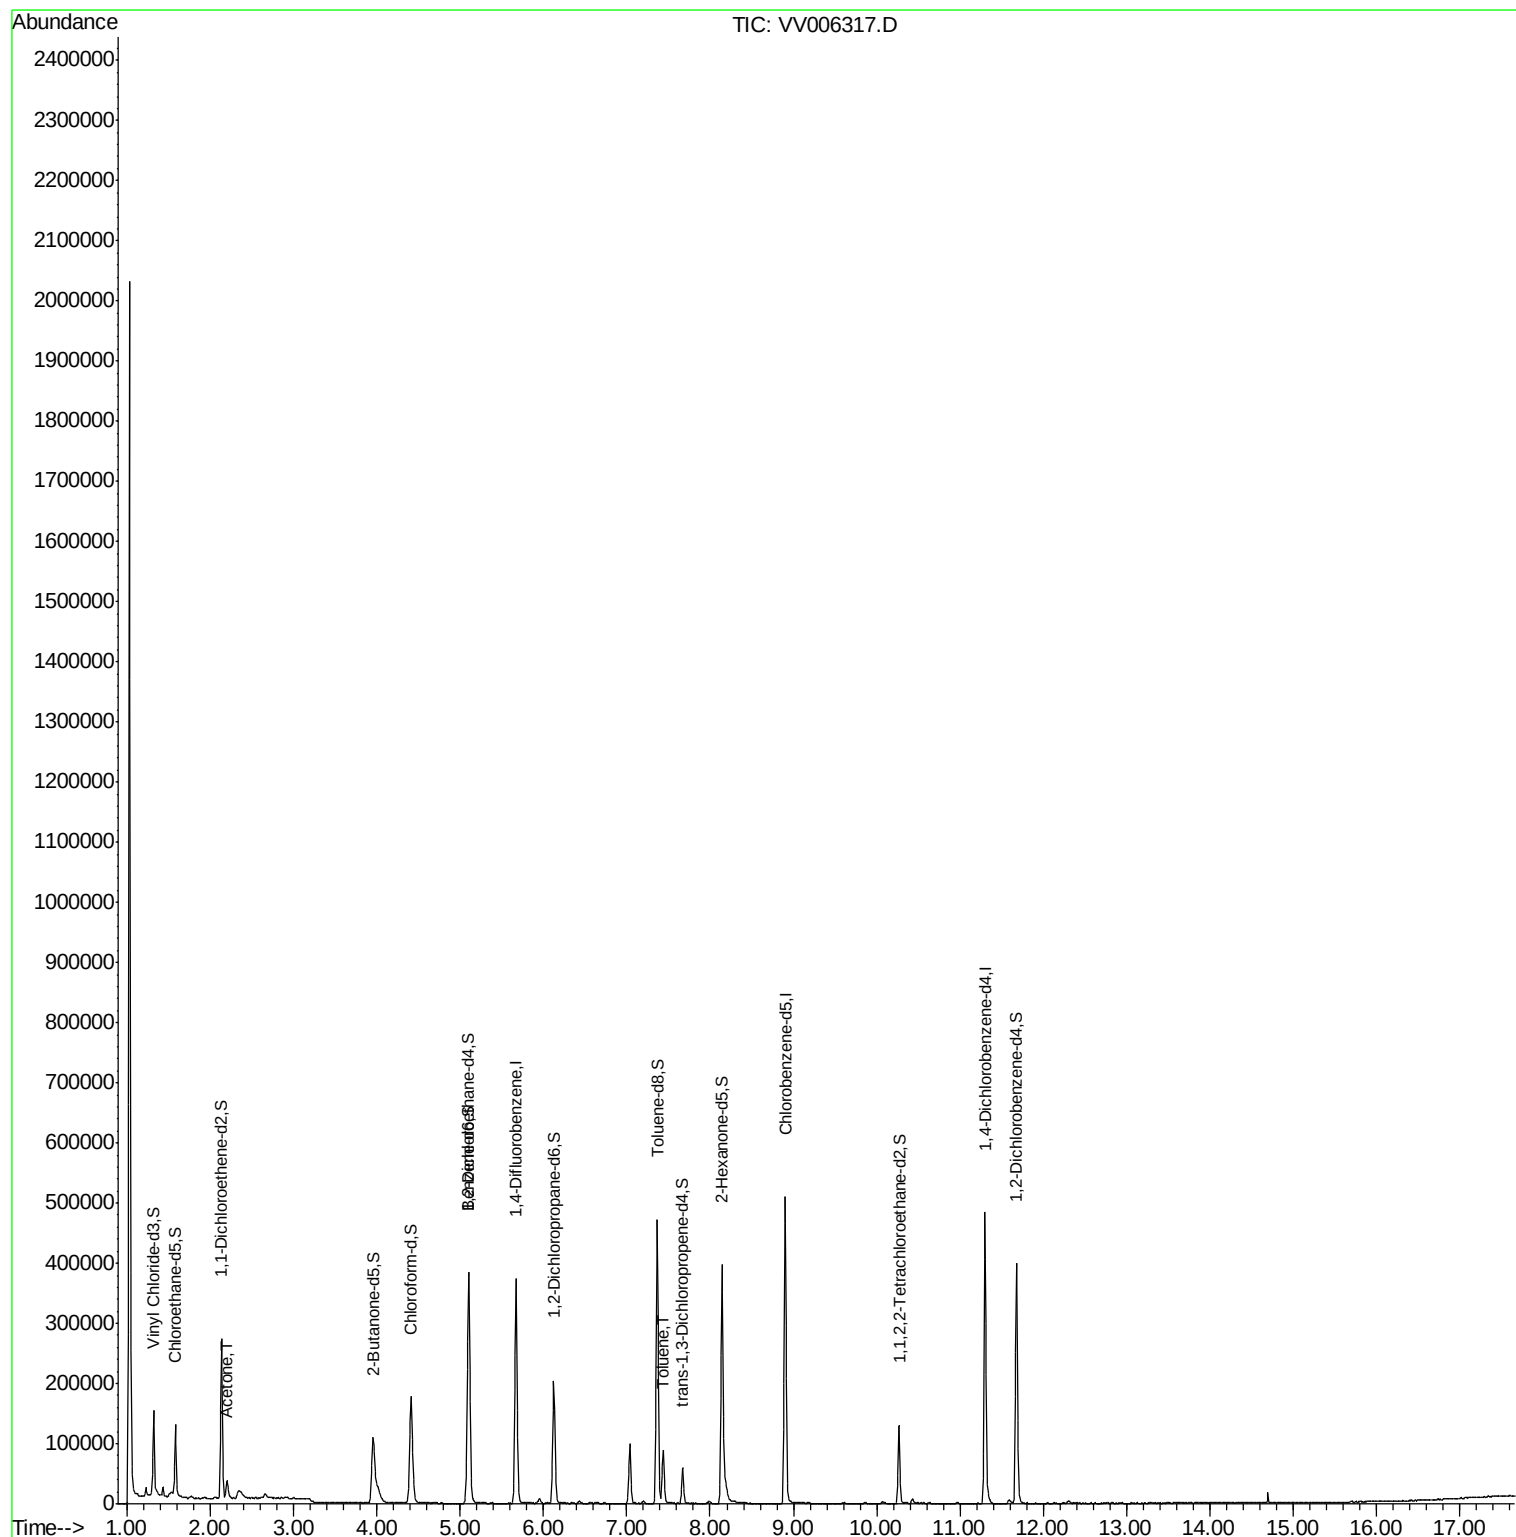

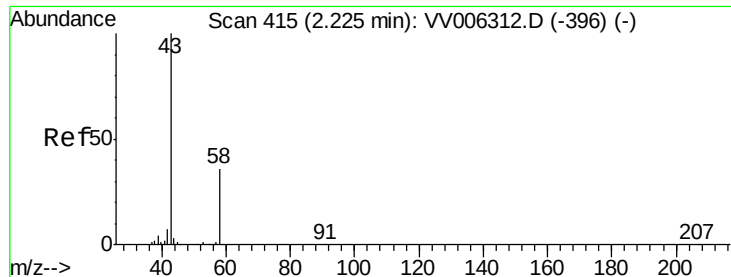

#13

Acetone

Concen: 14.069 ug/L

RT: 2.20 min Scan# 408

Delta R.T. -0.02 min

Lab File: VV006317.D

Acq: 16 Jun 2018 13:39





Instrument :
MSVOA_V
ClientSampleId :
ESWE6

Tot Ion: 43 Resp: 29631

Ion Ratio Lower Upper

43 100

58 38.1 0.0 67.4

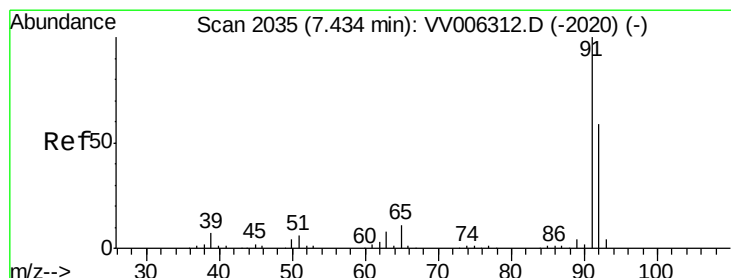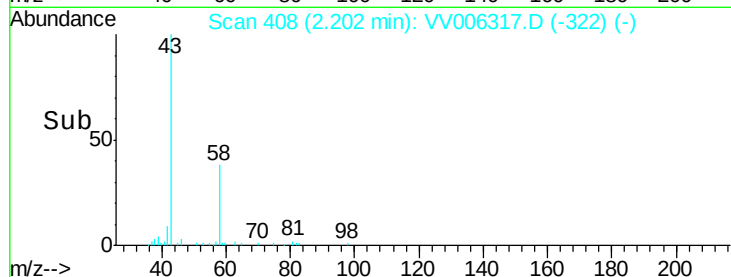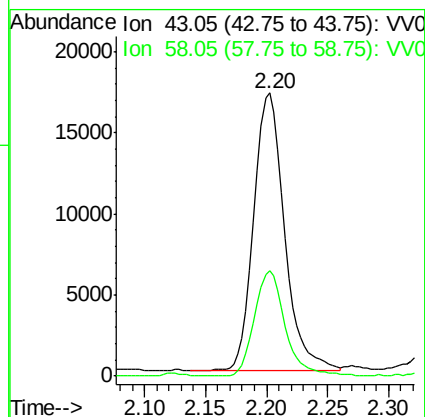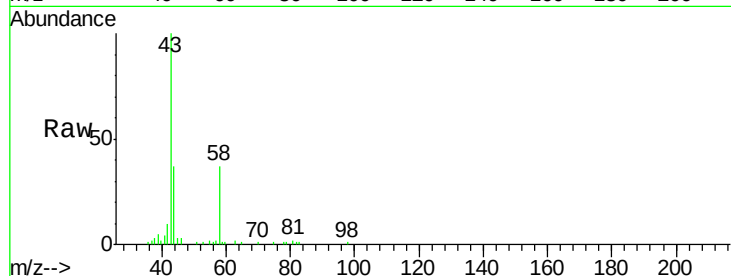

#42

Toluene

Concen: 0.690 ug/L

RT: 7.44 min Scan# 2036

Delta R.T. 0.00 min

Lab File: VV006317.D

Acq: 16 Jun 2018 13:39

Tgt Ion: 91 Resp: 62905

Ion Ratio Lower Upper

91 100

92 57.8 41.1 76.3

