

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061618\
 Data File : VV006318.D
 Acq On : 16 Jun 2018 14:06
 Operator : SY/MD
 Sample : J3549-05
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWE0

Quant Time: Jun 18 01:40:28 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 18 01:15:51 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	291143	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	259539	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	115926	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	72548	4.56	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.20%
7) Chloroethane-d5	1.58	69	63902	5.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.40%
11) 1,1-Dichloroethene-d2	2.13	63	102181	3.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.20%
20) 2-Butanone-d5	3.95	46	200249	59.31	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.62%
24) Chloroform-d	4.41	84	143831	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
26) 1,2-Dichloroethane-d4	5.09	65	74796	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.60%
32) Benzene-d6	5.11	84	298551	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
36) 1,2-Dichloropropane-d6	6.13	67	93491	4.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.80%
41) Toluene-d8	7.37	98	270639	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.00%
43) trans-1,3-Dichloropropene-	7.67	79	30445	3.63	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	72.60%
46) 2-Hexanone-d5	8.14	63	161379	44.55	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.10%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	64884	4.78	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	104224	5.18	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.60%


Target Compounds					Ovalue
13) Acetone	2.20	43	8555	4.676 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061618\
Data File : VV006318.D
Acq On : 16 Jun 2018 14:06
Operator : SY/MD
Sample : J3549-05
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWE0

Quant Time: Jun 18 01:40:28 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 18 01:15:51 2018
Response via : Initial Calibration

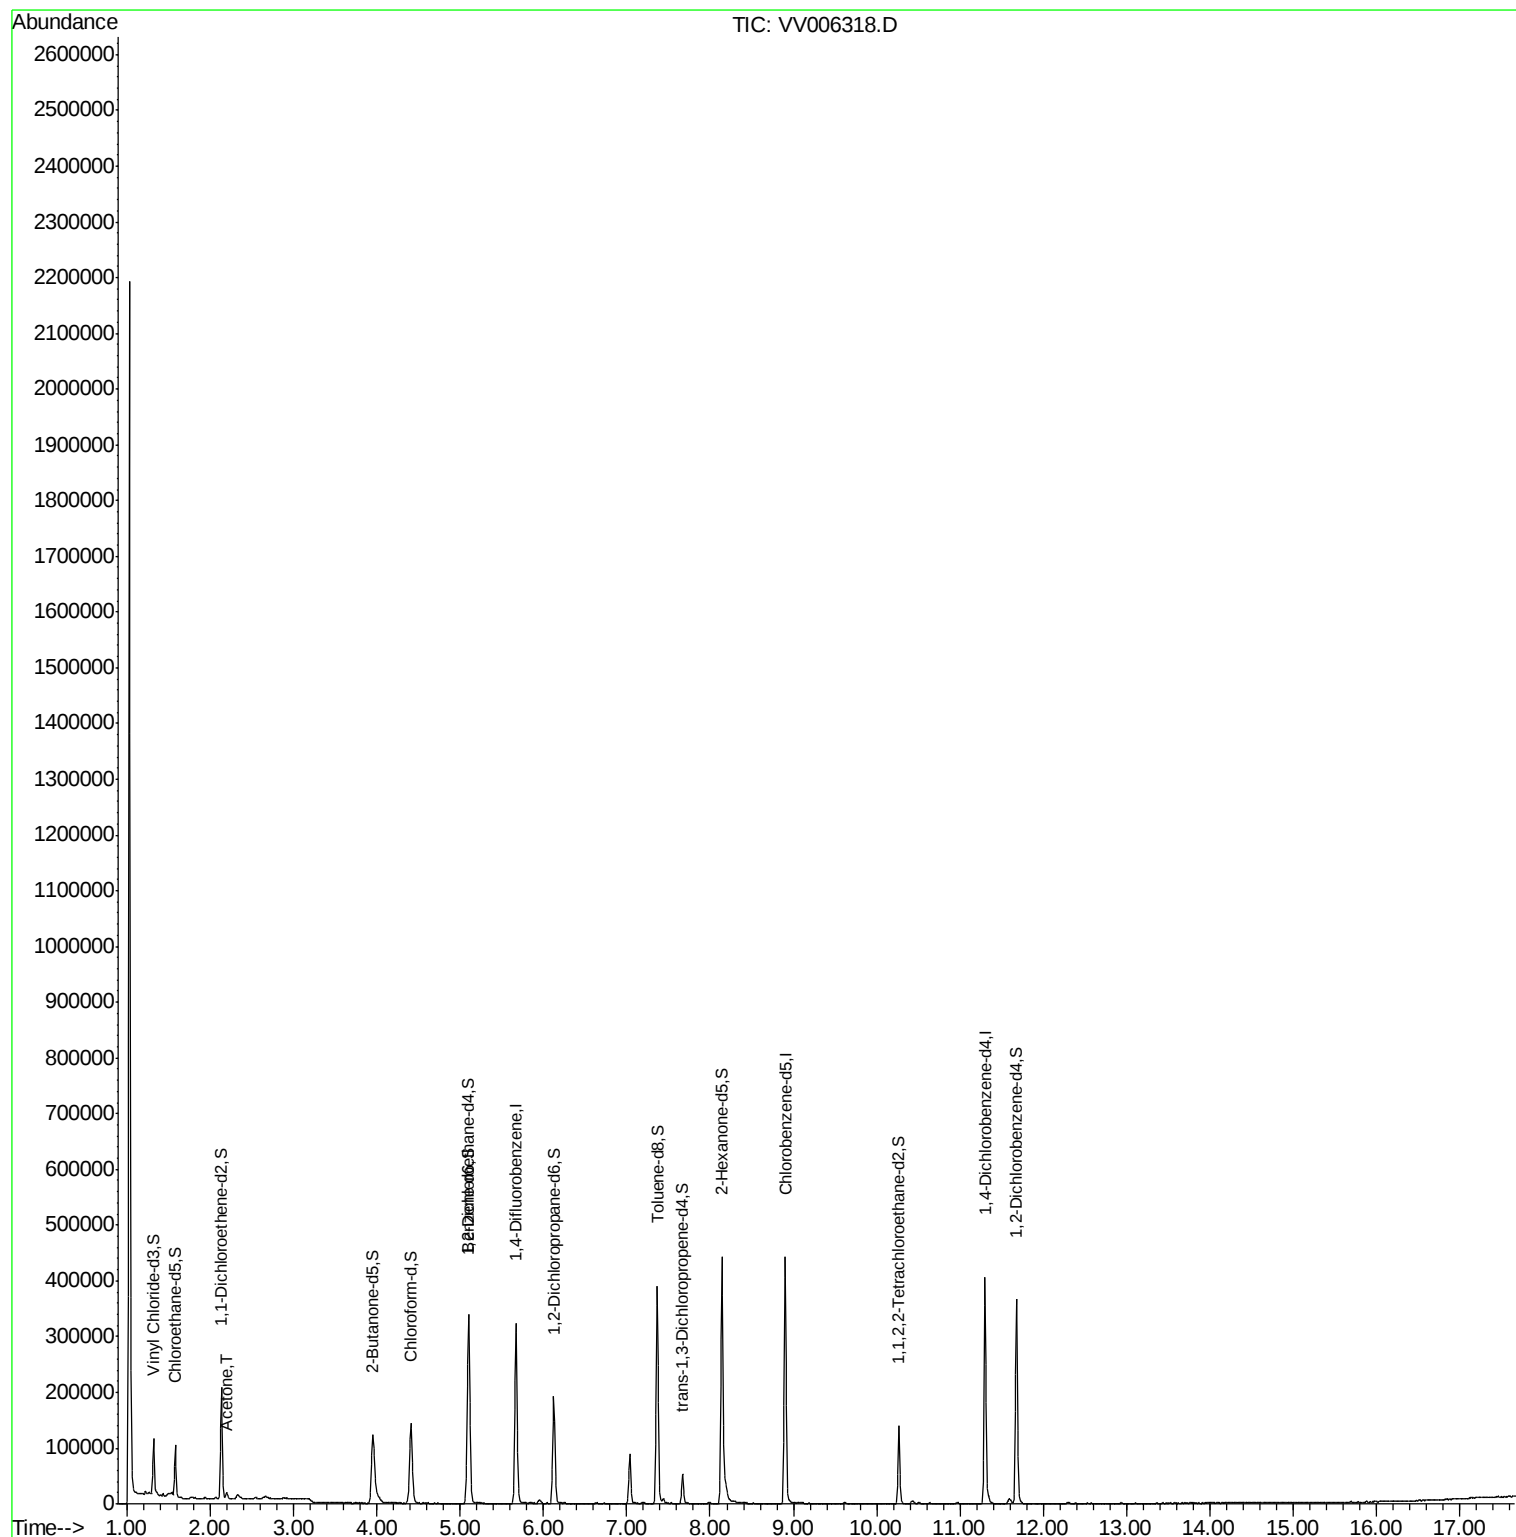

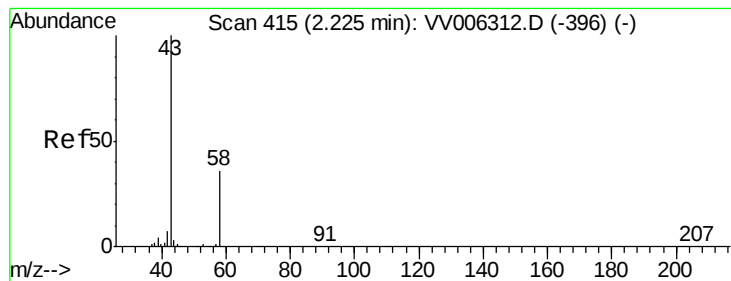

#13

Acetone

Concen: 4.676 ug/L

RT: 2.20 min Scan# 406

Delta R.T. -0.03 min

Lab File: VV006318.D

Acq: 16 Jun 2018 14:06

Instrument :
MSVOA_V
ClientSampleId :
ESWE0

Tot Ion: 43 Resp: 8555

Ion Ratio Lower Upper

43 100

58 39.1 0.0 67.4

