

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061618\
 Data File : VV006329.D
 Acq On : 16 Jun 2018 19:04
 Operator : SY/MD
 Sample : J3549-19
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWF2

Quant Time: Jun 18 02:03:00 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 18 01:15:51 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	310994	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	279912	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	124183	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	69899	4.12	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.40%
7) Chloroethane-d5	1.58	69	60639	4.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.20%
11) 1,1-Dichloroethene-d2	2.13	63	98506	2.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.60%#
20) 2-Butanone-d5	3.95	46	202529	56.16	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.32%
24) Chloroform-d	4.41	84	141605	4.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.20%
26) 1,2-Dichloroethane-d4	5.09	65	74981	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.40%
32) Benzene-d6	5.11	84	298038	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.60%
36) 1,2-Dichloropropane-d6	6.12	67	92912	4.59	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.80%
41) Toluene-d8	7.37	98	267667	4.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.40%
43) trans-1,3-Dichloropropene-	7.67	79	28720	3.17	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	63.40%
46) 2-Hexanone-d5	8.14	63	159205	40.75	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.50%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	64153	4.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	104041	4.83	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.60%


Target Compounds					Ovalue
13) Acetone	2.20	43	12799	6.549 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061618\
Data File : VV006329.D
Acq On : 16 Jun 2018 19:04
Operator : SY/MD
Sample : J3549-19
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWF2

Quant Time: Jun 18 02:03:00 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 18 01:15:51 2018
Response via : Initial Calibration

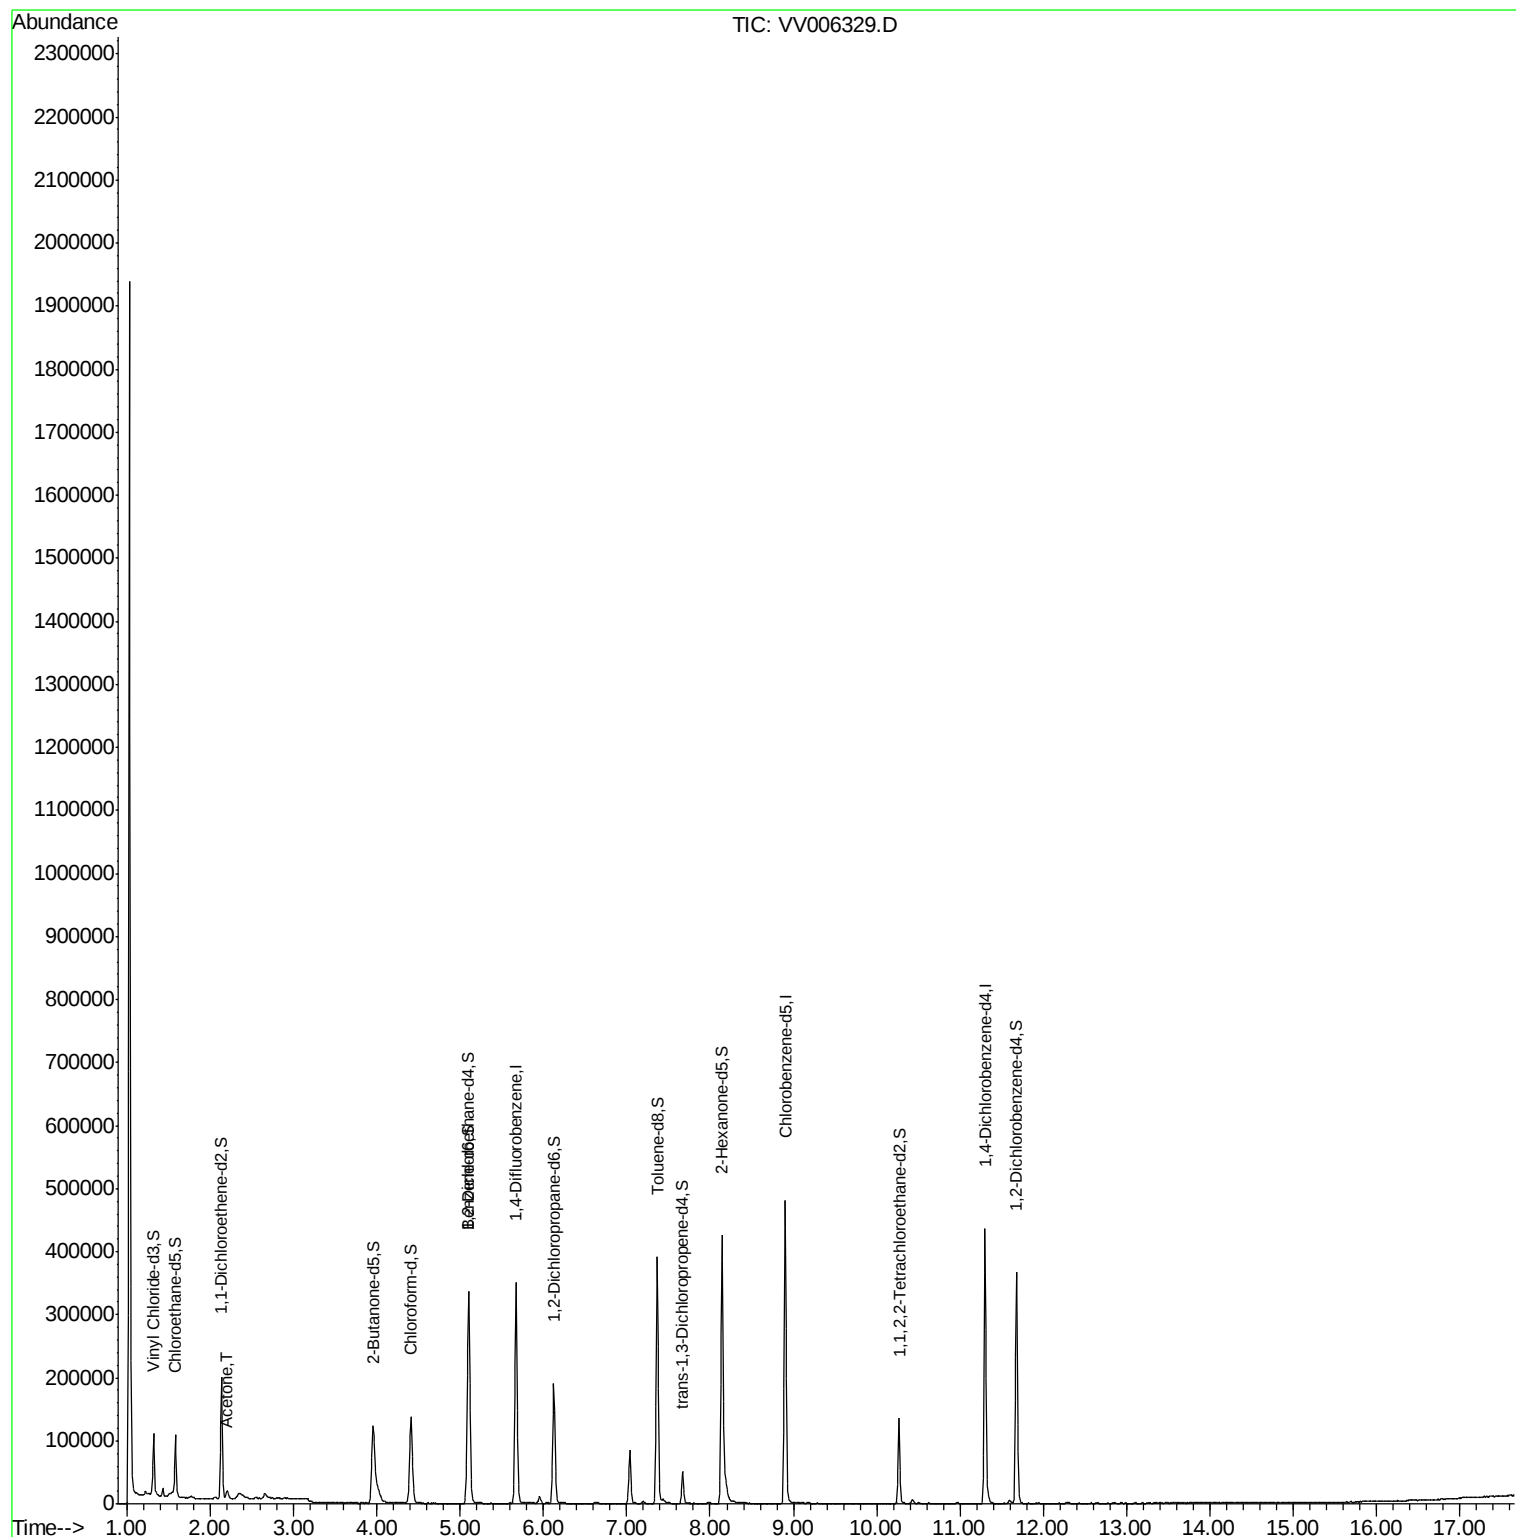

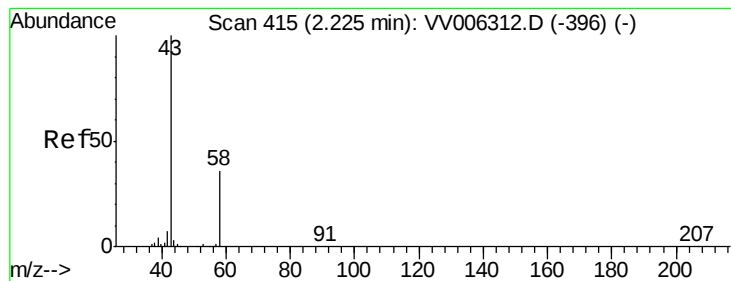

#13
 Acetone
 Concen: 6.549 ug/L
 RT: 2.20 min Scan# 408
 Delta R.T. -0.02 min
 Lab File: VV006329.D
 Acq: 16 Jun 2018 19:04

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWF2

Tot Ion: 43 Resp: 12799
 Ion Ratio Lower Upper
 43 100
 58 36.4 0.0 67.4

