

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061719\
 Data File : VV011560.D
 Acq On : 17 Jun 2019 19:37
 Operator : SY/MD
 Sample : K3289-14
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFCL1

Quant Time: Jun 18 09:27:57 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 18 08:42:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	177439	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	164697	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	65320	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	45105	3.37	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	67.40%
7) Chloroethane-d5	1.58	69	38280	4.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.20%
11) 1,1-Dichloroethene-d2	2.12	63	75239	2.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.00%#
20) 2-Butanone-d5	3.96	46	189641	50.31	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.62%
24) Chloroform-d	4.40	84	112332	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.20%
26) 1,2-Dichloroethane-d4	5.08	65	67111	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.20%
32) Benzene-d6	5.09	84	219276	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.20%
36) 1,2-Dichloropropane-d6	6.12	67	71301	4.57	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.40%
41) Toluene-d8	7.36	98	181491	4.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.80%
43) trans-1,3-Dichloropropene-	7.66	79	21114	4.07	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.40%
46) 2-Hexanone-d5	8.14	63	141129	47.12	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.24%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	51183	4.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	63566	4.88	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.60%


Target Compounds					Ovalue
22) cis-1,2-Dichloroethene	3.96	96	5101	0.361 ug/L	87
34) Trichloroethene	5.96	95	283620	20.675 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061719\
Data File : VV011560.D
Acq On : 17 Jun 2019 19:37
Operator : SY/MD
Sample : K3289-14
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCL1

Quant Time: Jun 18 09:27:57 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 18 08:42:07 2019
Response via : Initial Calibration

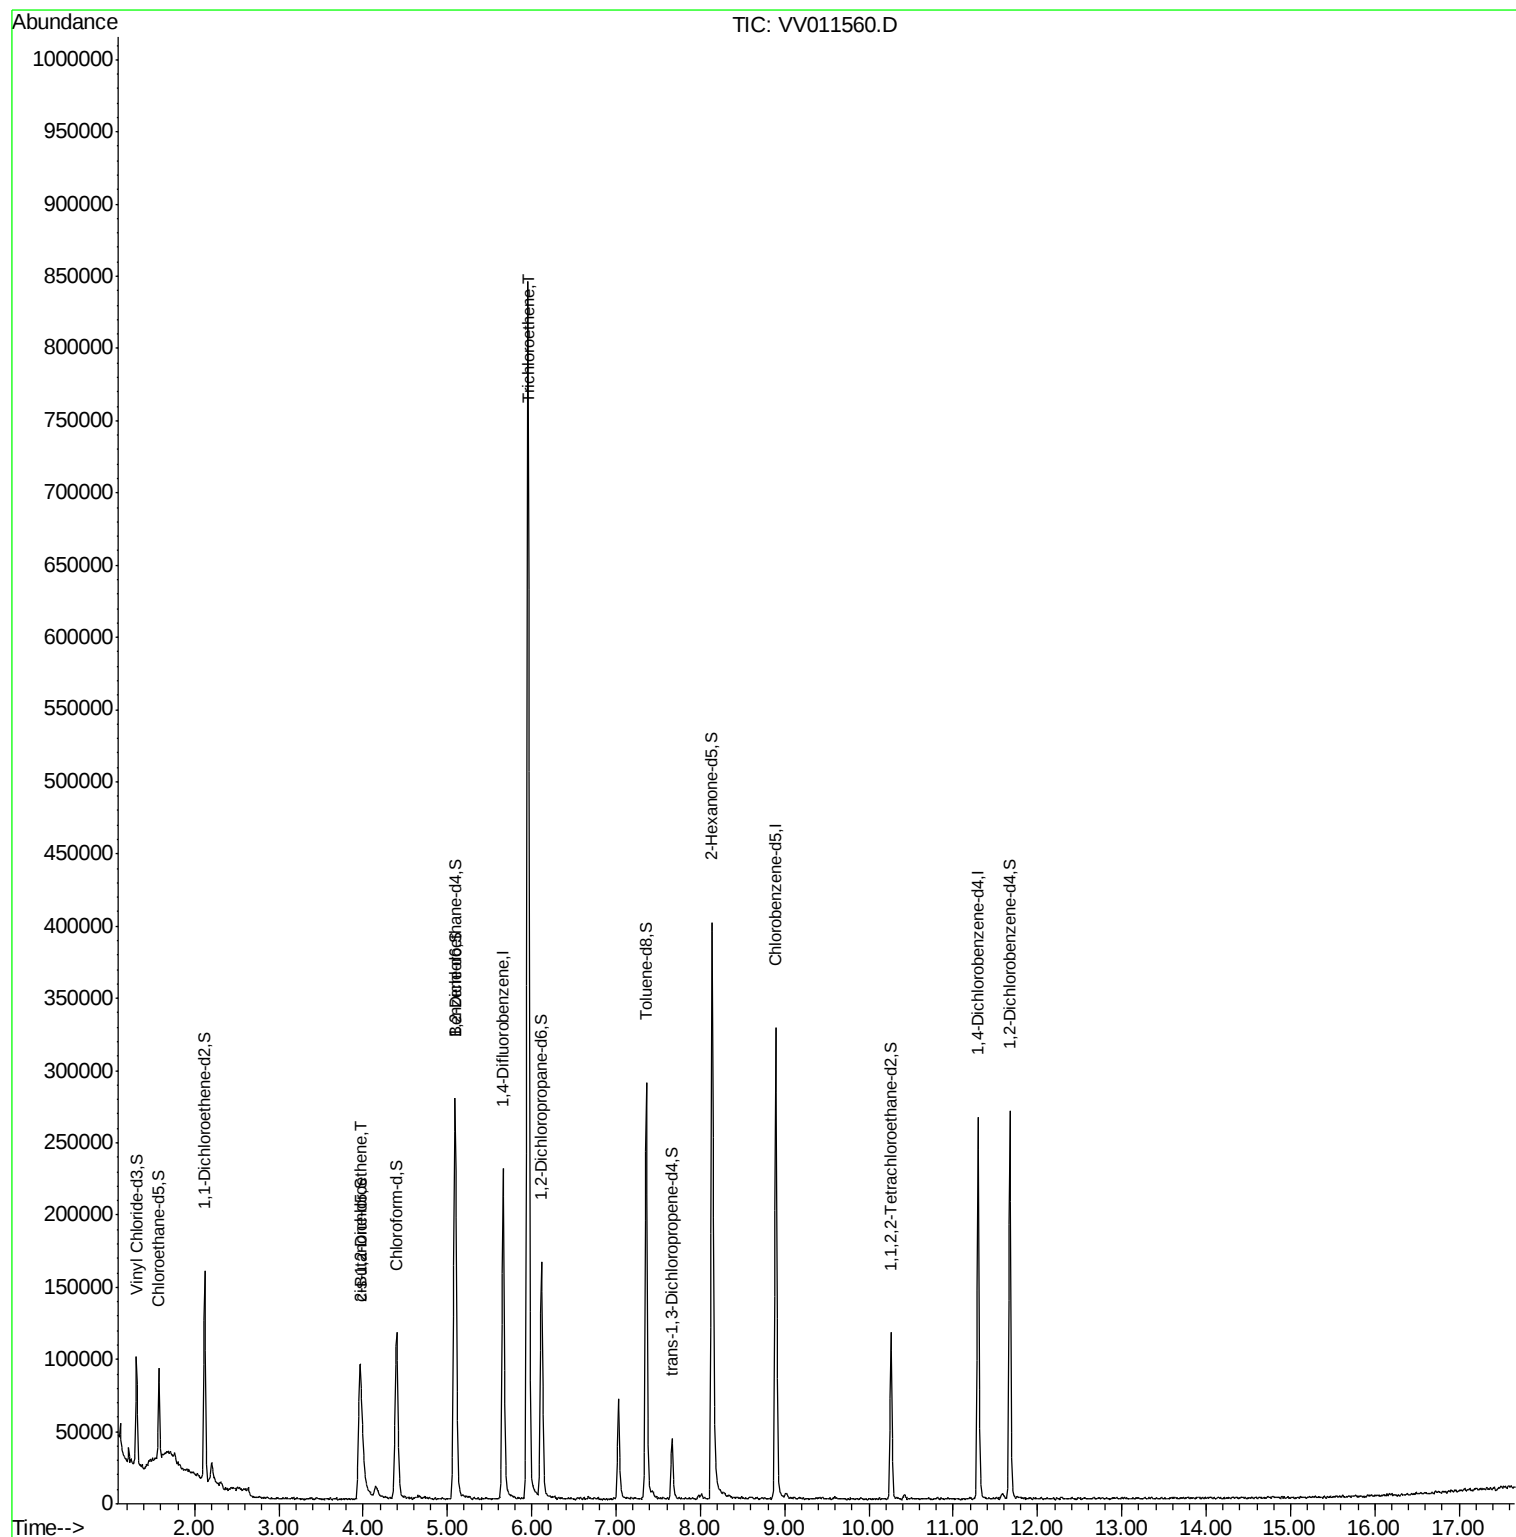

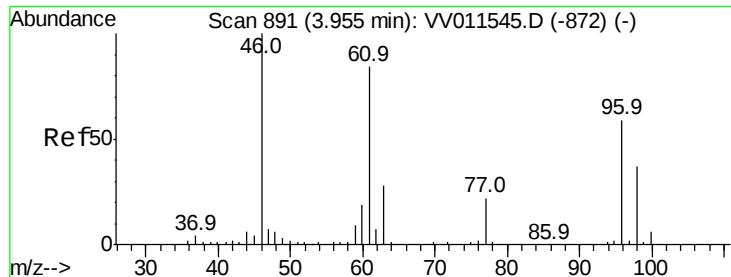


#22




cis-1,2-Dichloroethene
Concen: 0.361 ug/L
RT: 3.96 min Scan# 892
Delta R.T. 0.00 min
Lab File: VV011560.D
Acq: 17 Jun 2019 19:37

Instrument :
MSVOA_V
ClientSampleId :
BFCL1

Tot Ion: 96 Resp: 5101
Ion Ratio Lower Upper
96 100
61 130.4 102.2 189.8
68 0.0 0.0 0.0

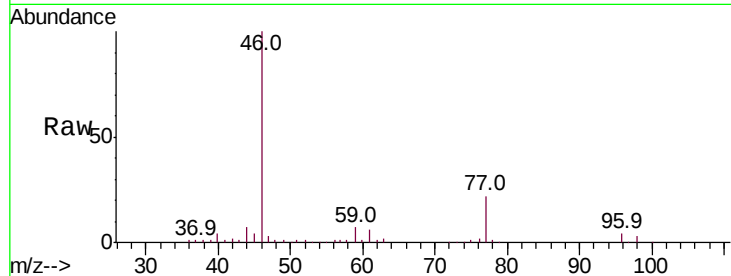


Abundance Ion 96.00 (95.70 to 96.70): VV0
Ion 61.05 (60.75 to 61.75): VV0
Ion 68.15 (67.85 to 68.85): VV0

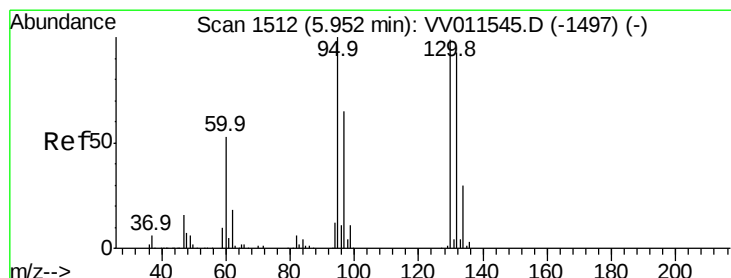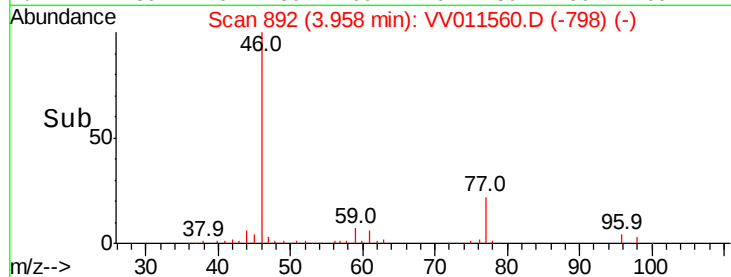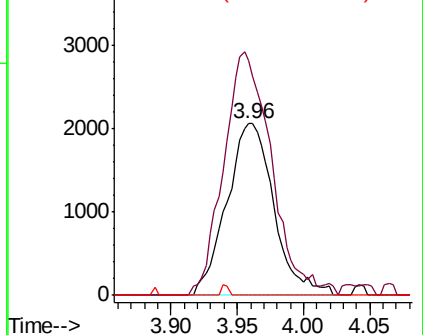

#34

Trichloroethene
Concen: 20.675 ug/L
RT: 5.96 min Scan# 1513
Delta R.T. 0.00 min
Lab File: VV011560.D
Acq: 17 Jun 2019 19:37

Tgt Ion: 95 Resp: 283620
Ion Ratio Lower Upper
95 100
97 62.7 44.4 82.4
132 91.6 63.5 117.9
130 95.7 68.5 127.3

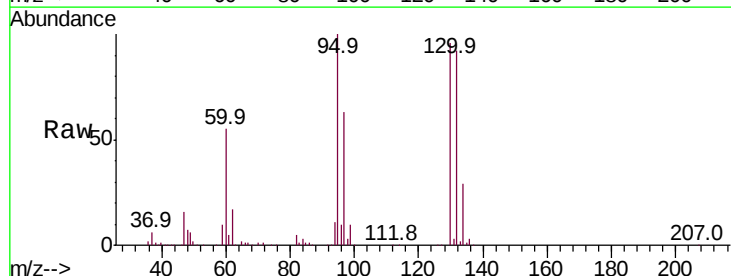

Abundance Ion 95.00 (94.70 to 95.70): VV0
Ion 96.95 (96.65 to 97.65): VV0
Ion 131.95 (131.65 to 132.65): VV0
Ion 129.95 (129.65 to 130.65): VV0

