


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV061719\
 Data File : VV011544.D
 Acq On : 17 Jun 2019 09:07
 Operator : SY/MD
 Sample : BFB49
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB49

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Jun 18 11:44:39 2019

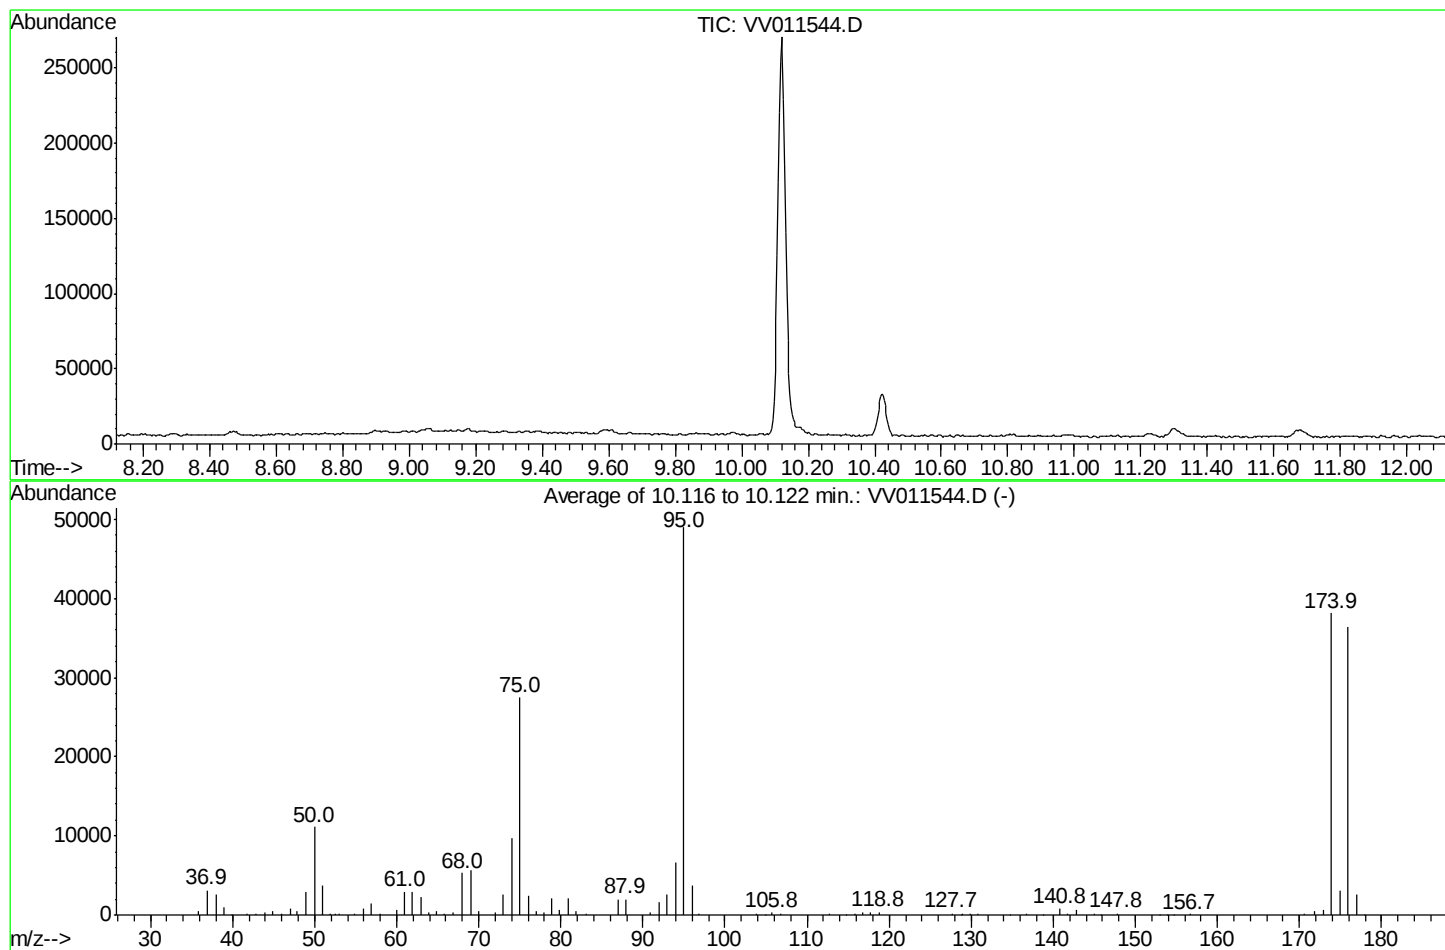

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	11125	PASS
75	95	30	80	56.0	27437	PASS
95	95	100	100	100.0	48994	PASS
96	95	5	9	7.6	3721	PASS
173	174	0.00	2	1.9	717	PASS
174	95	50	120	77.8	38112	PASS
175	174	5	9	8.0	3054	PASS
176	174	95	101	95.6	36437	PASS
177	176	5	9	7.3	2670	PASS

Scan 2794 (10.074 min): VV011544.D
BFB49

m/z	Abundance
35.90	1817.0
37.00	247.0
37.90	798.0
38.90	183.0
39.90	1775.0
40.90	135.0
42.00	143.0
42.30	132.0
42.80	123.0
43.90	487.0
45.00	145.0
55.90	102.0
56.40	108.0
56.90	116.0
73.20	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
35.90	2360.0
36.90	3313.0
38.00	3347.0
38.90	1123.0
39.90	1784.0
40.70	127.0
41.70	202.0
42.90	223.0
44.00	752.0
44.80	663.0
47.00	724.0
47.90	565.0
49.00	2960.0
50.00	10799.0
51.00	3869.0
52.00	186.0
54.80	206.0
55.90	870.0
56.90	1713.0
57.90	233.0
60.00	642.0
61.00	3008.0
61.90	2853.0
62.90	2137.0
63.90	394.0
64.90	472.0
65.80	133.0
66.90	304.0
68.00	5252.0
69.00	5696.0
70.00	559.0
71.90	332.0
73.00	2566.0
74.00	9507.0
75.00	26800.0
76.00	2387.0
77.00	470.0
78.00	342.0
78.90	2032.0
79.80	541.0
80.90	2127.0
81.90	507.0
83.10	152.0
86.90	1930.0
87.90	1984.0
90.90	245.0
91.90	1576.0
92.90	2407.0
94.00	6628.0
95.00	47872.0
96.00	3772.0
96.80	116.0
103.80	222.0
104.90	126.0
105.70	304.0
106.70	104.0
112.80	124.0
114.80	140.0
115.90	234.0
116.80	301.0
117.70	270.0
118.80	352.0
127.70	225.0
128.80	153.0
129.90	208.0
130.80	113.0
136.70	134.0
138.70	101.0
140.80	789.0
141.80	151.0
142.80	637.0
147.70	133.0
156.80	112.0
170.60	105.0
171.90	524.0
173.00	700.0
173.90	36520.0
174.90	3078.0
175.90	34512.0
176.90	2519.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
35.90	2374.0
36.90	3482.0
38.00	3460.0
38.90	1234.0
39.90	1821.0
40.80	145.0
41.70	186.0
42.90	271.0
43.90	795.0
44.80	629.0
45.90	164.0
47.00	795.0
47.90	563.0
49.00	3067.0
50.00	11393.0
51.00	3897.0
51.90	227.0
52.50	151.0
52.90	128.0
54.80	224.0
56.00	938.0
56.90	1665.0
57.90	216.0
60.00	614.0
61.00	3054.0
61.90	3058.0
62.90	2313.0
63.90	353.0
64.90	543.0
65.80	153.0
66.90	343.0
68.00	5410.0
69.00	5910.0
70.00	557.0
72.00	351.0
73.00	2710.0
74.00	10091.0
75.00	28256.0
76.00	2525.0
76.90	429.0
77.90	340.0
78.90	2235.0
79.80	605.0
80.90	2231.0
81.90	550.0
83.10	172.0
87.00	2057.0
87.90	2102.0
90.80	273.0
91.90	1713.0
92.90	2654.0
94.00	6831.0
95.00	50312.0
96.00	3933.0
96.80	133.0
103.90	225.0
104.90	106.0
105.80	294.0
106.70	130.0
112.70	146.0
115.80	250.0
116.80	326.0
117.80	268.0
118.80	427.0
127.60	226.0
129.00	151.0
129.90	192.0
130.80	128.0
136.80	141.0
138.70	120.0
140.90	783.0
141.80	179.0
142.90	672.0
144.90	115.0
145.90	109.0
147.80	166.0
153.00	105.0
154.60	125.0
156.70	128.0
170.60	115.0
171.80	520.0
172.90	742.0
173.90	39392.0
174.90	3189.0
175.90	37688.0
176.90	2794.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
35.90	2285.0
36.90	3325.0
38.00	3332.0
38.90	1244.0
39.90	1771.0
40.80	130.0
41.70	153.0
42.90	272.0
43.90	824.0
44.80	620.0
45.90	183.0
47.00	799.0
47.90	458.0
49.00	2687.0
50.00	11183.0
51.00	3497.0
51.90	269.0
52.60	164.0
53.00	169.0
54.80	222.0
56.00	988.0
57.00	1577.0
58.00	163.0
59.90	548.0
61.00	2831.0
61.90	2937.0
62.90	2344.0
63.90	347.0
64.90	512.0
65.70	155.0
66.90	294.0
68.00	5232.0
69.00	5612.0
70.00	488.0
72.00	360.0
73.00	2706.0
74.00	9656.0
75.00	27256.0
76.00	2372.0
76.90	371.0
77.90	281.0
78.90	2165.0
79.80	641.0
80.90	2026.0
81.90	553.0
82.90	162.0
87.00	1953.0
87.90	1948.0
90.80	299.0
91.90	1702.0
92.90	2564.0
94.00	6422.0
95.00	48800.0
96.00	3460.0
96.90	154.0
103.90	223.0
105.80	290.0
106.80	130.0
112.70	147.0
115.80	243.0
116.80	343.0
117.80	263.0
118.80	440.0
127.70	220.0
129.00	133.0
129.80	181.0
130.80	122.0
134.70	106.0
136.80	155.0
140.90	705.0
141.80	157.0
142.90	694.0
145.00	145.0
145.80	111.0
147.80	189.0
153.00	104.0
153.90	113.0
154.60	104.0
156.60	131.0
170.60	110.0
171.80	505.0
173.00	710.0
173.90	38424.0
174.90	2897.0
175.90	37112.0
176.90	2697.0
177.90	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49