

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061818\
 Data File : VV006337.D
 Acq On : 18 Jun 2018 13:20
 Operator : SY/MD
 Sample : J3550-16
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWG6

Quant Time: Jun 18 13:45:37 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 18 03:14:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	309179	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	276966	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	126642	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	104823	6.21	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	124.20%
7) Chloroethane-d5	1.58	69	82911	6.13	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	122.60%
11) 1,1-Dichloroethene-d2	2.13	63	143588	4.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.60%
20) 2-Butanone-d5	3.95	46	208752	58.22	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.44%
24) Chloroform-d	4.41	84	173789	5.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.40%
26) 1,2-Dichloroethane-d4	5.09	65	88077	5.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.40%
32) Benzene-d6	5.11	84	388476	5.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	116.80%
36) 1,2-Dichloropropane-d6	6.12	67	113227	5.66	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	113.20%
41) Toluene-d8	7.37	98	360907	5.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.80%
43) trans-1,3-Dichloropropene-	7.67	79	38884	4.34	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.80%
46) 2-Hexanone-d5	8.14	63	171186	44.28	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.56%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	70225	4.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	127784	5.82	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.40%


Target Compounds					Ovalue
13) Acetone	2.20	43	8626	4.440 ug/L	88
21) 2-Butanone	4.04	43	10523	2.977 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061818\
Data File : VV006337.D
Acq On : 18 Jun 2018 13:20
Operator : SY/MD
Sample : J3550-16
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWG6

Quant Time: Jun 18 13:45:37 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 18 03:14:32 2018
Response via : Initial Calibration

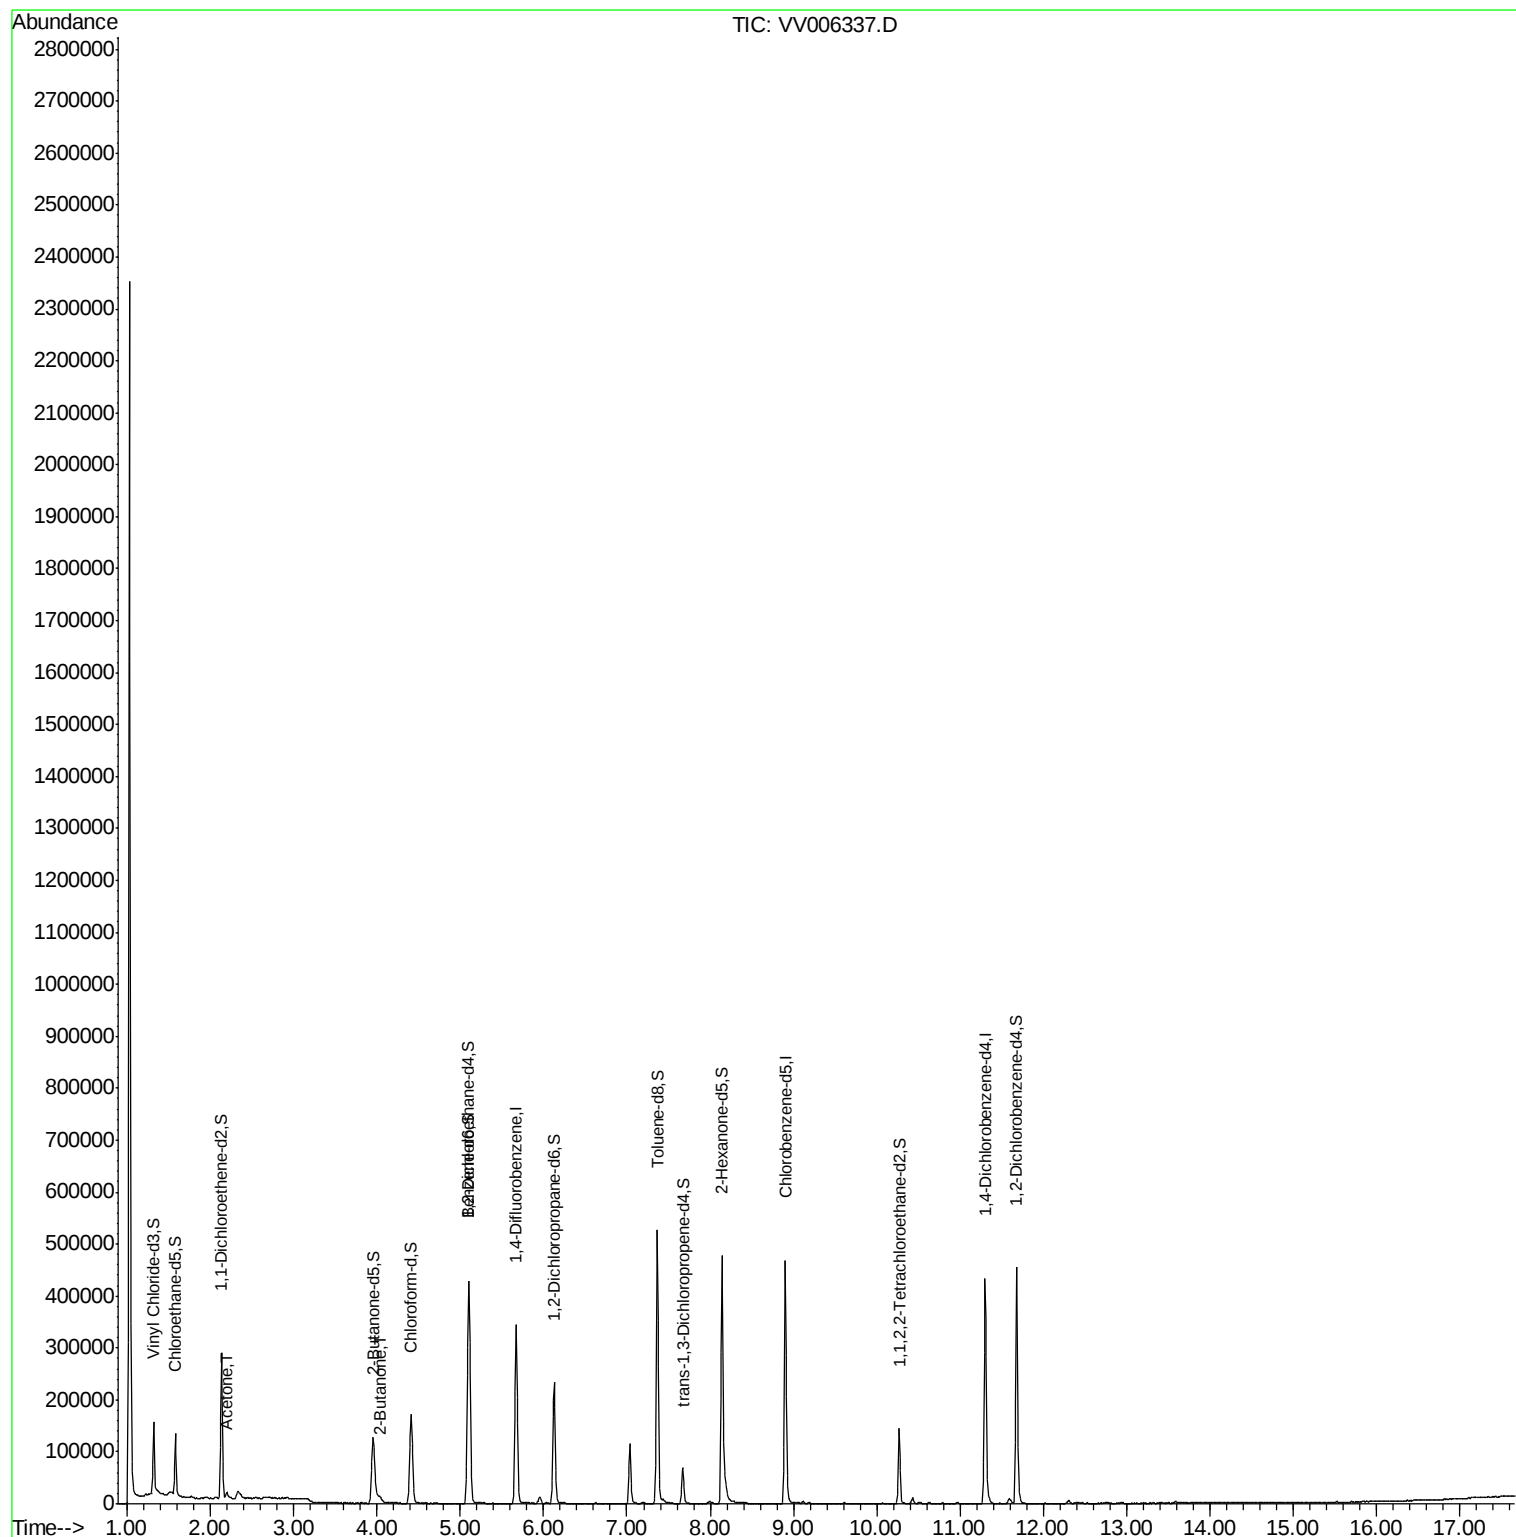

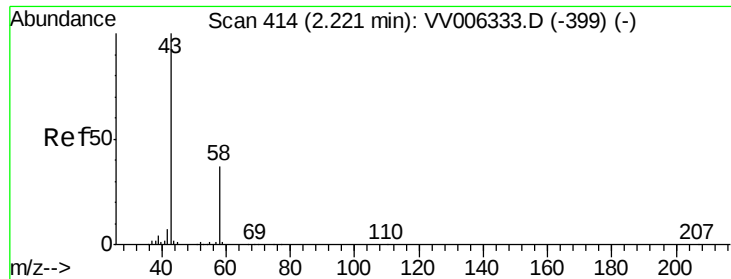

#13

Acetone

Concen: 4.440 ug/L

RT: 2.20 min Scan# 407

Delta R.T. -0.02 min

Lab File: VV006337.D

Acq: 18 Jun 2018 13:20

Instrument :

MSVOA_V

ClientSampleId :


ESWG6

Tot Ion: 43 Resp: 8626

Ion Ratio Lower Upper




43 100

58 40.3 0.0 67.4

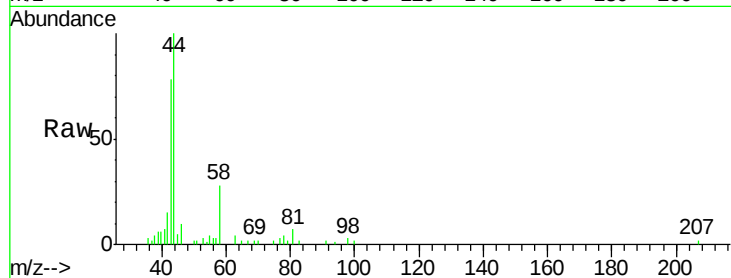

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

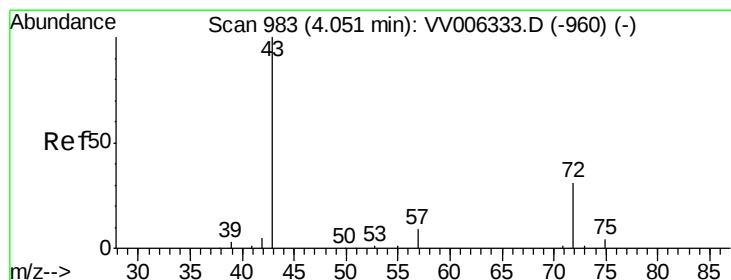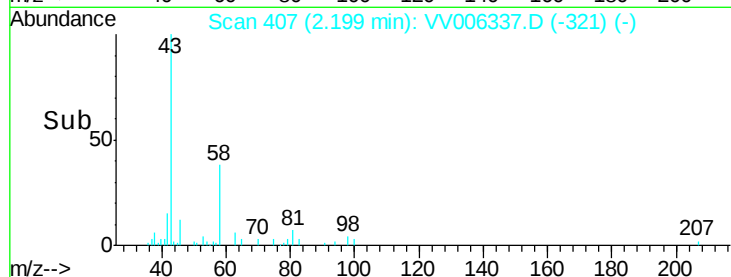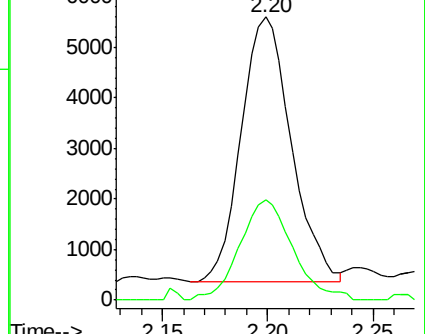

#21

2-Butanone

Concen: 2.977 ug/L

RT: 4.04 min Scan# 981

Delta R.T. -0.01 min

Lab File: VV006337.D


Acq: 18 Jun 2018 13:20

Tgt Ion: 43 Resp: 10523

Ion Ratio Lower Upper

43 100

72 30.9 13.8 41.3

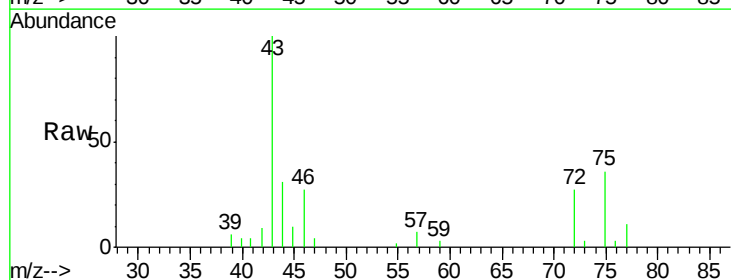

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 72.10 (71.80 to 72.80): VV0

