

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061818\
 Data File : VV006339.D
 Acq On : 18 Jun 2018 14:14
 Operator : SY/MD
 Sample : J3550-05
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWF7

Quant Time: Jun 19 02:06:51 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 19 02:03:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	309330	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	278264	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	126963	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	97912	5.80	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	116.00%
7) Chloroethane-d5	1.58	69	76798	5.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	113.60%
11) 1,1-Dichloroethene-d2	2.13	63	132331	4.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.60%
20) 2-Butanone-d5	3.95	46	196913	54.89	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.78%
24) Chloroform-d	4.41	84	161148	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
26) 1,2-Dichloroethane-d4	5.09	65	81603	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.20%
32) Benzene-d6	5.11	84	360992	5.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.00%
36) 1,2-Dichloropropane-d6	6.12	67	104606	5.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.00%
41) Toluene-d8	7.37	98	330469	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.60%
43) trans-1,3-Dichloropropene-	7.67	79	35180	3.91	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.20%
46) 2-Hexanone-d5	8.14	63	159988	41.19	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.38%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	65609	4.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	119716	5.44	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.80%


Target Compounds					Ovalue
13) Acetone	2.20	43	16219	8.344 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061818\
Data File : VV006339.D
Acq On : 18 Jun 2018 14:14
Operator : SY/MD
Sample : J3550-05
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWF7

Quant Time: Jun 19 02:06:51 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 19 02:03:29 2018
Response via : Initial Calibration

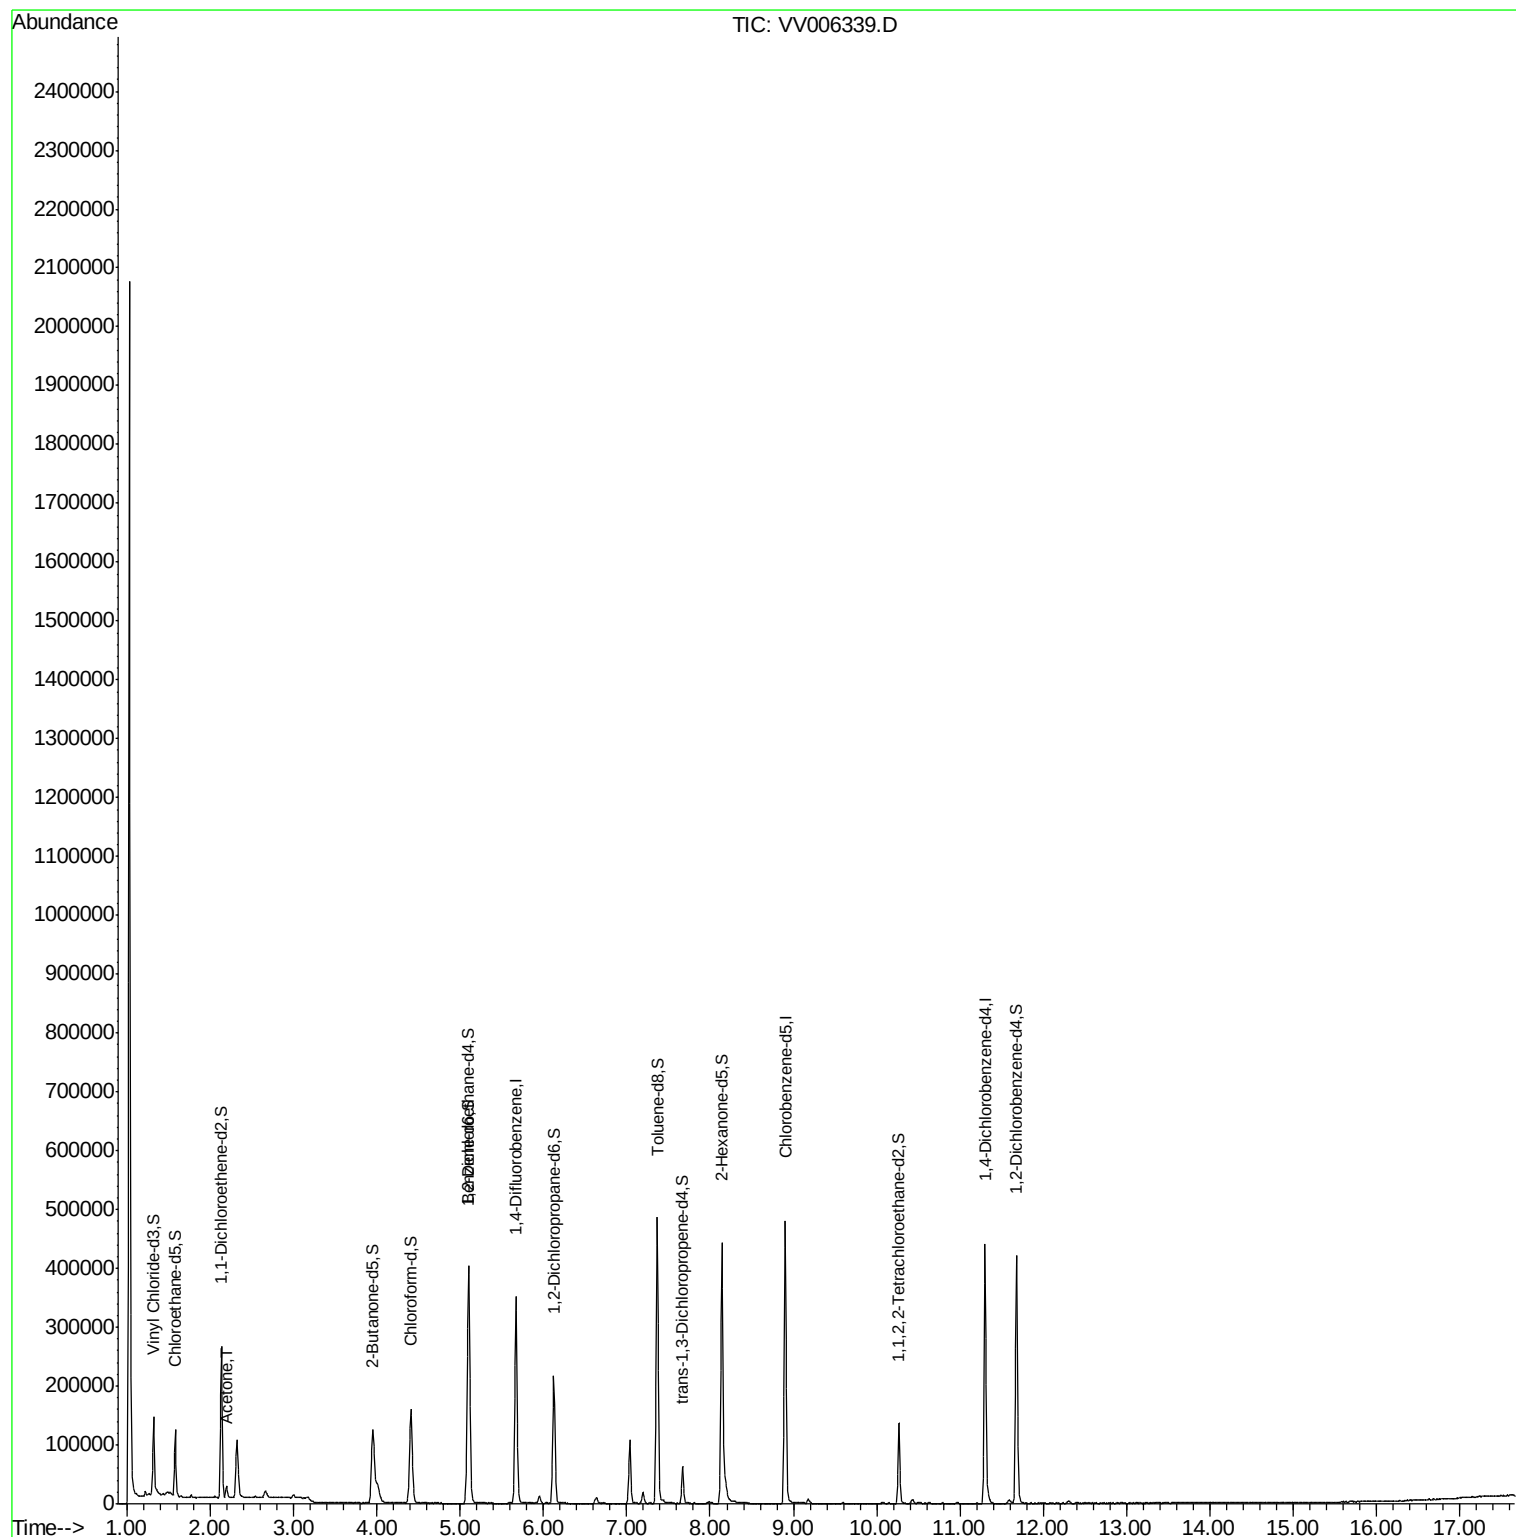

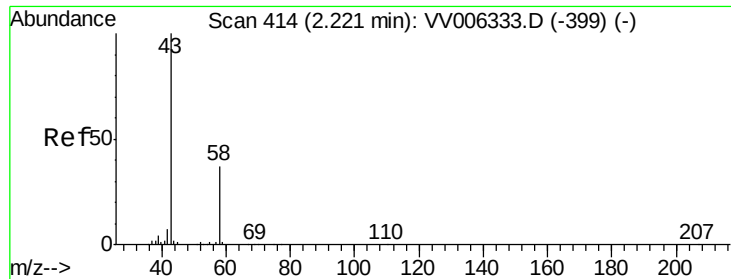

#13

Acetone

Concen: 8.344 ug/L

RT: 2.20 min Scan# 406

Delta R.T. -0.03 min

Lab File: VV006339.D

Acq: 18 Jun 2018 14:14

Instrument :
MSVOA_V
ClientSampleId :
ESWF7

Tot Ion: 43 Resp: 16219

Ion Ratio Lower Upper

43 100

58 38.1 0.0 67.4

