

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061818\
 Data File : VV006340.D
 Acq On : 18 Jun 2018 14:44
 Operator : SY/MD
 Sample : J3514-01
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KF8

Quant Time: Jun 19 02:07:52 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 19 02:03:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	296855	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	267889	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	117890	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	63708	3.93	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.60%
7) Chloroethane-d5	1.58	69	57547	4.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.60%
11) 1,1-Dichloroethene-d2	2.13	63	87314	2.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.40%#
20) 2-Butanone-d5	3.95	46	191212	55.54	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.08%
24) Chloroform-d	4.41	84	136914	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.20%
26) 1,2-Dichloroethane-d4	5.09	65	70190	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.60%
32) Benzene-d6	5.10	84	282770	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.80%
36) 1,2-Dichloropropane-d6	6.12	67	88261	4.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.20%
41) Toluene-d8	7.37	98	250356	4.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.60%
43) trans-1,3-Dichloropropene-	7.67	79	24853	2.87	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	57.40%
46) 2-Hexanone-d5	8.14	63	141239	37.77	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.54%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	59525	4.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	97829	4.79	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.80%


Target Compounds					Ovalue
13) Acetone	2.19	43	14496	7.771 ug/L	91
34) Trichloroethene	5.96	95	40979	2.033 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061818\
Data File : VV006340.D
Acq On : 18 Jun 2018 14:44
Operator : SY/MD
Sample : J3514-01
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KF8

Quant Time: Jun 19 02:07:52 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 19 02:03:29 2018
Response via : Initial Calibration

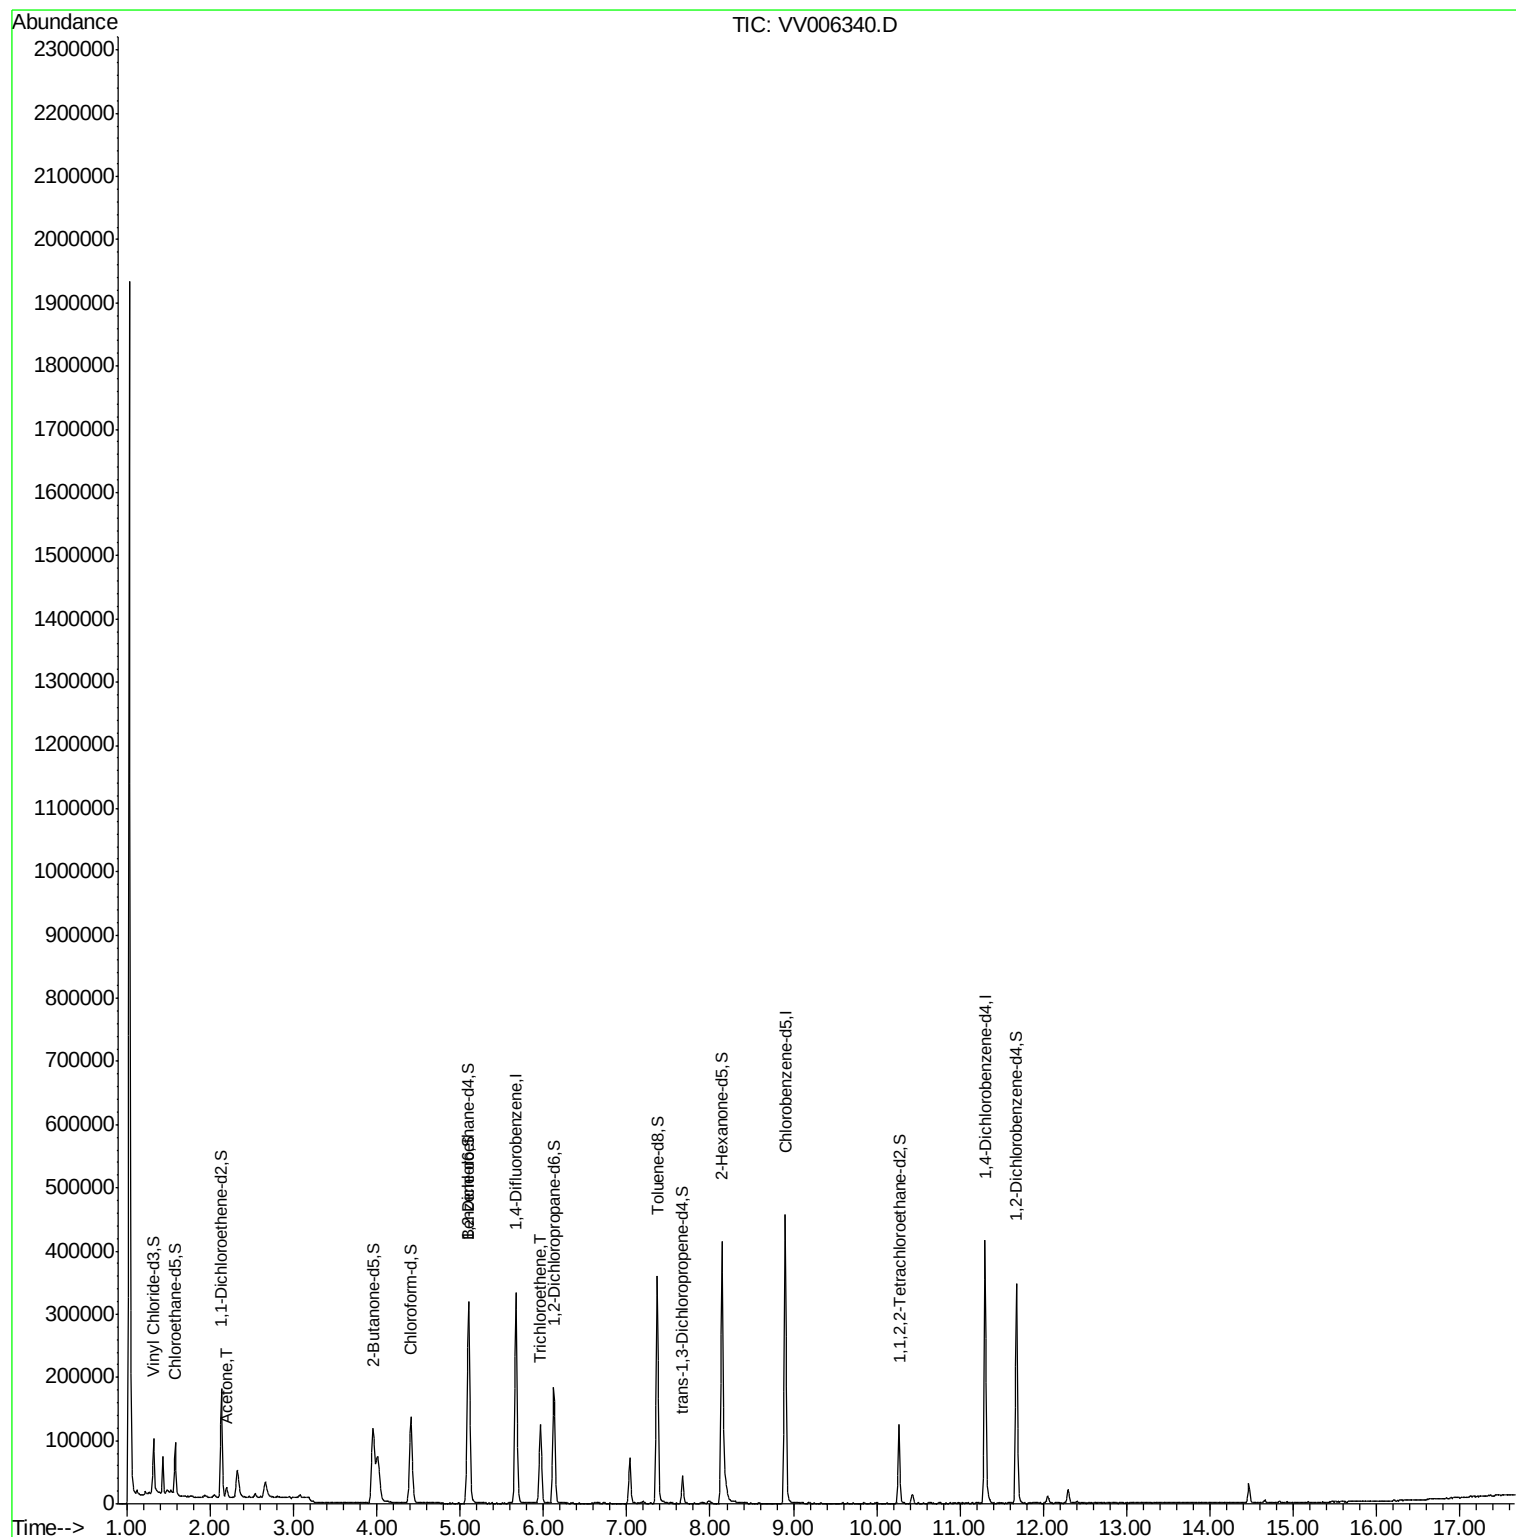

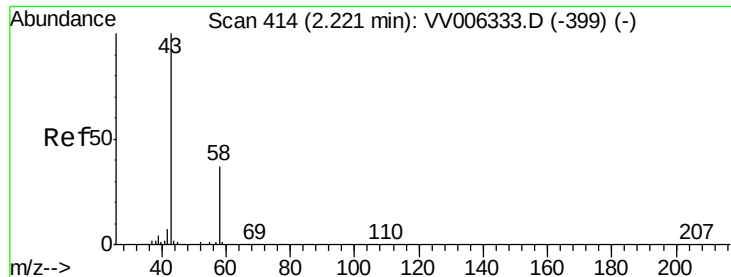

#13

Acetone

Concen: 7.771 ug/L

RT: 2.19 min Scan# 405

Delta R.T. -0.03 min

Lab File: VV006340.D

Acq: 18 Jun 2018 14:44

Instrument :

MSVOA_V

ClientSampled :


C0KF8

Tot Ion: 43 Resp: 14496

Ion Ratio Lower Upper

43 100

58 38.7 0.0 67.4

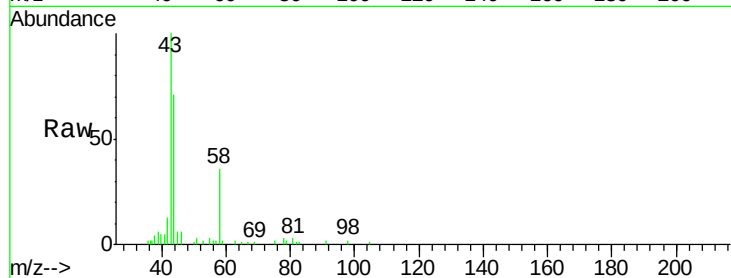

Abundance Ion 43.05 (42.75 to 43.75): VV006333.D (-399) (-)

Ion 58.05 (57.75 to 58.75): VV006333.D (-399) (-)

2.19

10000

8000

6000



4000

2000

0

Time-->

2.10 2.15 2.20 2.25 2.30

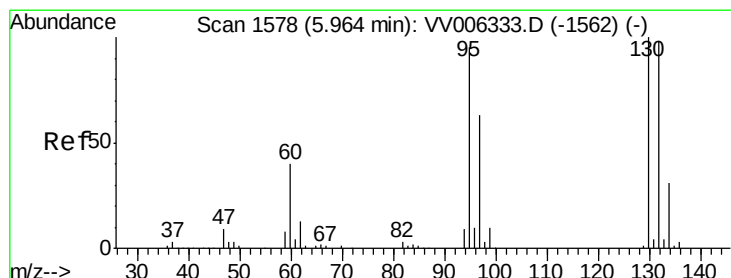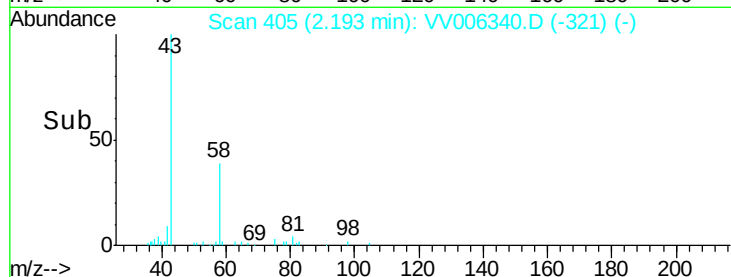

#34

Trichloroethene

Concen: 2.033 ug/L

RT: 5.96 min Scan# 1578

Delta R.T. 0.00 min

Lab File: VV006340.D

Acq: 18 Jun 2018 14:44

Tgt Ion: 95 Resp: 40979


Ion Ratio Lower Upper

95 100

97 64.2 45.1 83.9

132 101.6 69.0 128.1

130 107.7 72.8 135.2

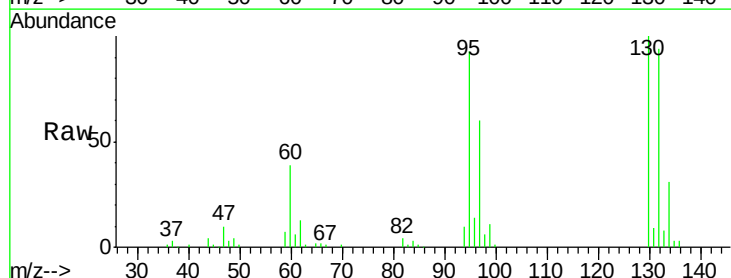

Abundance Ion 95.00 (94.70 to 95.70): VV006333.D (-1562) (-)

Ion 96.95 (96.65 to 97.65): VV006333.D (-1562) (-)

Ion 131.95 (131.65 to 132.65): VV006333.D (-1562) (-)

Ion 129.95 (129.65 to 130.65): VV006333.D (-1562) (-)

30000

20000

10000

0

Time-->

5.90 5.95 6.00 6.05

