

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061818\
 Data File : VV006341.D
 Acq On : 18 Jun 2018 15:11
 Operator : SY/MD
 Sample : J3514-02
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KF9

Quant Time: Jun 19 02:08:55 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 19 02:03:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	296388	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	261924	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	114239	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	64643	3.99	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.80%
7) Chloroethane-d5	1.58	69	57486	4.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.60%
11) 1,1-Dichloroethene-d2	2.13	63	92086	2.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.60%#
20) 2-Butanone-d5	3.95	46	194569	56.61	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.22%
24) Chloroform-d	4.41	84	138845	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.60%
26) 1,2-Dichloroethane-d4	5.09	65	72483	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.60%
32) Benzene-d6	5.11	84	283058	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.00%
36) 1,2-Dichloropropane-d6	6.12	67	89469	4.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.60%
41) Toluene-d8	7.37	98	249825	4.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.20%
43) trans-1,3-Dichloropropene-	7.67	79	24093	2.84	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	56.80%
46) 2-Hexanone-d5	8.14	63	140738	38.50	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.00%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	59982	4.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	97282	4.91	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.20%


Target Compounds					Ovalue
13) Acetone	2.20	43	14932	8.017 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061818\
Data File : VV006341.D
Acq On : 18 Jun 2018 15:11
Operator : SY/MD
Sample : J3514-02
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KF9

Quant Time: Jun 19 02:08:55 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 19 02:03:29 2018
Response via : Initial Calibration

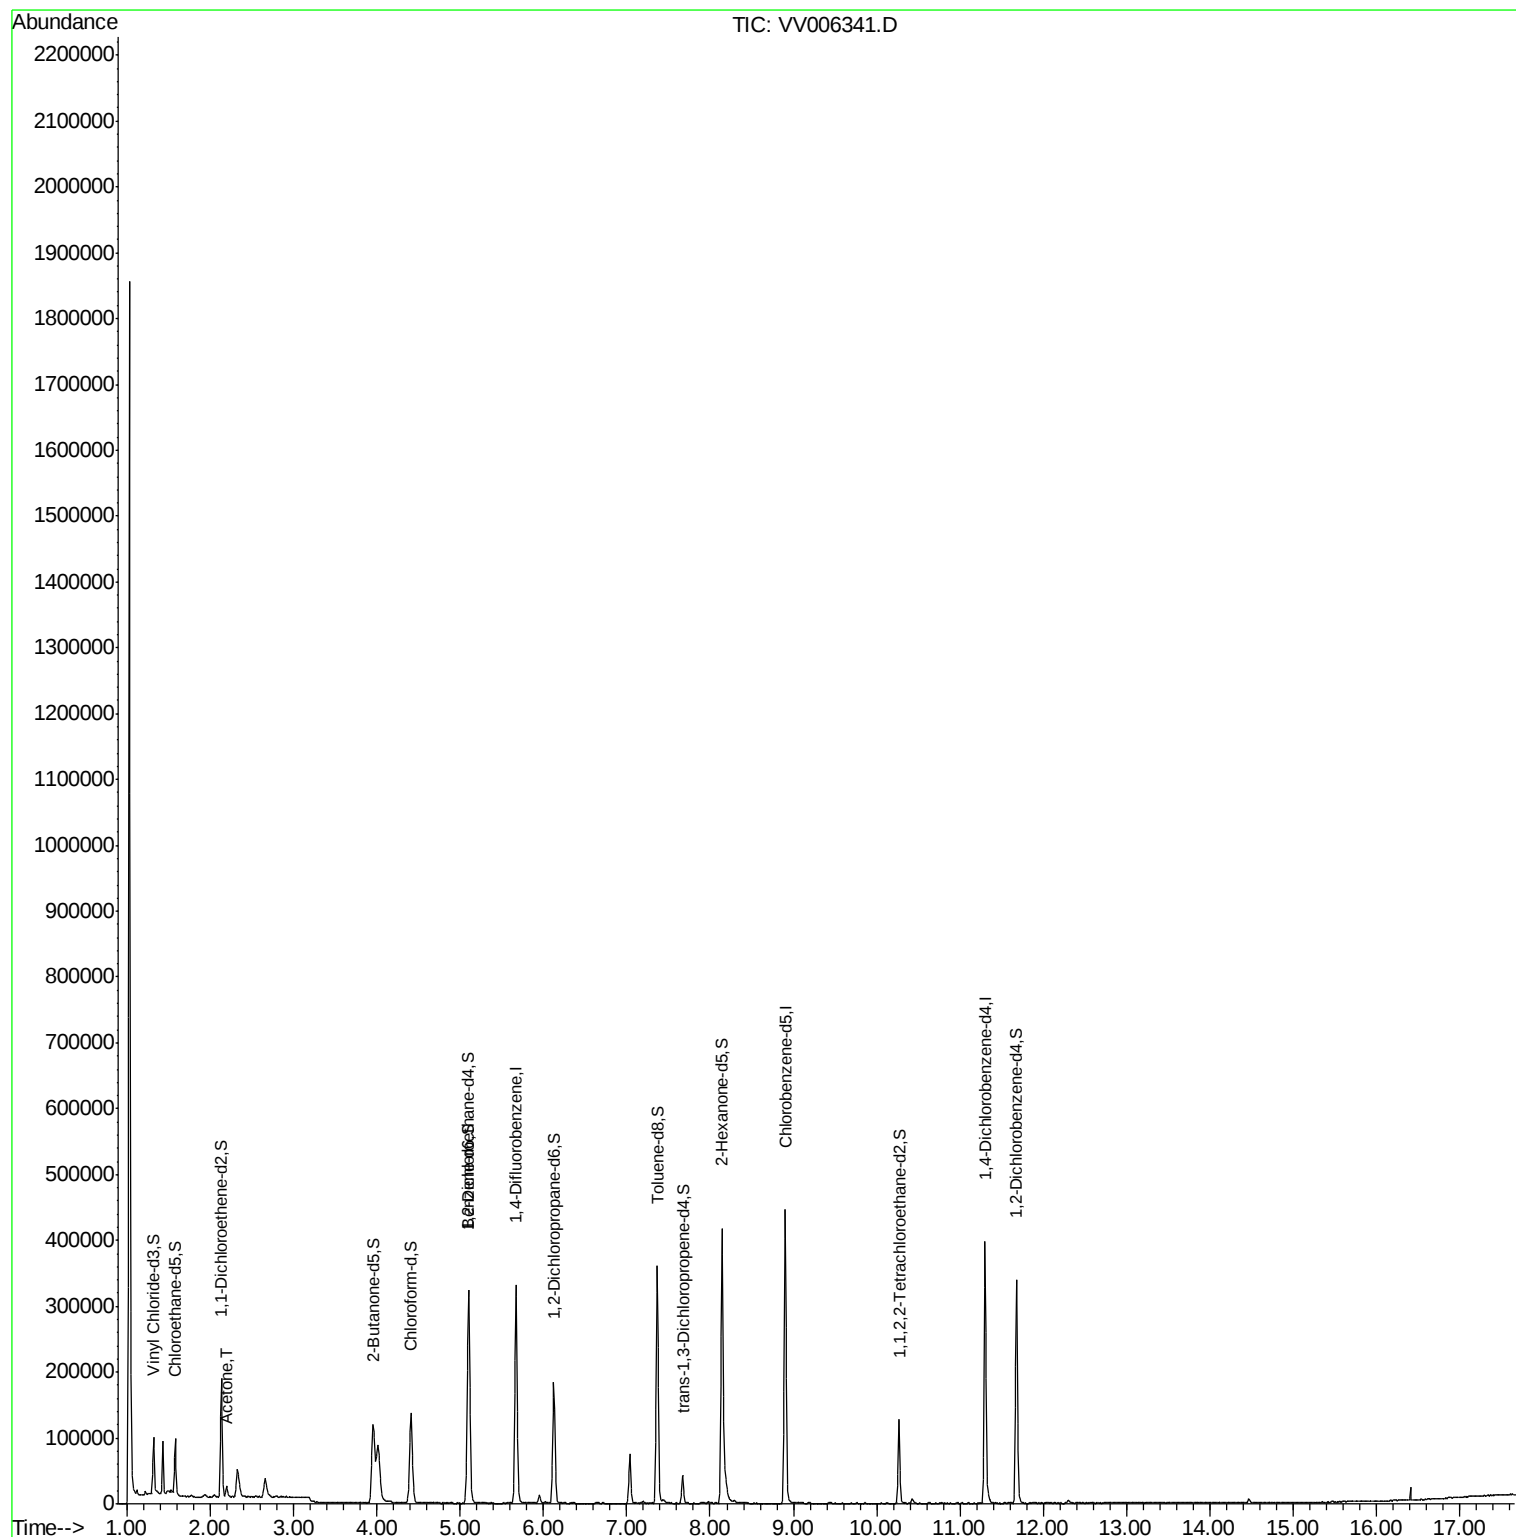

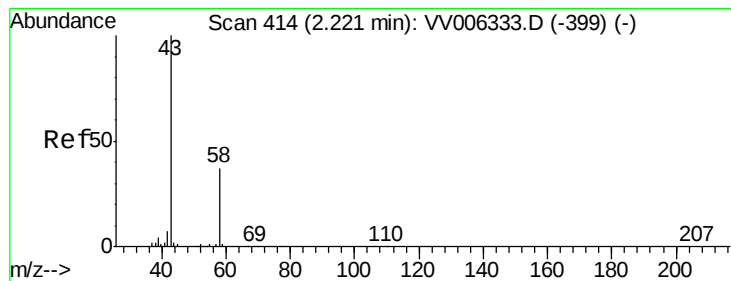

#13
 Acetone
 Concen: 8.017 ug/L
 RT: 2.20 min Scan# 406
 Delta R.T. -0.03 min
 Lab File: VV006341.D
 Acq: 18 Jun 2018 15:11

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KF9

Tot Ion: 43 Resp: 14932
 Ion Ratio Lower Upper
 43 100
 58 35.2 0.0 67.4

