

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061818\
 Data File : VV006343.D
 Acq On : 18 Jun 2018 16:05
 Operator : SY/MD
 Sample : J3514-04
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KG1

Quant Time: Jun 19 02:13:16 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 19 02:03:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	300495	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	273920	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	120228	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	65936	4.02	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.40%
7) Chloroethane-d5	1.58	69	58626	4.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.20%
11) 1,1-Dichloroethene-d2	2.13	63	90634	2.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.80%#
20) 2-Butanone-d5	3.95	46	197171	56.58	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.16%
24) Chloroform-d	4.41	84	140140	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.20%
26) 1,2-Dichloroethane-d4	5.09	65	73110	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.20%
32) Benzene-d6	5.11	84	287234	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.20%
36) 1,2-Dichloropropane-d6	6.12	67	91412	4.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.40%
41) Toluene-d8	7.37	98	256128	4.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.60%
43) trans-1,3-Dichloropropene-	7.67	79	24990	2.82	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	56.40%
46) 2-Hexanone-d5	8.14	63	143020	37.41	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.82%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	61986	4.32	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	100444	4.82	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.40%


Target Compounds					Ovalue
13) Acetone	2.19	43	12007	6.358 ug/L	92




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061818\
Data File : VV006343.D
Acq On : 18 Jun 2018 16:05
Operator : SY/MD
Sample : J3514-04
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KG1

Quant Time: Jun 19 02:13:16 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 19 02:03:29 2018
Response via : Initial Calibration

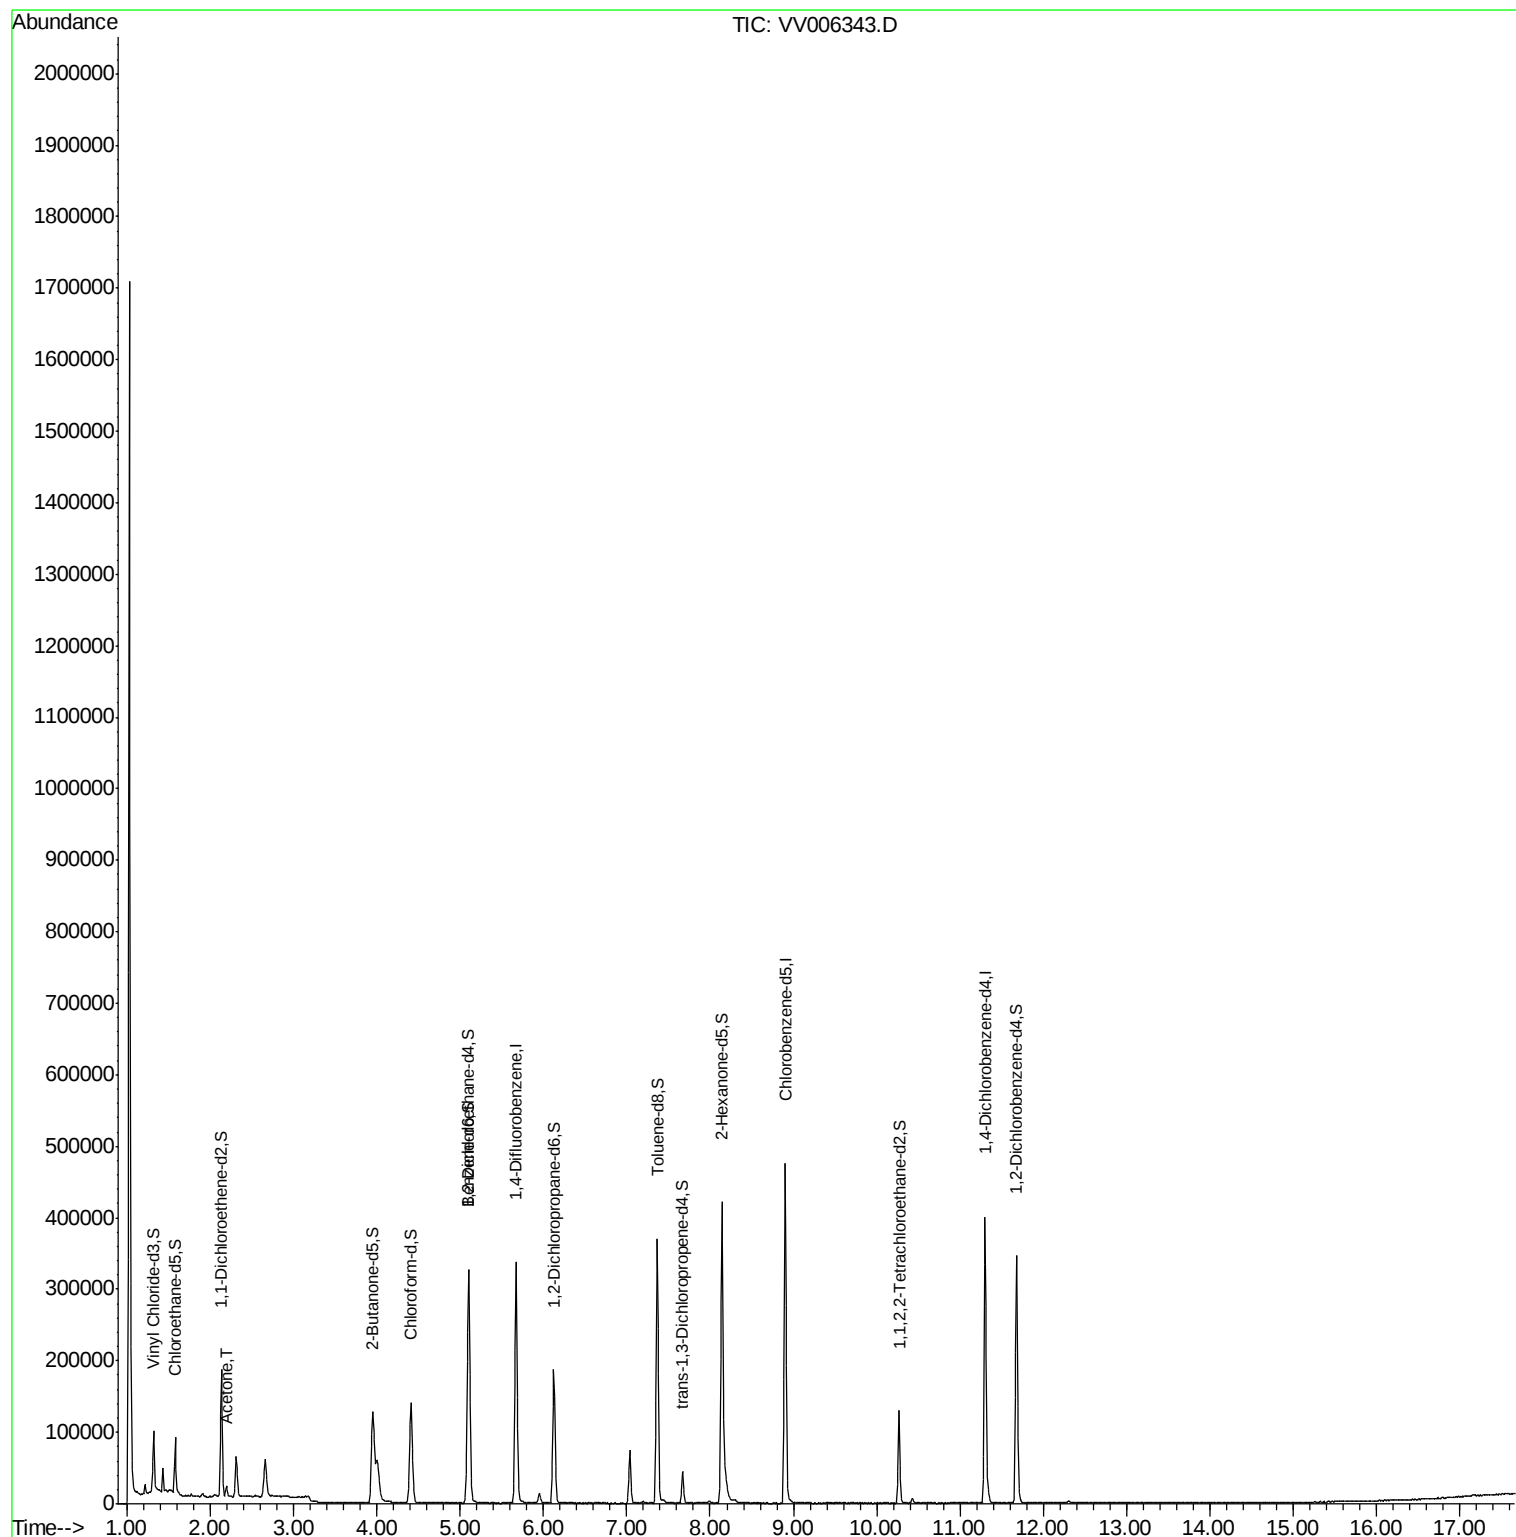

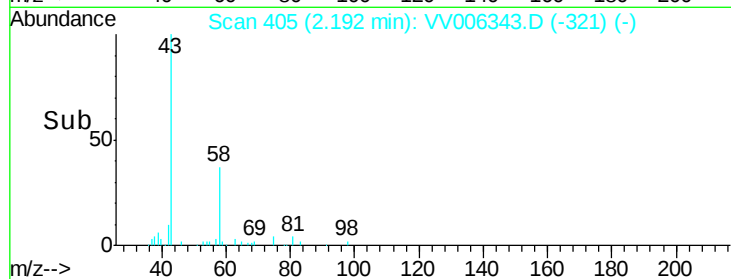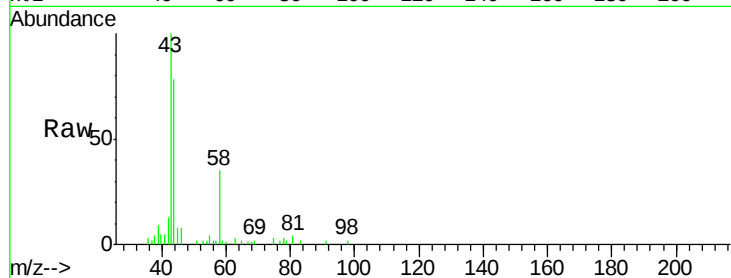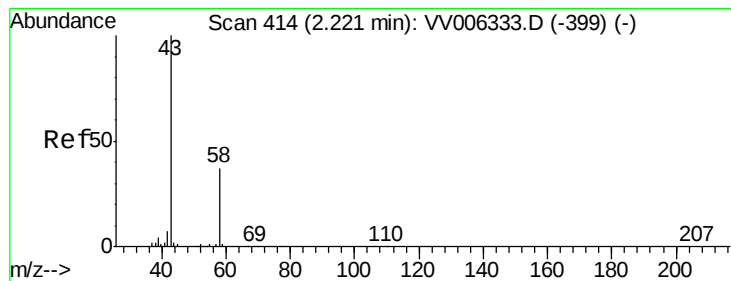

#13

Acetone

Concen: 6.358 ug/L

RT: 2.19 min Scan# 405

Delta R.T. -0.03 min

Lab File: VV006343.D

Acq: 18 Jun 2018 16:05

Instrument :

MSVOA_V

ClientSampleId :

C0KG1

Tot Ion: 43 Resp: 12007

Ion Ratio Lower Upper

43 100

58 38.3 0.0 67.4

