


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061818\
Data File : VV006332.D
Acq On : 18 Jun 2018 09:18
Operator : SY/MD
Sample : BFB74
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB74

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Jun 22 23:56:13 2018

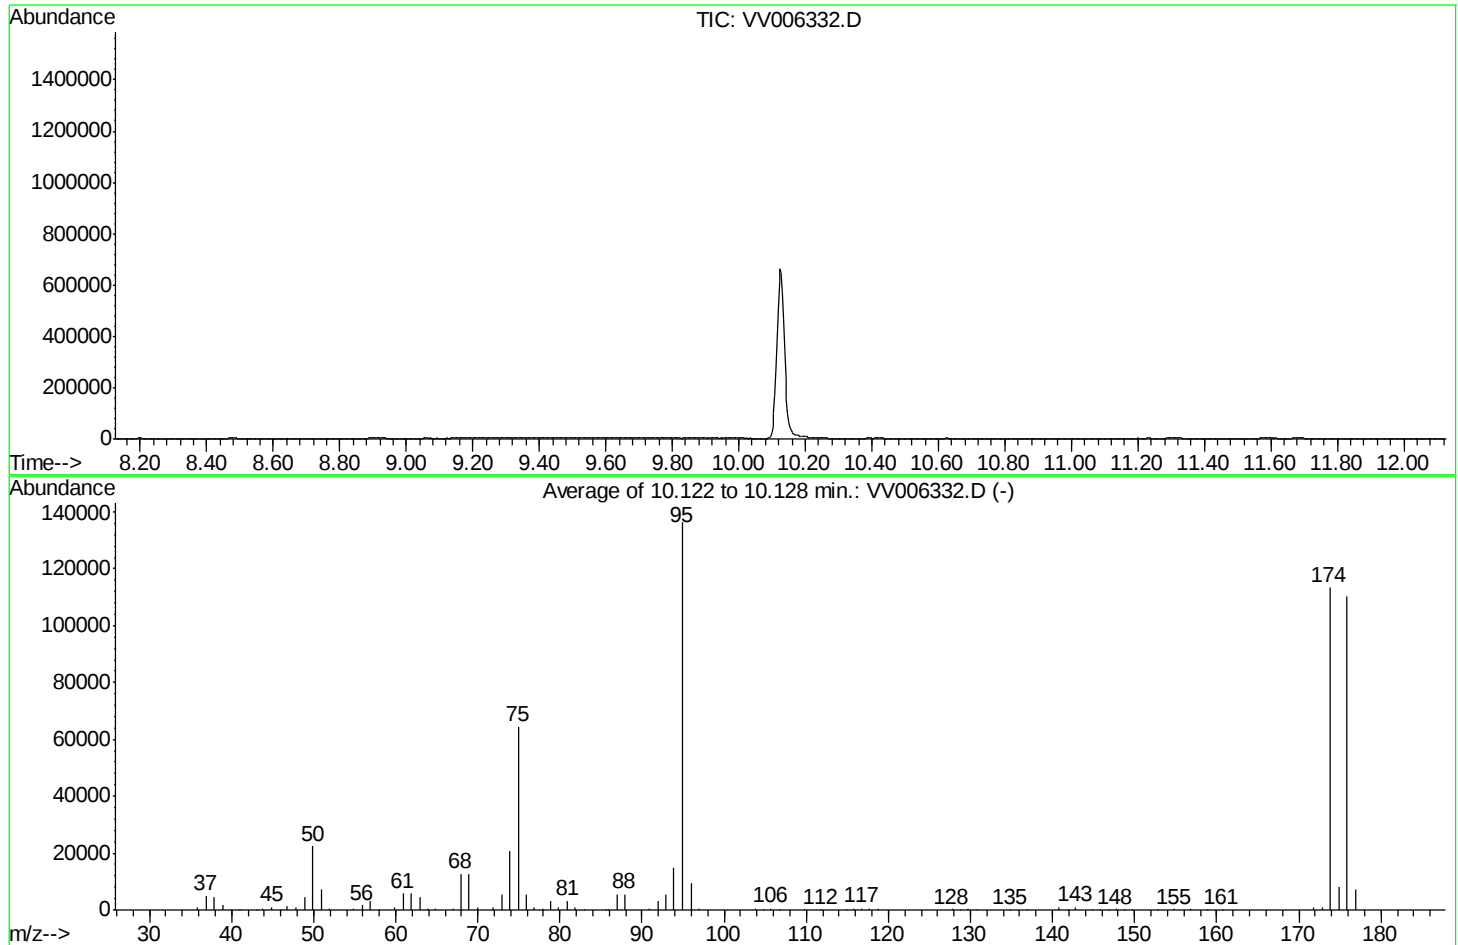

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	22378	PASS
75	95	30	80	47.3	64496	PASS
95	95	100	100	100.0	136314	PASS
96	95	5	9	6.8	9316	PASS
173	174	0.00	2	0.9	966	PASS
174	95	50	120	83.1	113301	PASS
175	174	5	9	7.3	8296	PASS
176	174	95	101	97.4	110317	PASS
177	176	5	9	6.6	7334	PASS

Scan 2858 (10.080 min): VV006332.D
BFB74

m/z	Abundance
35.90	1173.0
37.80	414.0
39.80	163.0
43.80	619.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
35.90	2106.0
36.90	4841.0
37.90	4958.0
38.90	1941.0
39.90	223.0
40.80	146.0
43.00	143.0
43.90	1151.0
44.90	952.0
45.90	129.0
46.80	1372.0
47.80	751.0
48.90	4638.0
49.90	22000.0
50.90	6932.0
51.90	287.0
54.90	436.0
55.90	1698.0
56.90	3142.0
57.90	132.0
59.90	1076.0
60.90	5660.0
61.90	5420.0
62.90	4412.0
63.90	506.0
64.90	625.0
67.00	342.0
67.90	12359.0
68.90	12398.0
69.90	1097.0
71.90	775.0
72.90	4967.0
73.90	20520.0
74.90	62696.0
75.90	5370.0
76.90	882.0
78.00	476.0
78.90	3076.0
79.80	1035.0
80.90	3185.0
81.80	760.0
82.90	110.0
85.90	194.0
86.90	5259.0
87.90	5260.0
90.80	514.0
91.90	3168.0
92.90	5241.0
93.90	14437.0
94.90	130480.0
96.00	8940.0
97.00	248.0
103.80	419.0
104.80	183.0
105.80	433.0
106.70	145.0
115.70	471.0
116.80	657.0
117.80	400.0
118.80	553.0
127.80	365.0
128.70	200.0
129.70	353.0
130.80	175.0
134.90	168.0
136.90	155.0
140.80	915.0
141.80	108.0
142.80	1077.0
144.80	150.0
145.80	135.0
147.70	289.0
148.70	105.0
149.70	122.0
154.80	335.0
156.80	232.0
158.80	154.0
171.80	742.0
172.90	964.0
173.80	106552.0
174.90	7881.0
175.80	103296.0
176.90	7018.0
177.80	156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
35.90	2146.0
36.90	5219.0
37.90	5073.0
38.90	1972.0
39.90	255.0
40.90	137.0
43.00	146.0
43.90	1210.0
44.90	1023.0
45.90	136.0
46.80	1536.0
47.80	777.0
48.90	4899.0
49.90	23128.0
50.90	7252.0
51.90	358.0
54.90	414.0
55.90	1835.0
56.90	3270.0
57.90	148.0
59.90	1174.0
60.90	5952.0
61.90	5913.0
62.90	4626.0
63.90	501.0
64.90	614.0
67.00	373.0
67.90	13320.0
68.90	13131.0
69.90	1105.0
71.90	811.0
72.90	5458.0
73.90	21592.0
74.90	66552.0
75.90	5712.0
76.90	897.0
78.00	481.0
78.80	3300.0
79.80	1129.0
80.90	3368.0
81.80	804.0
82.90	112.0
85.90	171.0
86.90	5728.0
87.90	5801.0
90.90	572.0
91.90	3364.0
92.90	5581.0
93.90	15389.0
94.90	141248.0
96.00	9689.0
97.00	299.0
103.80	448.0
104.70	180.0
105.80	480.0
106.70	151.0
109.70	107.0
111.80	106.0
115.80	507.0
116.80	702.0
117.80	435.0
118.80	649.0
127.80	442.0
128.70	193.0
129.70	399.0
130.80	189.0
134.90	197.0
136.90	191.0
140.80	1076.0
141.80	101.0
142.80	1109.0
144.80	168.0
145.80	138.0
146.80	105.0
147.70	302.0
148.70	109.0
149.70	148.0
152.70	117.0
154.80	393.0
156.80	257.0
158.80	176.0
160.70	118.0
171.90	856.0
172.90	1010.0
173.80	116928.0
174.90	8596.0
175.80	113992.0
176.90	7648.0
177.90	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
35.90	1994.0
36.90	4948.0
37.90	4913.0
38.90	1876.0
39.90	252.0
41.00	135.0
43.00	157.0
43.90	1210.0
44.90	1030.0
46.00	114.0
46.80	1479.0
47.80	738.0
48.90	4671.0
49.90	22008.0
50.90	6812.0
51.90	365.0
54.90	369.0
55.90	1739.0
56.90	3143.0
57.90	142.0
59.90	1128.0
60.90	5733.0
61.90	5734.0
62.90	4443.0
63.90	448.0
64.90	554.0
67.00	361.0
67.90	12706.0
68.90	12619.0
69.90	1056.0
71.90	747.0
72.90	5400.0
73.90	20680.0
74.90	64240.0
75.90	5480.0
76.90	827.0
77.90	489.0
78.80	3157.0
79.80	1082.0
80.90	3238.0
81.80	779.0
82.90	104.0
85.60	190.0
86.90	5815.0
87.80	5770.0
90.90	545.0
91.90	3250.0
92.90	5397.0
93.90	15093.0
94.90	137216.0
96.00	9321.0
97.00	299.0
103.70	468.0
104.70	163.0
105.70	471.0
106.80	157.0
109.70	109.0
114.90	106.0
115.80	473.0
116.80	689.0
117.70	413.0
118.80	677.0
127.80	442.0
128.80	157.0
129.70	422.0
130.80	168.0
134.80	213.0
136.90	206.0
140.80	1134.0
142.80	1033.0
144.80	182.0
145.80	133.0
146.80	116.0
147.70	281.0
149.70	133.0
152.70	133.0
154.80	376.0
156.80	263.0
158.80	156.0
160.70	115.0
171.90	880.0
172.90	924.0
173.80	116424.0
174.90	8413.0
175.80	113664.0
176.90	7336.0
177.90	189.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74