


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV061819\
Data File : VV011563.D
Acq On : 18 Jun 2019 08:33
Operator : SY/MD
Sample : BFB50
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB50

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Jun 18 11:44:39 2019

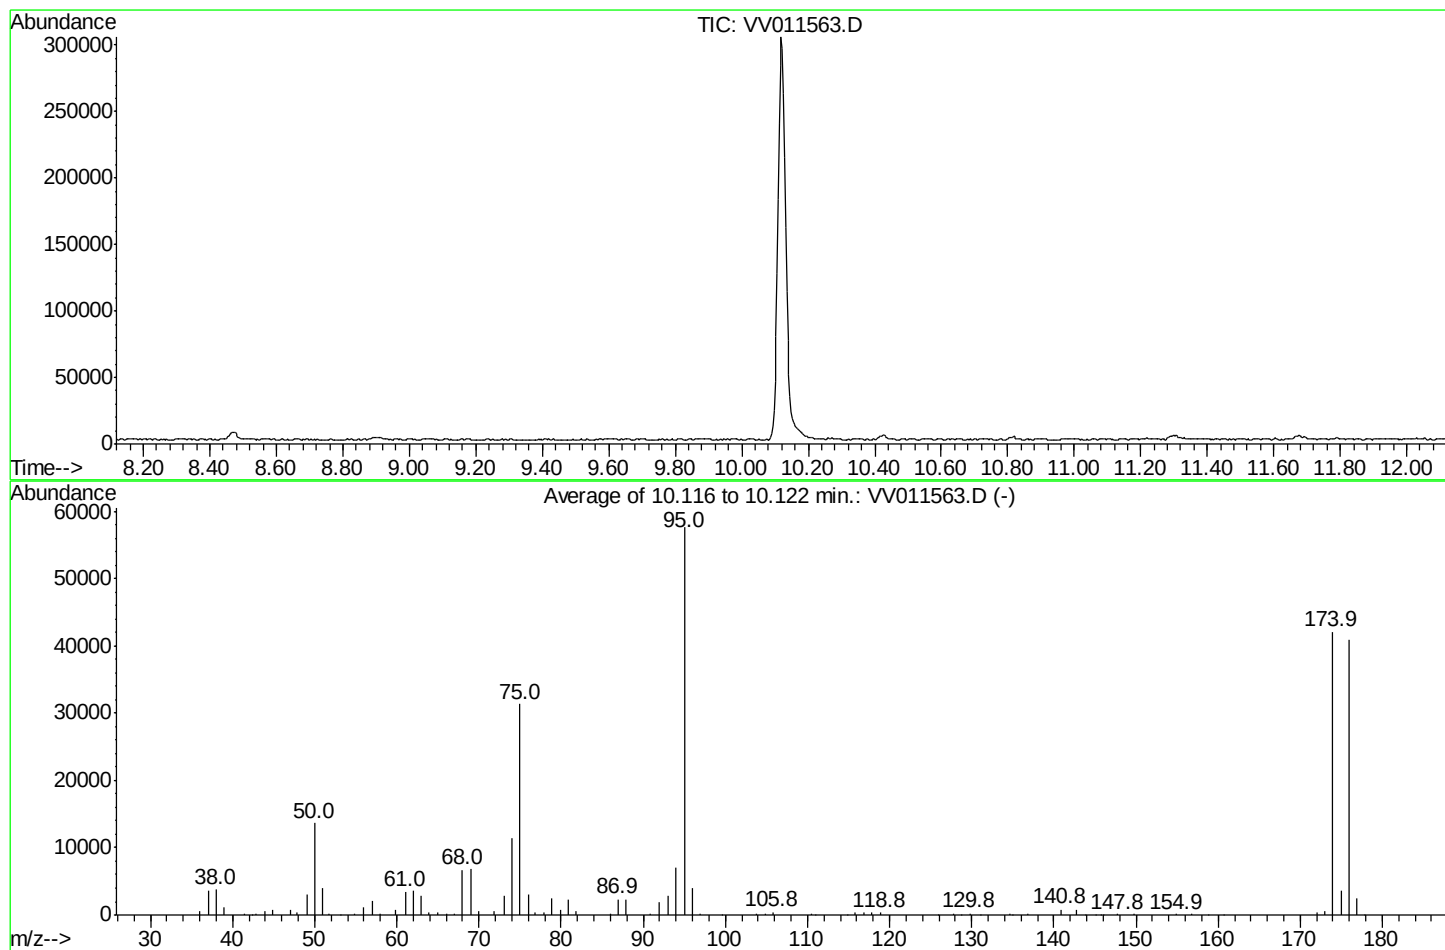

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	13624	PASS
75	95	30	80	54.4	31341	PASS
95	95	100	100	100.0	57613	PASS
96	95	5	9	6.8	3911	PASS
173	174	0.00	2	1.2	521	PASS
174	95	50	120	73.1	42141	PASS
175	174	5	9	8.5	3585	PASS
176	174	95	101	97.1	40912	PASS
177	176	5	9	6.3	2572	PASS

Scan 2794 (10.074 min): VV011563.D
BFB50

m/z	Abundance
35.40	171.0
37.30	117.0
38.00	114.0
38.80	110.0
39.90	1738.0
41.00	134.0
42.90	106.0
43.90	474.0
49.70	126.0
50.30	102.0
51.10	112.0
56.60	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

m/z	Abundance
35.90	641.0
37.00	3581.0
38.00	3811.0
39.00	1303.0
39.90	1756.0
41.50	104.0
42.80	204.0
44.00	917.0
44.90	673.0
47.00	838.0
47.80	411.0
49.00	3055.0
50.00	13576.0
51.00	4166.0
51.80	150.0
54.90	261.0
55.90	1017.0
56.90	1945.0
58.00	157.0
59.90	674.0
61.00	3453.0
62.00	3561.0
63.00	2900.0
63.90	278.0
64.90	290.0
66.00	131.0
67.00	211.0
68.00	6782.0
69.00	6701.0
70.00	540.0
71.90	447.0
73.00	2856.0
74.00	11380.0
75.00	30872.0
76.00	2910.0
76.90	352.0
78.00	255.0
78.90	2413.0
79.90	843.0
80.90	2308.0
81.80	565.0
86.00	165.0
86.90	2223.0
87.90	2302.0
90.80	252.0
91.90	1950.0
93.00	2818.0
94.00	6983.0
95.00	55688.0
96.00	3799.0
97.00	128.0
99.60	122.0
103.80	282.0
104.80	176.0
105.80	317.0
110.50	107.0
111.00	111.0
114.80	122.0
115.80	269.0
116.90	347.0
117.80	256.0
118.90	378.0
127.80	254.0
128.70	106.0
129.70	246.0
135.00	165.0
136.90	121.0
140.80	875.0
142.80	718.0
143.80	102.0
146.00	129.0
147.80	135.0
149.80	157.0
155.00	151.0
156.70	127.0
172.00	392.0
173.90	39368.0
175.00	3375.0
175.90	38360.0
176.90	2509.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

m/z	Abundance
35.90	615.0
37.00	3649.0
38.00	4018.0
39.00	1390.0
39.90	1646.0
41.40	113.0
42.80	230.0
44.00	1008.0
44.90	720.0
47.00	895.0
47.90	467.0
49.00	3139.0
50.00	14081.0
51.00	4330.0
51.70	150.0
54.90	287.0
55.90	1141.0
57.00	2075.0
58.00	152.0
59.90	734.0
61.00	3631.0
62.00	3718.0
63.00	3033.0
63.90	304.0
64.90	327.0
66.00	127.0
67.10	199.0
68.00	7063.0
69.00	7085.0
70.00	625.0
71.80	507.0
73.00	3016.0
74.00	11884.0
75.00	32312.0
76.00	3208.0
76.80	399.0
77.90	324.0
78.90	2647.0
79.90	885.0
80.90	2415.0
81.90	643.0
86.00	160.0
86.90	2397.0
87.90	2435.0
90.80	285.0
91.90	2019.0
93.00	2879.0
94.00	7352.0
95.00	59664.0
96.00	4075.0
97.00	144.0
103.80	285.0
104.80	212.0
105.70	405.0
110.50	124.0
111.00	101.0
115.80	335.0
116.90	355.0
117.80	293.0
118.90	400.0
127.80	276.0
128.70	107.0
129.80	272.0
131.10	106.0
134.70	165.0
136.80	155.0
140.90	842.0
142.80	822.0
146.00	110.0
147.80	169.0
149.80	154.0
155.00	165.0
156.80	138.0
158.80	105.0
160.70	110.0
172.00	498.0
173.00	768.0
173.90	43480.0
175.00	3710.0
175.90	42080.0
176.90	2635.0
177.80	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

m/z	Abundance
35.90	598.0
37.00	3584.0
38.00	3870.0
39.00	1343.0
39.90	1596.0
40.80	127.0
41.40	125.0
42.30	143.0
42.80	210.0
43.90	1004.0
44.90	660.0
47.00	833.0
47.90	466.0
49.00	3011.0
50.00	13216.0
51.00	3957.0
51.80	163.0
53.10	120.0
54.90	276.0
56.00	1161.0
57.00	2003.0
58.00	125.0
59.90	691.0
61.00	3433.0
62.00	3544.0
63.00	2800.0
63.90	306.0
64.90	388.0
66.00	116.0
67.00	171.0
68.00	6385.0
69.00	6696.0
70.00	664.0
71.80	519.0
73.00	2865.0
74.00	11076.0
75.00	30840.0
76.00	3169.0
76.90	367.0
77.90	347.0
78.90	2646.0
79.90	834.0
80.90	2280.0
81.90	643.0
86.00	115.0
86.90	2329.0
87.90	2189.0
90.90	277.0
91.90	1939.0
92.90	2799.0
94.00	7001.0
95.00	57488.0
96.00	3861.0
96.90	143.0
103.70	268.0
104.90	219.0
105.80	429.0
110.50	119.0
115.80	353.0
116.90	330.0
117.80	329.0
118.80	353.0
125.90	105.0
127.80	257.0
129.70	283.0
130.90	116.0
134.70	153.0
136.80	154.0
140.80	739.0
142.80	883.0
145.10	118.0
145.70	116.0
147.80	196.0
149.80	139.0
154.90	128.0
156.70	140.0
160.80	125.0
172.00	511.0
172.90	795.0
173.90	43576.0
175.00	3671.0
175.90	42296.0
176.90	2572.0
177.80	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50