

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061822\
 Data File : VW026425.D
 Acq On : 18 Jun 2022 15:11
 Operator : SY/MD
 Sample : N3256-08DL 2X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH2DL

Quant Time: Jun 20 01:29:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 20 01:25:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.626	114	267854	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	232046	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.256	152	117821	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	70456	3.028	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	60.600%
7) Chloroethane-d5	1.581	69	105949	5.792	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	115.800%
11) 1,1-Dichloroethene-d2	2.121	63	103054	2.579	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	51.600%#
20) 2-Butanone-d5	3.925	46	89096	39.247	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	78.500%
24) Chloroform-d	4.365	84	151753	4.450	ug/L	0.01
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
26) 1,2-Dichloroethane-d4	5.044	65	61410	4.257	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
32) Benzene-d6	5.060	84	308595	4.974	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.400%
36) 1,2-Dichloropropane-d6	6.079	67	87228	4.818	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.400%
41) Toluene-d8	7.323	98	303382	5.363	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.200%
43) trans-1,3-Dichloroprop...	7.629	79	19906	3.390	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	67.800%
46) 2-Hexanone-d5	8.095	63	99246	55.959	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.920%
56) 1,1,2,2-Tetrachloroeth...	10.227	84	46403	4.160	ug/L	0.01
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.200%
66) 1,2-Dichlorobenzene-d4	11.628	152	94749	5.221	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.400%
Target Compounds						
					Qvalue	
3) Chloromethane	1.230	50	88030	3.958	ug/L #	68
8) Chloroethane	1.500	64	370172	25.790	ug/L #	50
10) 1,1,2-Trichloro-1,2,2-...	2.127	101	2594	0.140	ug/L #	47
12) 1,1-Dichloroethene	2.130	96	2296	0.136	ug/L #	1
13) Acetone	2.143	43	540359	307.148	ug/L	57
14) Carbon disulfide	2.314	76	13706	0.328	ug/L	99
15) Methyl Acetate	2.545	43	14546083	3445.977	ug/L #	48
16) Methylene chloride	2.462	84	273827	12.683	ug/L #	5
17) Methyl tert-butyl Ether	2.780	73	5667	0.195	ug/L #	1
19) 1,1-Dichloroethane	3.169	63	23576	0.753	ug/L #	1
21) 2-Butanone	3.864	43	71519	31.418	ug/L #	68
22) cis-1,2-Dichloroethene	3.937	96	2618	0.158	ug/L #	80
25) Chloroform	4.420	83	205175	6.043	ug/L #	39
27) 1,2-Dichloroethane	5.111	62	1719	0.111	ug/L #	1
29) 1,1,1-Trichloroethane	4.606	97	669	0.026	ug/L #	1
30) Cyclohexane	4.690	56	2181853	113.772	ug/L	89
33) Benzene	5.108	78	387697	6.517	ug/L	100
34) Trichloroethene	5.947	95	40080	2.468	ug/L #	19
35) Methylcyclohexane	6.137	83	1934439	86.101	ug/L	91

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
 Data File : VV026425.D
 Acq On : 18 Jun 2022 15:11
 Operator : SY/MD
 Sample : N3256-08DL 2X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH2DL

Quant Time: Jun 20 01:29:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 20 01:25:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


37) 1,2-Dichloropropane	6.137	63	20274	1.303	ug/L #	69
38) Bromodichloromethane	6.571	83	52309	2.772	ug/L #	26
39) cis-1,3-Dichloropropene	6.995	75	2053	0.116	ug/L #	1
40) 4-Methyl-2-pentanone	7.243	43	32615	5.701	ug/L #	52
44) trans-1,3-Dichloropropene	7.400	75	316303	22.302	ug/L #	1
45) 1,1,2-Trichloroethane	7.793	97	173276	16.966	ug/L #	23
47) Tetrachloroethene	7.982	164	1558	0.130	ug/L	91
48) 2-Hexanone	8.150	43	59064	14.409	ug/L #	31
49) Dibromochloromethane	7.982	129	1621	0.143	ug/L #	9
55) Styrene	9.577	104	2211111	55.588	ug/L #	1
60) Isopropylbenzene	9.937	105	3875038	61.693	ug/L #	87
61) 1,2,3-Trichloropropane	10.358	75	88329	11.553	ug/L #	42
62) 1,3,5-Trimethylbenzene	10.358	105	586084	11.759	ug/L #	1
63) 1,2,4-Trimethylbenzene	11.092	105	716061	14.515	ug/L #	30
68) 1,2-Dibromo-3-chloropr...	12.413	75	40932	30.224	ug/L #	3
71) Naphthalene	13.503	128	12309862	538.664	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
Data File : VV026425.D
Acq On : 18 Jun 2022 15:11
Operator : SY/MD
Sample : N3256-08DL 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH2DL

Quant Time: Jun 20 01:29:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 20 01:25:22 2022
Response via : Initial Calibration




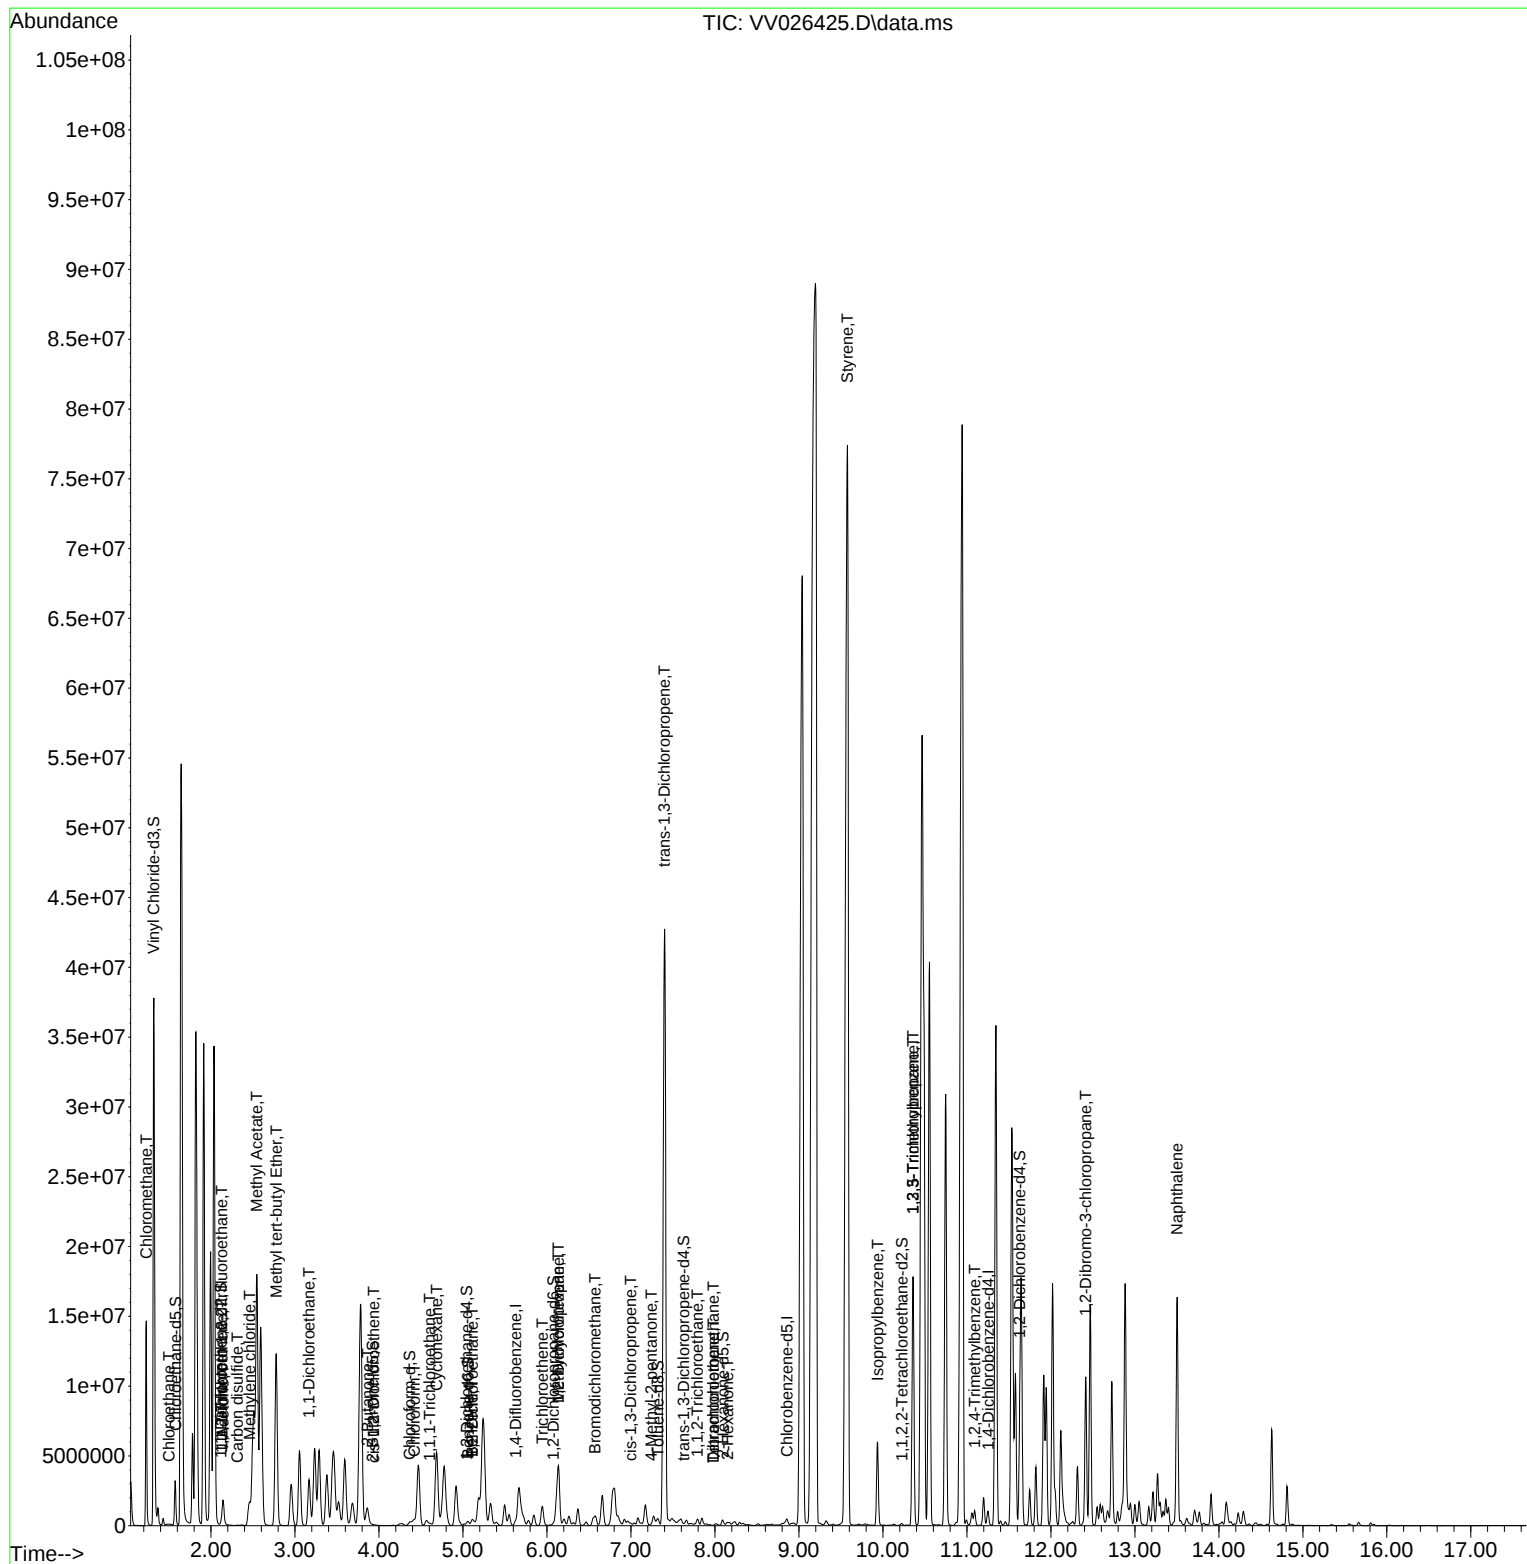


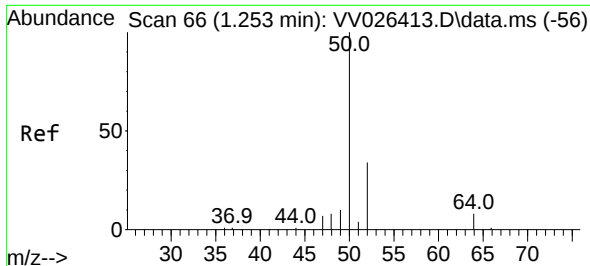

#3
Chloromethane
Concen: 3.958 ug/L
RT: 1.230 min Scan# 51
Delta R.T. -0.022 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11




Instrument :
MSVOA_V
ClientSampleId :
C0AH2DL


Tgt Ion: 50 Resp: 88030
Ion Ratio Lower Upper
50 100
52 15.8 23.7 44.1#

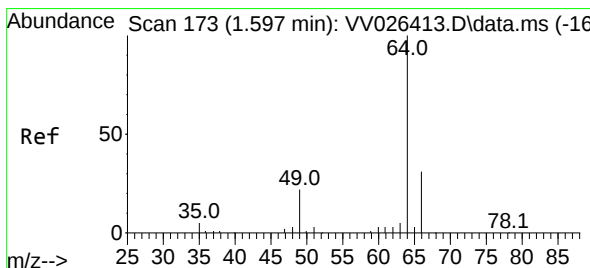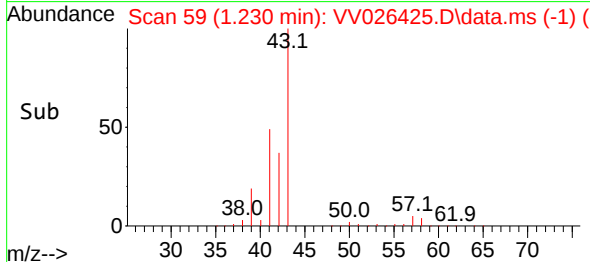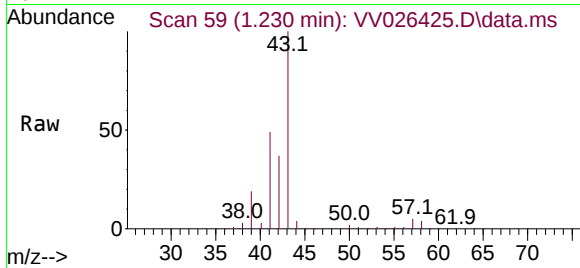

#8
Chloroethane
Concen: 25.790 ug/L
RT: 1.500 min Scan# 143
Delta R.T. -0.096 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11

Tgt Ion: 64 Resp: 370172
Ion Ratio Lower Upper
64 100
66 5.5 24.1 44.7#


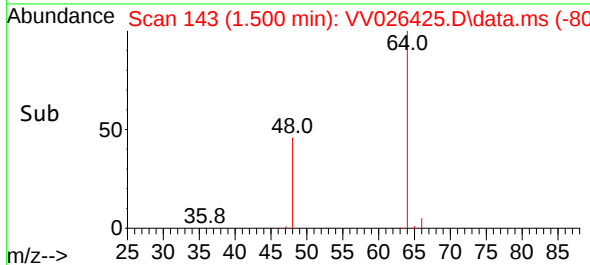

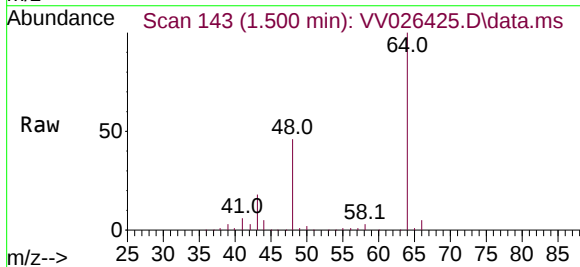




#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.140 ug/L
 RT: 2.127 min Scan# 338
 Delta R.T. 0.000 min
 Lab File: VV026425.D
 Acq: 18 Jun 2022 15:11




Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH2DL


Tgt Ion:101 Resp: 2594
 Ion Ratio Lower Upper
 101 100
 85 88.4 35.3 52.9#
 151 35.1 56.8 85.2#

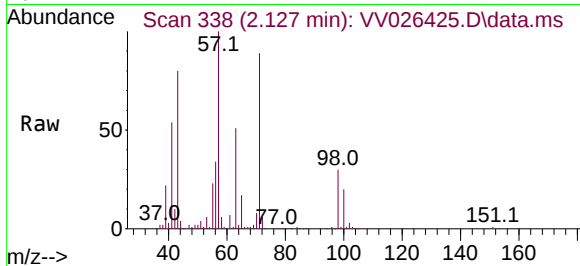

#12
 1,1-Dichloroethene
 Concen: 0.136 ug/L
 RT: 2.130 min Scan# 339
 Delta R.T. 0.000 min
 Lab File: VV026425.D
 Acq: 18 Jun 2022 15:11

Tgt Ion: 96 Resp: 2296
 Ion Ratio Lower Upper
 96 100
 61 527.1 117.1 217.5#
 63 3773.5 92.8 172.4#

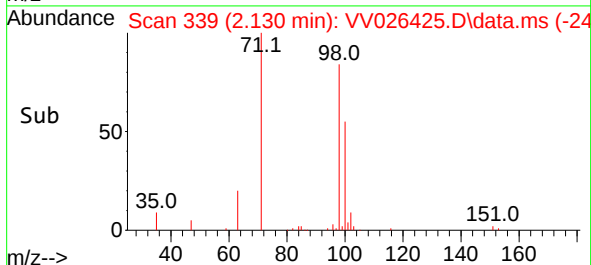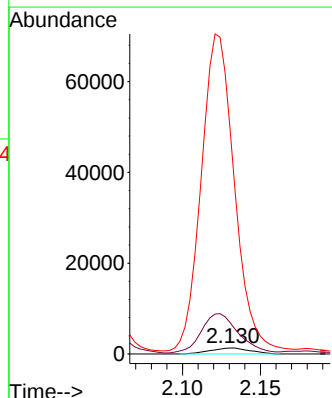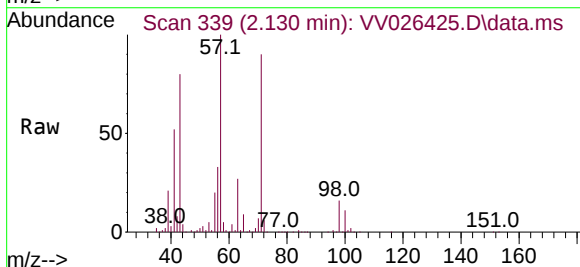



#13

Acetone

Concen: 307.148 ug/L

RT: 2.143 min Scan# 34

Delta R.T. -0.067 min

Lab File: VV026425.D

Acq: 18 Jun 2022 15:11

Instrument :

MSVOA_V

ClientSampleId :





C0AH2DL

Tgt Ion: 43 Resp: 540359

Ion Ratio Lower Upper

43 100

58 7.0 0.0 60.0

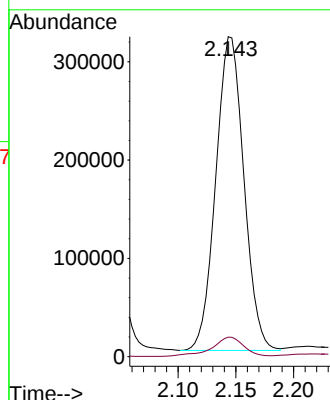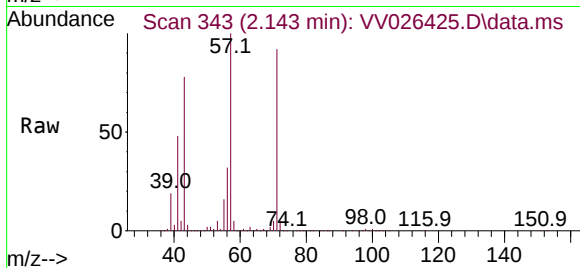

#14

Carbon disulfide

Concen: 0.328 ug/L

RT: 2.314 min Scan# 396

Delta R.T. 0.010 min

Lab File: VV026425.D




Acq: 18 Jun 2022 15:11


Tgt Ion: 76 Resp: 13706

Ion Ratio Lower Upper

76 100

78 9.8 7.7 11.5


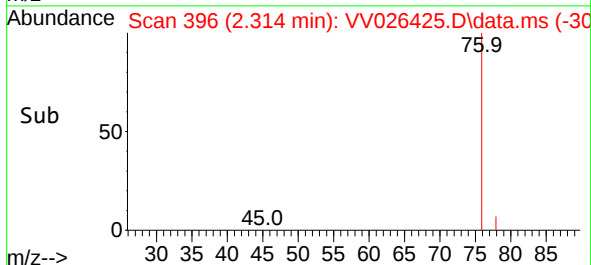
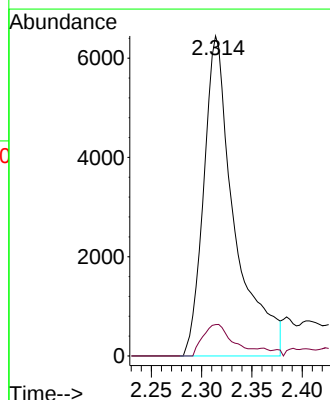
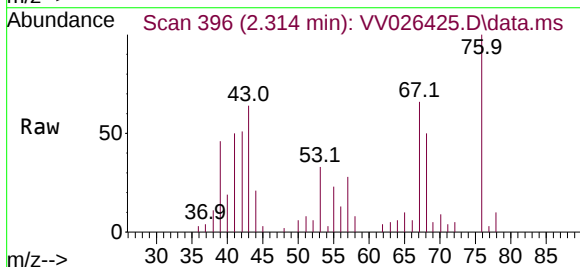




#15
Methyl Acetate
Concen: 3445.977 ug/L
RT: 2.545 min Scan# 415
Delta R.T. 0.090 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11




Instrument :
MSVOA_V
ClientSampleId :
C0AH2DL


Tgt Ion: 43 Resp:14546083
Ion Ratio Lower Upper
43 100
74 0.0 21.4 32.0#



#16
Methylene chloride
Concen: 12.683 ug/L
RT: 2.462 min Scan# 442
Delta R.T. -0.055 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11

Tgt Ion: 84 Resp: 273827
Ion Ratio Lower Upper
84 100
86 0.2 44.0 81.8#
49 1.5 77.3 143.7#


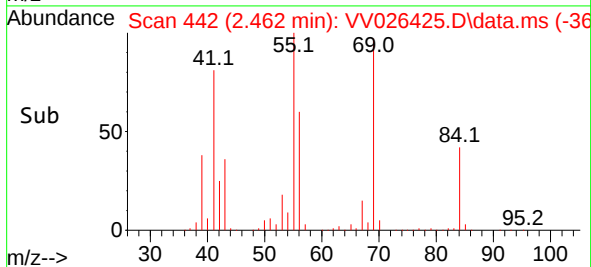

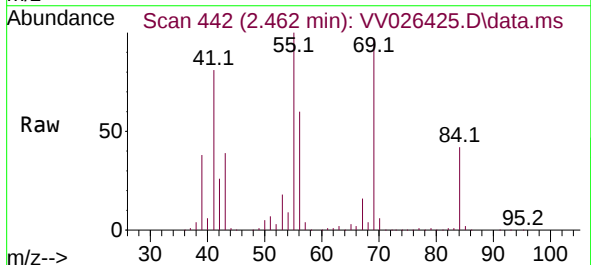




#17
Methyl tert-butyl Ether
Concen: 0.195 ug/L
RT: 2.780 min Scan# 541
Delta R.T. 0.000 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11




Instrument :
MSVOA_V
ClientSampleId :
C0AH2DL


Tgt Ion: 73 Resp: 5667
Ion Ratio Lower Upper
73 100
43 28460.7 13.0 19.6#
57 133490.0 17.6 26.4#

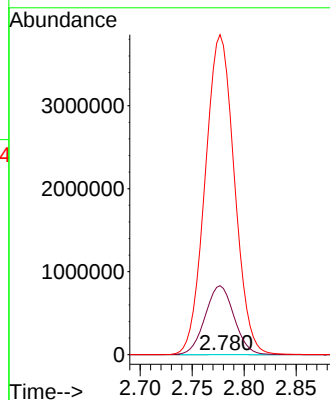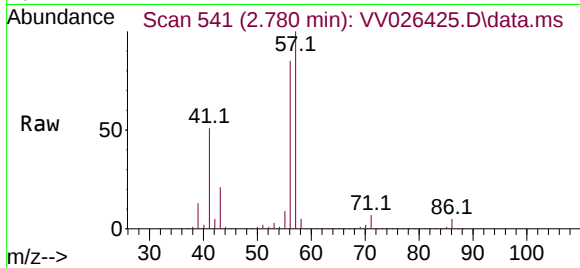

#19
1,1-Dichloroethane
Concen: 0.753 ug/L
RT: 3.169 min Scan# 662
Delta R.T. -0.029 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11

Tgt Ion: 63 Resp: 23576
Ion Ratio Lower Upper
63 100
65 189.1 22.3 41.3#
83 38.8 8.9 16.5#


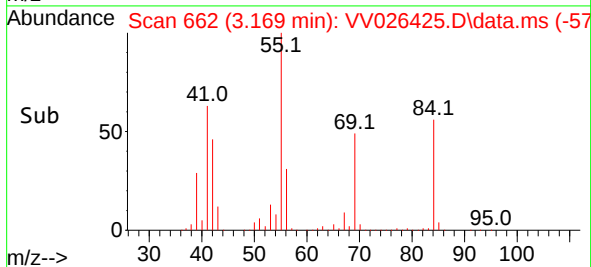
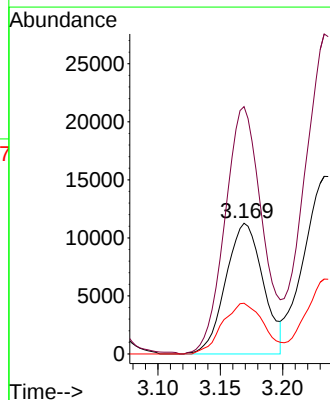
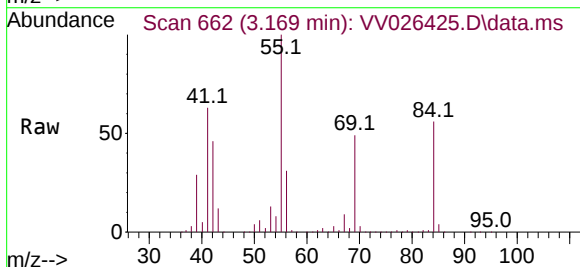


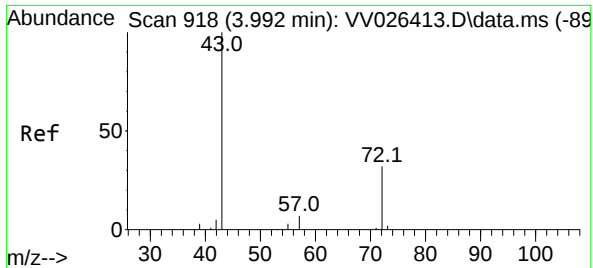

#21
2-Butanone
Concen: 31.418 ug/L
RT: 3.864 min Scan# 81
Delta R.T. -0.129 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11




Instrument :
MSVOA_V
ClientSampleId :
C0AH2DL


Tgt Ion: 43 Resp: 71519
Ion Ratio Lower Upper
43 100
72 9.1 12.7 38.0#

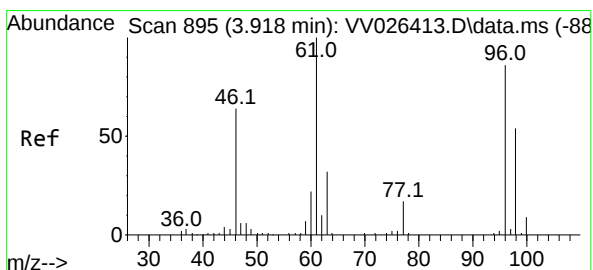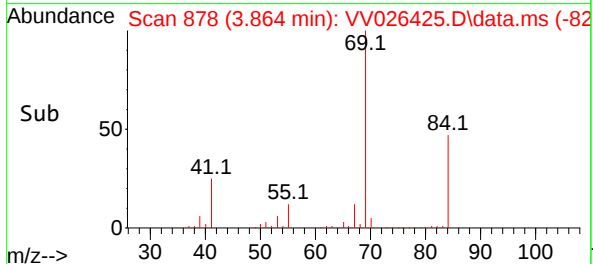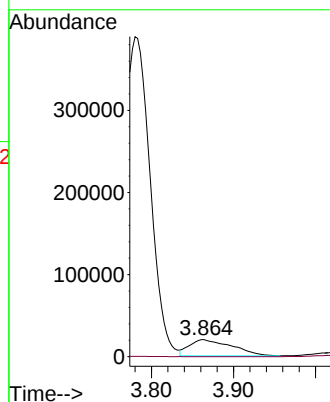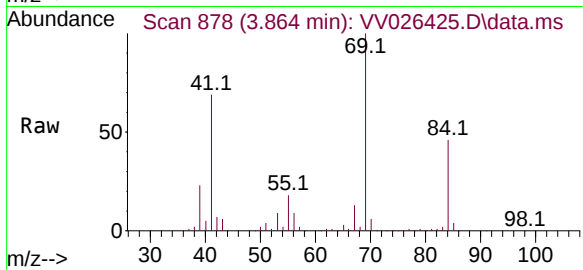

#22
cis-1,2-Dichloroethene
Concen: 0.158 ug/L
RT: 3.937 min Scan# 901
Delta R.T. 0.019 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11

Tgt Ion: 96 Resp: 2618
Ion Ratio Lower Upper
96 100
61 141.0 83.6 155.2
68 23.4 0.0 0.0#

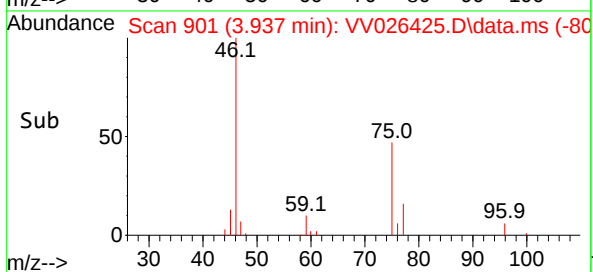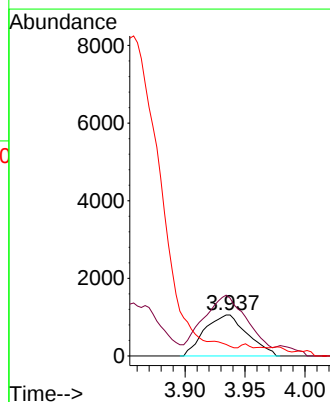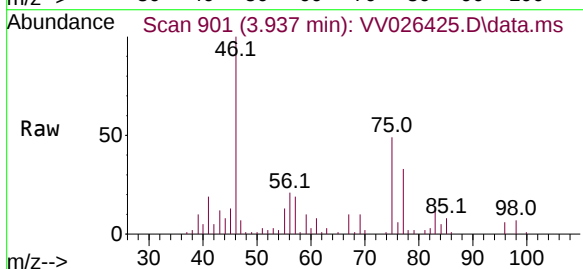

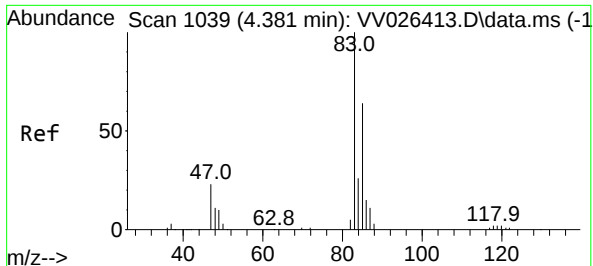

#25

Chloroform

Concen: 6.043 ug/L

RT: 4.420 min Scan# 1051

Delta R.T. 0.039 min

Lab File: VV026425.D

Acq: 18 Jun 2022 15:11

Instrument :

MSVOA_V

ClientSampleId :





C0AH2DL

Tgt Ion: 83 Resp: 205175

Ion Ratio Lower Upper

83 100

85 18.1 46.5 86.3#

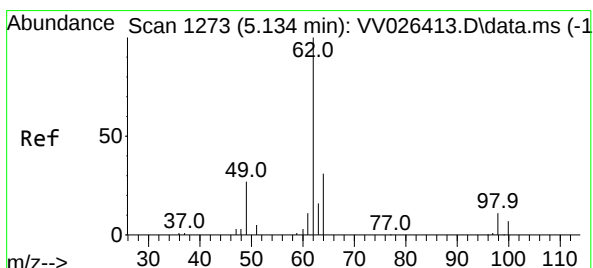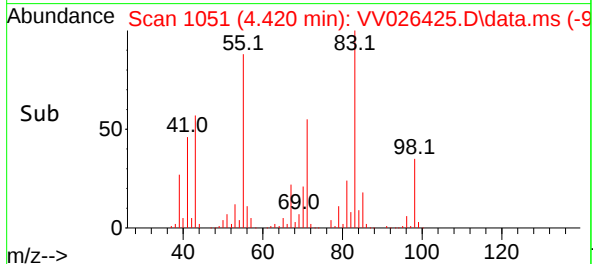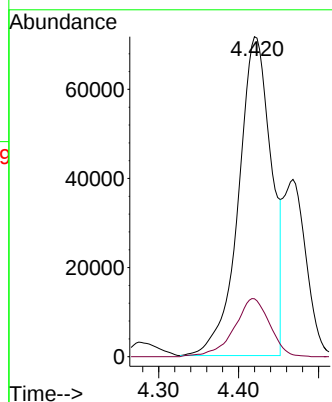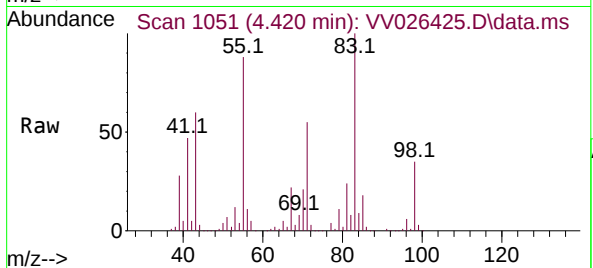

#27

1,2-Dichloroethane

Concen: 0.111 ug/L

RT: 5.111 min Scan# 1266

Delta R.T. -0.022 min

Lab File: VV026425.D




Acq: 18 Jun 2022 15:11


Tgt Ion: 62 Resp: 1719

Ion Ratio Lower Upper

62 100

98 507.0 8.6 13.0#

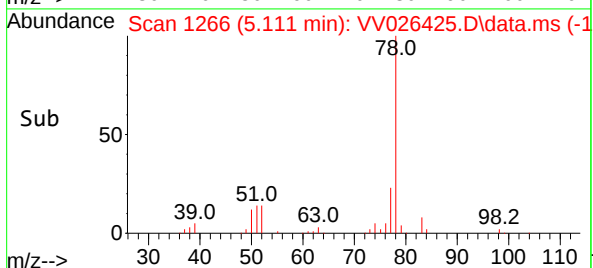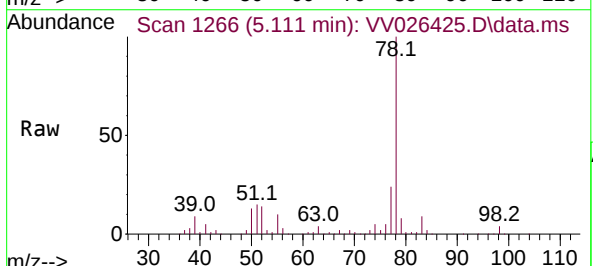



#29

1,1,1-Trichloroethane

Concen: 0.026 ug/L

RT: 4.606 min Scan# 1111

Delta R.T. -0.006 min

Lab File: VV026425.D

Acq: 18 Jun 2022 15:11

Instrument :

MSVOA_V

ClientSampleId :

C0AH2DL





Tgt Ion: 97 Resp: 669

Ion Ratio Lower Upper

97 100

99 445.6 50.3 75.5#

61 478.9 33.4 50.0#

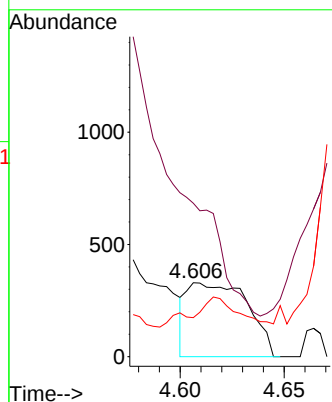

#30

Cyclohexane

Concen: 113.772 ug/L

RT: 4.690 min Scan# 1135

Delta R.T. 0.006 min

Lab File: VV026425.D

Acq: 18 Jun 2022 15:11




Tgt Ion: 56 Resp: 2181853


Ion Ratio Lower Upper

56 100

69 26.4 24.9 37.3

84 83.7 76.4 114.6


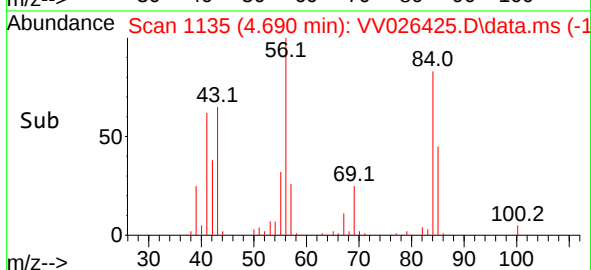






#33
Benzene
Concen: 6.517 ug/L
RT: 5.108 min Scan# 11
Delta R.T. 0.006 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11




Instrument :
MSVOA_V
ClientSampleId :
C0AH2DL


Tgt Ion: 78 Resp: 387697

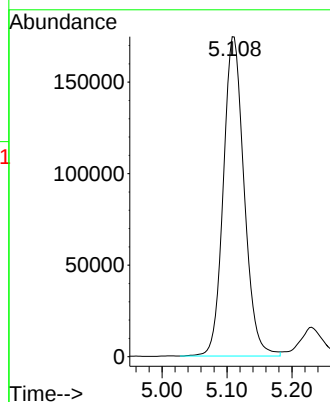

#34
Trichloroethene
Concen: 2.468 ug/L
RT: 5.947 min Scan# 1526
Delta R.T. 0.032 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11

Tgt Ion: 95 Resp: 40080
Ion Ratio Lower Upper
95 100
97 36.6 46.5 86.3#
132 5.4 68.8 127.8#
130 6.4 73.6 136.6#


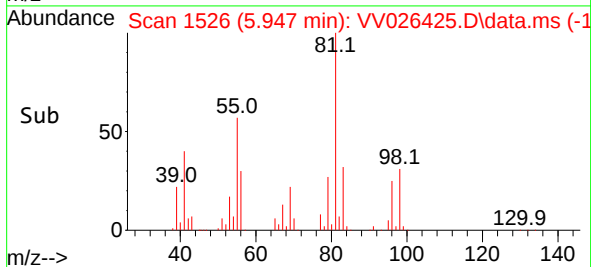
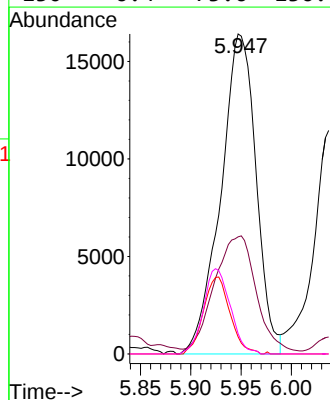
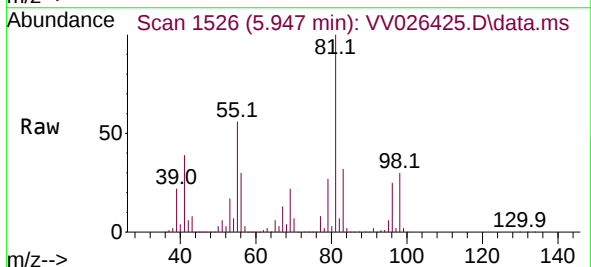


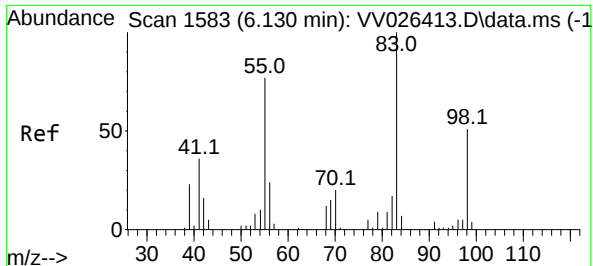

#35
Methylcyclohexane
Concen: 86.101 ug/L
RT: 6.137 min Scan# 1585
Delta R.T. 0.006 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11




Instrument :
MSVOA_V
ClientSampleId :
C0AH2DL


Tgt Ion: 83 Resp: 1934439
Ion Ratio Lower Upper
83 100
55 85.8 59.3 88.9
98 49.1 39.9 59.9

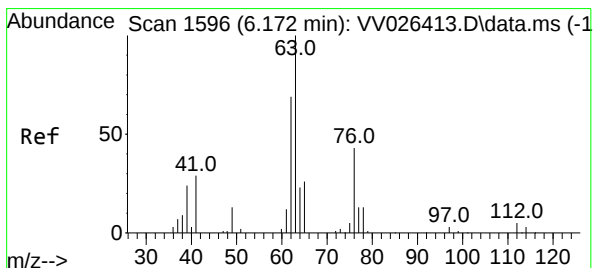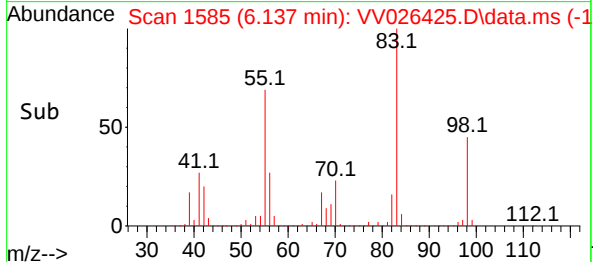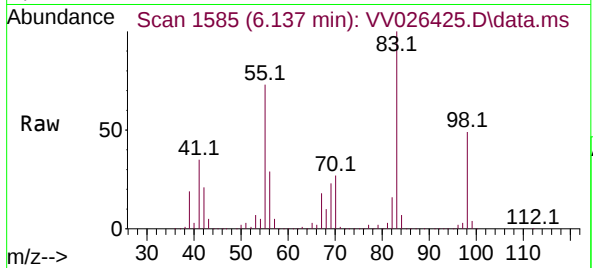

#37
1,2-Dichloropropane
Concen: 1.303 ug/L
RT: 6.137 min Scan# 1585
Delta R.T. -0.035 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11

Tgt Ion: 63 Resp: 20274
Ion Ratio Lower Upper
63 100
112 14.4 3.3 4.9#


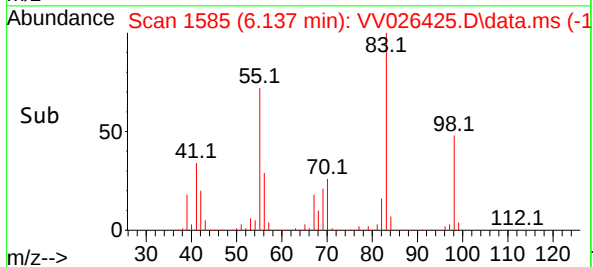

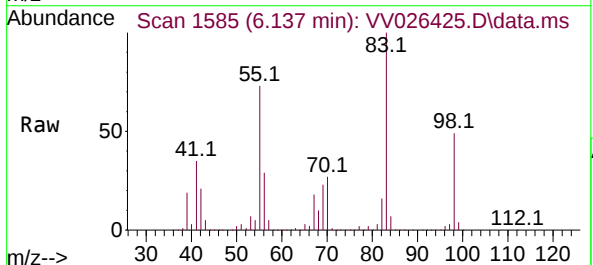


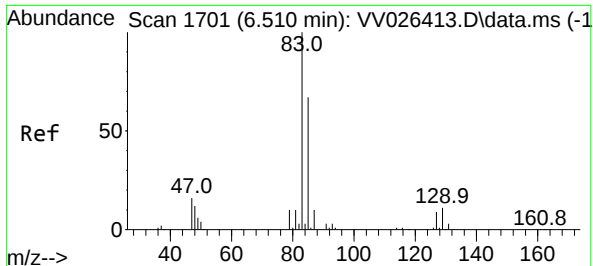

#38
Bromodichloromethane
Concen: 2.772 ug/L
RT: 6.571 min Scan# 11
Delta R.T. 0.061 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11




Instrument :
MSVOA_V
ClientSampleId :
C0AH2DL


Tgt Ion: 83 Resp: 52309
Ion Ratio Lower Upper
83 100
85 1.5 45.6 84.6#
127 0.0 7.2 10.8#

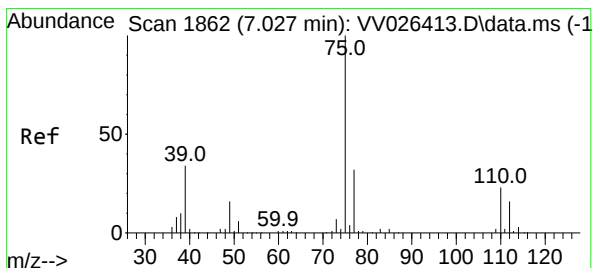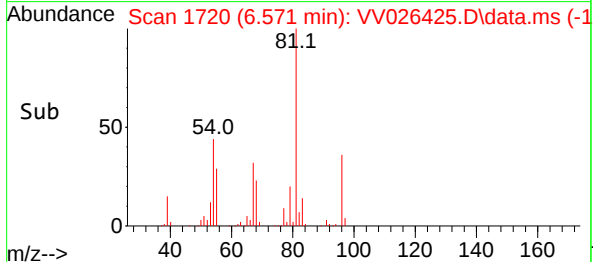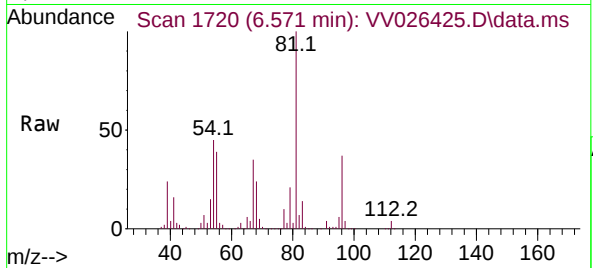

#39
cis-1,3-Dichloropropene
Concen: 0.116 ug/L
RT: 6.995 min Scan# 1852
Delta R.T. -0.032 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11

Tgt Ion: 75 Resp: 2053
Ion Ratio Lower Upper
75 100
77 199.0 23.0 42.6#

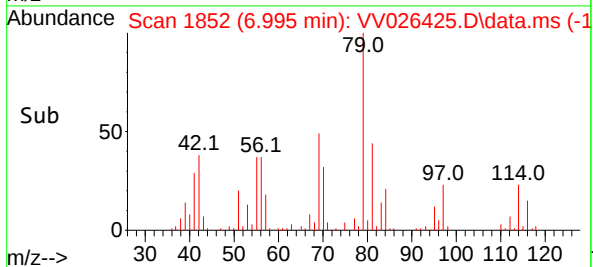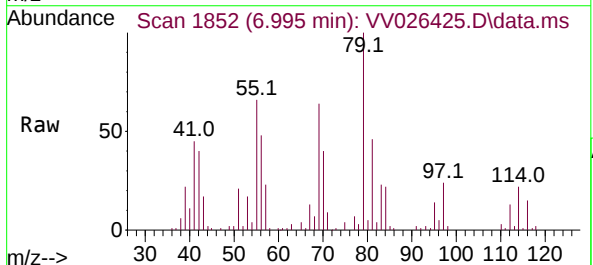



#40

4-Methyl-2-pentanone

Concen: 5.701 ug/L

RT: 7.243 min Scan# 1924

Delta R.T. 0.016 min

Lab File: VV026425.D

Acq: 18 Jun 2022 15:11

Instrument :

MSVOA_V

ClientSampleId :

C0AH2DL





Tgt Ion: 43 Resp: 32615

Ion Ratio Lower Upper

43 100

58 78.3 33.3 49.9#

100 26.9 13.4 20.2#

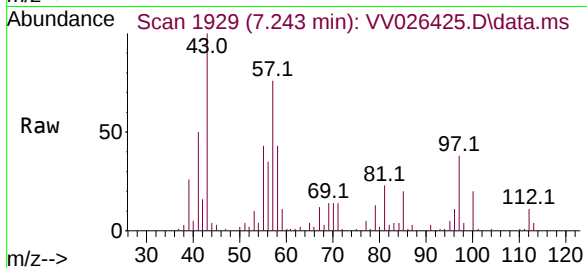

#44

trans-1,3-Dichloropropene

Concen: 22.302 ug/L

RT: 7.400 min Scan# 1978

Delta R.T. -0.251 min

Lab File: VV026425.D




Acq: 18 Jun 2022 15:11


Tgt Ion: 75 Resp: 316303

Ion Ratio Lower Upper

75 100

77 169.3 23.7 43.9#


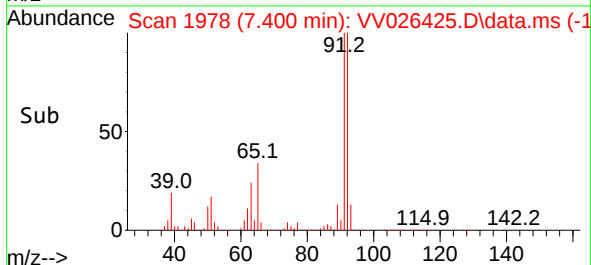
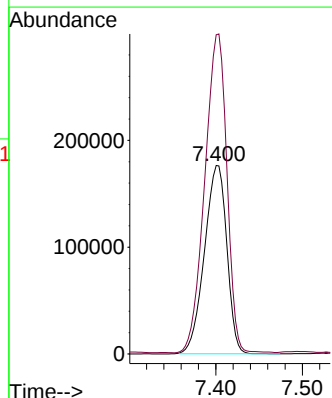
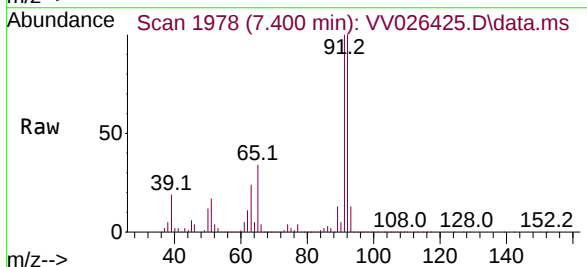




#45
1,1,2-Trichloroethane
Concen: 16.966 ug/L
RT: 7.793 min Scan# 2114
Delta R.T. -0.045 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11




Instrument :
MSVOA_V
ClientSampleId :
C0AH2DL


Tgt Ion: 97 Resp: 173276
Ion Ratio Lower Upper
97 100
99 0.5 42.4 78.6#
83 10.7 56.1 104.1#
85 0.5 36.3 67.5#

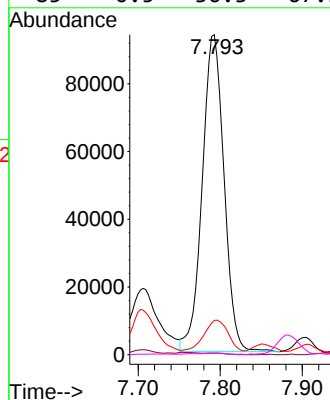

#47
Tetrachloroethene
Concen: 0.130 ug/L
RT: 7.982 min Scan# 2159
Delta R.T. 0.010 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11

Tgt Ion: 164 Resp: 1558
Ion Ratio Lower Upper
164 100
129 94.3 67.5 125.3
131 96.0 63.8 118.4
166 109.6 89.5 166.3


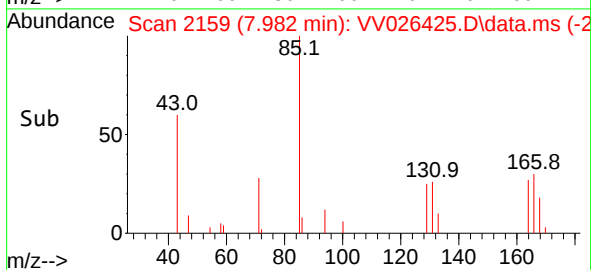
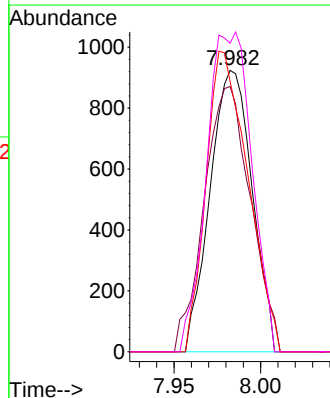





#48
2-Hexanone
Concen: 14.409 ug/L
RT: 8.150 min Scan# 2159
Delta R.T. 0.010 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11




Instrument :
MSVOA_V
ClientSampleId :
C0AH2DL


Tgt Ion: 43 Resp: 59064
Ion Ratio Lower Upper
43 100
58 71.3 48.7 73.1
57 148.8 16.0 24.0#
100 17.5 11.0 16.6#



#49
Dibromochloromethane
Concen: 0.143 ug/L
RT: 7.982 min Scan# 2159
Delta R.T. -0.260 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11

Tgt Ion: 129 Resp: 1621
Ion Ratio Lower Upper
129 100
127 0.0 56.4 104.7#

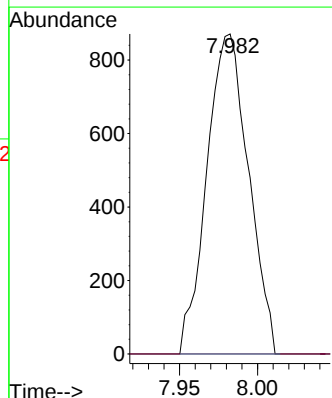



#55

Styrene

Concen: 55.588 ug/L

RT: 9.577 min Scan# 2

Delta R.T. 0.019 min

Lab File: VV026425.D

Acq: 18 Jun 2022 15:11

Instrument :

MSVOA_V

ClientSampleId :





C0AH2DL

Tgt Ion:104 Resp: 2211111

Ion Ratio Lower Upper

104 100

78 292.6 29.5 54.7#

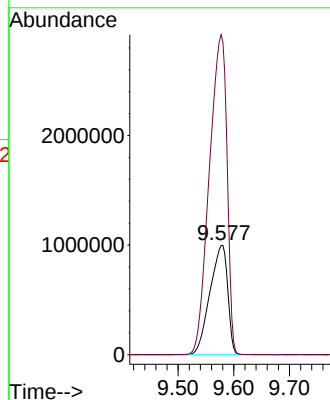

#60

Isopropylbenzene

Concen: 61.693 ug/L

RT: 9.937 min Scan# 2767

Delta R.T. 0.006 min

Lab File: VV026425.D

Acq: 18 Jun 2022 15:11




Tgt Ion:105 Resp: 3875038


Ion Ratio Lower Upper

105 100

120 27.0 21.5 32.3

77 0.0 12.2 18.4#


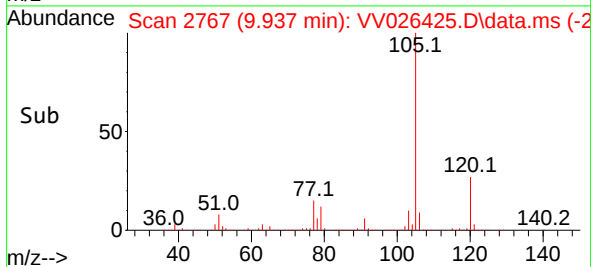
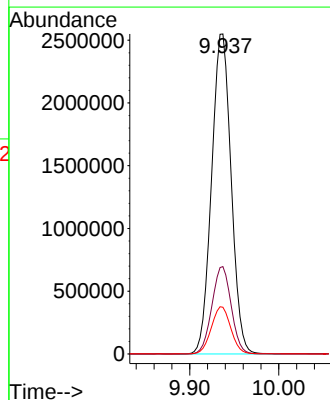
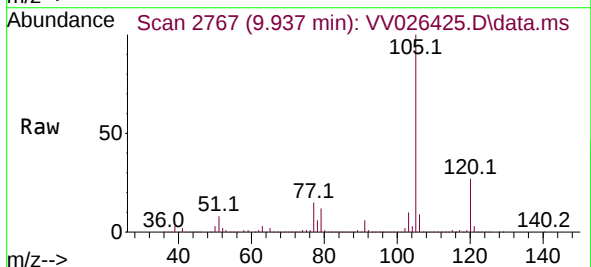




#61
1,2,3-Trichloropropane
Concen: 11.553 ug/L
RT: 10.358 min Scan# 2898
Delta R.T. 0.087 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11




Instrument :
MSVOA_V
ClientSampleId :
C0AH2DL


Tgt Ion: 75 Resp: 88329
Ion Ratio Lower Upper
75 100
77 0.0 26.9 40.3#
110 4.3 30.7 46.1#

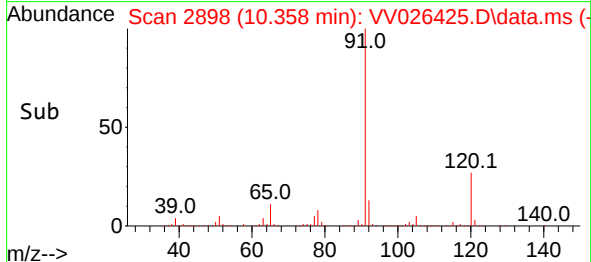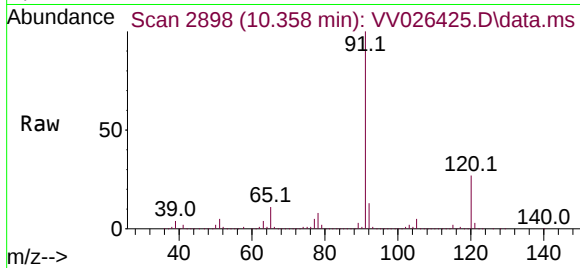

#62
1,3,5-Trimethylbenzene
Concen: 11.759 ug/L
RT: 10.358 min Scan# 2898
Delta R.T. -0.180 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11

Tgt Ion: 105 Resp: 586084
Ion Ratio Lower Upper
105 100
120 605.1 39.9 59.9#


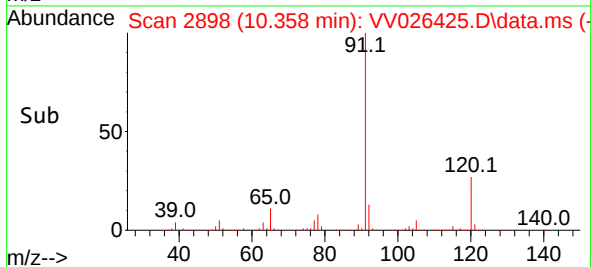

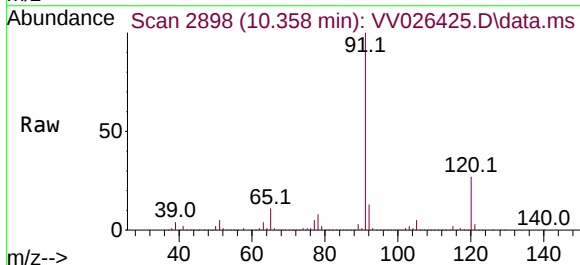




#63
 1,2,4-Trimethylbenzene
 Concen: 14.515 ug/L
 RT: 11.092 min Scan# 3126
 Delta R.T. 0.180 min
 Lab File: VV026425.D
 Acq: 18 Jun 2022 15:11




Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH2DL


Tgt Ion:105 Resp: 716061
 Ion Ratio Lower Upper
 105 100
 120 0.0 36.9 55.3#

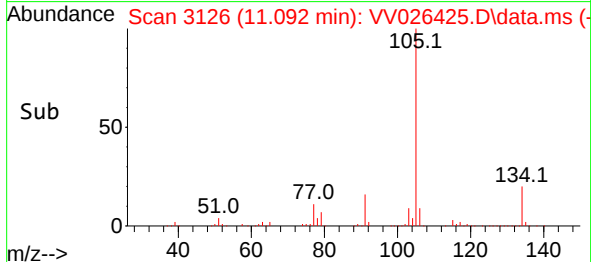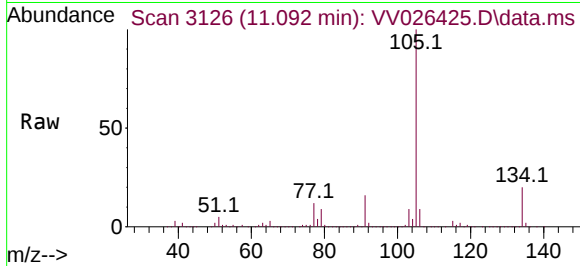

#68
 1,2-Dibromo-3-chloropropane
 Concen: 30.224 ug/L
 RT: 12.413 min Scan# 3537
 Delta R.T. -0.013 min
 Lab File: VV026425.D
 Acq: 18 Jun 2022 15:11


Tgt Ion: 75 Resp: 40932
 Ion Ratio Lower Upper
 75 100
 155 0.0 63.7 95.5#
 157 0.0 85.0 127.6#

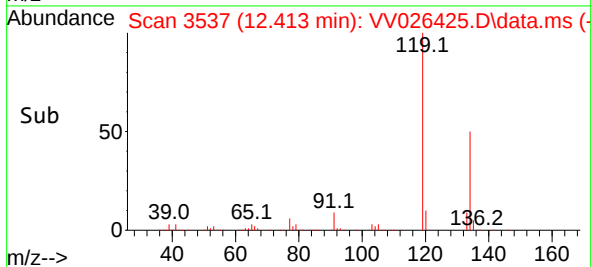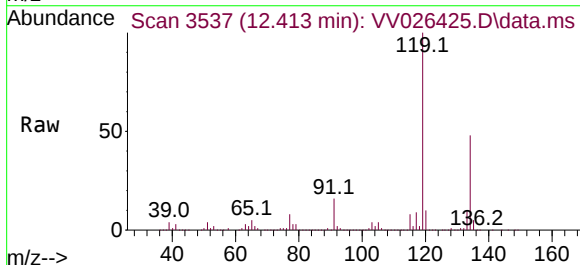



#71
Naphthalene
Concen: 538.664 ug/L
RT: 13.503 min Scan# 3876
Delta R.T. 0.003 min
Lab File: VV026425.D
Acq: 18 Jun 2022 15:11

Instrument :
MSVOA_V
ClientSampleId :
C0AH2DL

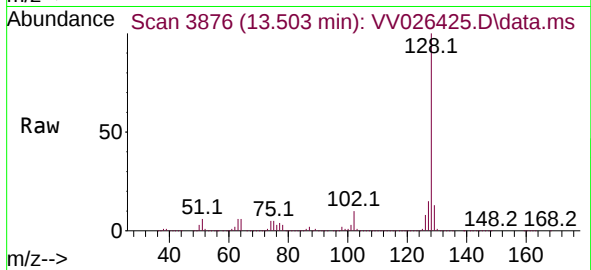

Tgt Ion:128 Resp:12309862
Ion Ratio Lower Upper
128 100
129 12.3 8.7 13.1
127 14.0 10.6 16.0

