

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061822\
 Data File : VW026435.D
 Acq On : 18 Jun 2022 20:36
 Operator : SY/MD
 Sample : N3358-14
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB333

Quant Time: Jun 20 01:32:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 20 01:25:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.661	114	276	5.000	ug/L	# 0.04
28) Chlorobenzene-d5	8.870	117	1072	5.000	ug/L	0.02
58) 1,4-Dichlorobenzene-d4	11.255	152	1707	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	213	8.885	ug/L	-0.04
Spiked Amount	5.000	Range 40 - 130	Recovery	=	177.800%#	
7) Chloroethane-d5	1.574	69	86	4.563	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	91.200%	
11) 1,1-Dichloroethene-d2	2.118	63	79	1.919	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	38.400%#	
20) 2-Butanone-d5	0.000	46	0	0.000	ug/L	
Spiked Amount	50.000	Range 40 - 130	Recovery	=	0.000%#	
24) Chloroform-d	4.381	84	20	0.569	ug/L	0.03
Spiked Amount	5.000	Range 70 - 125	Recovery	=	11.400%#	
26) 1,2-Dichloroethane-d4	0.000	65	0	0.000	ug/L	
Spiked Amount	5.000	Range 70 - 130	Recovery	=	0.000%#	
32) Benzene-d6	5.082	84	260	0.907	ug/L	0.03
Spiked Amount	5.000	Range 70 - 125	Recovery	=	18.200%#	
36) 1,2-Dichloropropane-d6	0.000	67	0	0.000	ug/L	
Spiked Amount	5.000	Range 60 - 140	Recovery	=	0.000%#	
41) Toluene-d8	7.336	98	655	2.506	ug/L	0.02
Spiked Amount	5.000	Range 70 - 130	Recovery	=	50.200%#	
43) trans-1,3-Dichloroprop...	0.000	79	0	0.000	ug/L	
Spiked Amount	5.000	Range 55 - 130	Recovery	=	0.000%#	
46) 2-Hexanone-d5	0.000	63	0	0.000	ug/L	
Spiked Amount	50.000	Range 45 - 130	Recovery	=	0.000%#	
56) 1,1,2,2-Tetrachloroeth...	10.227	84	141	2.736	ug/L	0.01
Spiked Amount	5.000	Range 65 - 120	Recovery	=	54.800%#	
66) 1,2-Dichlorobenzene-d4	11.625	152	1237	4.705	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	94.000%	
Target Compounds						
						Qvalue
2) Dichlorodifluoromethane	1.288	85	96	4.652	ug/L #	42
3) Chloromethane	1.262	50	1900	82.916	ug/L #	74
5) Vinyl chloride	1.327	62	45	1.889	ug/L #	1
6) Bromomethane	1.584	94	135	10.139	ug/L	92
8) Chloroethane	1.529	64	212620	14375.987	ug/L #	49
12) 1,1-Dichloroethene	2.130	96	131	7.513	ug/L	77
13) Acetone	2.147	43	628	346.429	ug/L	67
14) Carbon disulfide	2.314	76	26851	624.544	ug/L	98
15) Methyl Acetate	2.439	43	88	20.232	ug/L #	48
16) Methylene chloride	2.526	84	13860	623.024	ug/L	96
18) trans-1,2-Dichloroethene	2.790	96	46	2.720	ug/L #	1
19) 1,1-Dichloroethane	3.118	63	26	0.806	ug/L #	50
21) 2-Butanone	4.153	43	20	8.527	ug/L #	50
25) Chloroform	4.391	83	65	1.858	ug/L #	17
33) Benzene	5.117	78	90	0.327	ug/L	100
35) Methylcyclohexane	6.133	83	118	1.137	ug/L #	18
40) 4-Methyl-2-pentanone	7.230	43	45	1.703	ug/L #	42
42) Toluene	7.404	91	531	1.837	ug/L	80
51) Chlorobenzene	8.902	112	445	2.358	ug/L #	77

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061822\
 Data File : VW026435.D
 Acq On : 18 Jun 2022 20:36
 Operator : SY/MD
 Sample : N3358-14
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB333


Quant Time: Jun 20 01:32:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 20 01:25:22 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

52) Ethylbenzene	9.021	91	2816	9.718	ug/L	93
53) m,p-Xylene	9.143	106	3060	27.090	ug/L	72
54) o-Xylene	9.551	106	986	9.011	ug/L	73
55) Styrene	9.571	104	148	0.805	ug/L #	42
57) 1,1,2,2-Tetrachloroethane	10.243	83	47	0.982	ug/L #	23
60) Isopropylbenzene	9.934	105	1110	1.220	ug/L #	87
61) 1,2,3-Trichloropropane	10.284	75	90	0.813	ug/L #	4
62) 1,3,5-Trimethylbenzene	10.545	105	1302	1.803	ug/L	93
63) 1,2,4-Trimethylbenzene	10.918	105	2950	4.127	ug/L	96
64) 1,3-Dichlorobenzene	11.185	146	1472	3.292	ug/L #	73
65) 1,4-Dichlorobenzene	11.278	146	1481	3.259	ug/L #	82
67) 1,2-Dichlorobenzene	11.651	146	1324	3.343	ug/L	96
68) 1,2-Dibromo-3-chloropr...	12.654	75	356	18.144	ug/L #	3
69) 1,3,5-Trichlorobenzene	12.651	180	2061	6.375	ug/L #	85
70) 1,2,4-trichlorobenzene	13.262	180	2434	10.207	ug/L	96
71) Naphthalene	13.506	128	7002	21.148	ug/L	98
72) 1,2,3-Trichlorobenzene	13.747	180	3524	17.652	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jun 20 01:32:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 20 01:25:22 2022
Response via : Initial Calibration







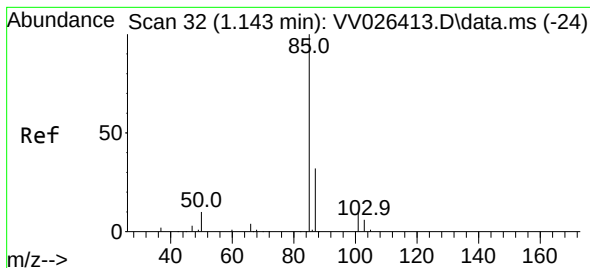

#2
Dichlorodifluoromethane
Concen: 4.652 ug/L
RT: 1.288 min Scan# 71
Delta R.T. 0.145 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36




Instrument :
MSVOA_V
ClientSampleId :
BFB333


Tgt Ion: 85 Resp: 96
Ion Ratio Lower Upper
85 100
87 0.0 26.0 39.0#

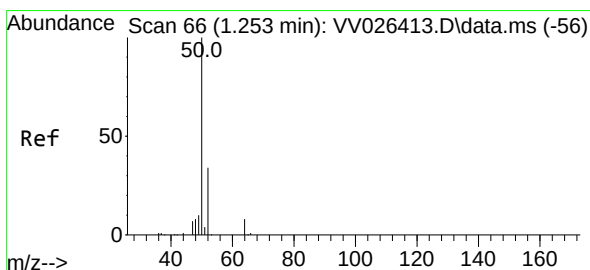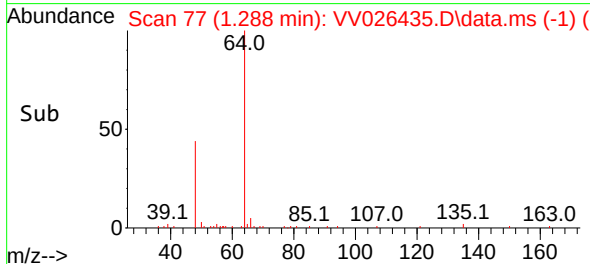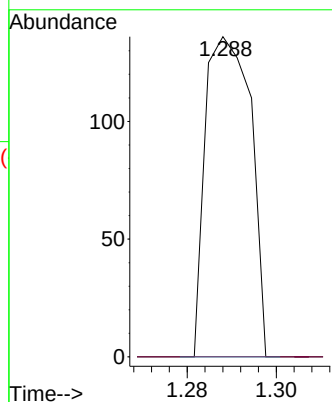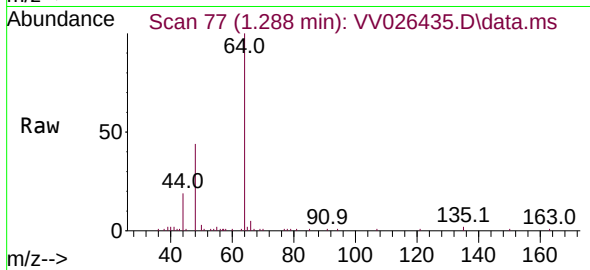

#3
Chloromethane
Concen: 82.916 ug/L
RT: 1.262 min Scan# 69
Delta R.T. 0.010 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36

Tgt Ion: 50 Resp: 1900
Ion Ratio Lower Upper
50 100
52 18.9 23.7 44.1#

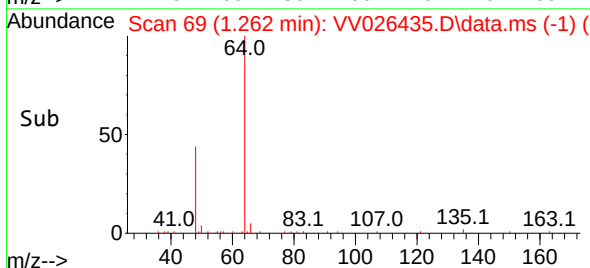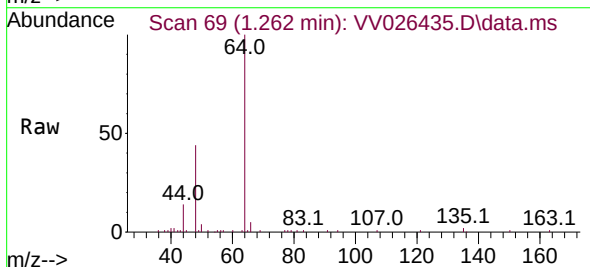

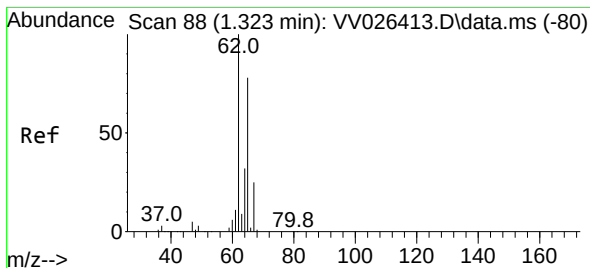

#5

Vinyl chloride

Concen: 1.889 ug/L

RT: 1.327 min Scan# 89

Delta R.T. 0.003 min

Lab File: VV026435.D

Acq: 18 Jun 2022 20:36

Instrument :

MSVOA_V

ClientSampleId :





BFB333

Tgt Ion: 62 Resp: 45

Ion Ratio Lower Upper

62 100

64 10971.4 23.2 43.2#

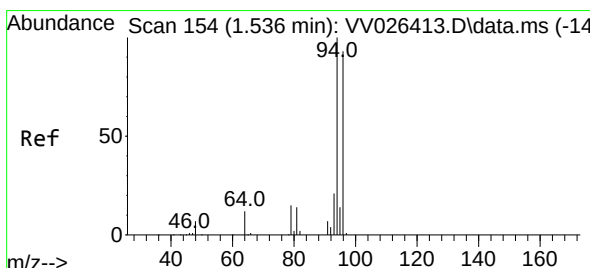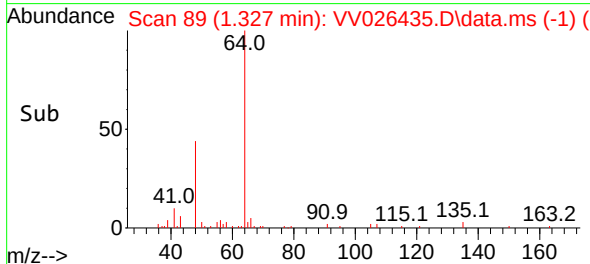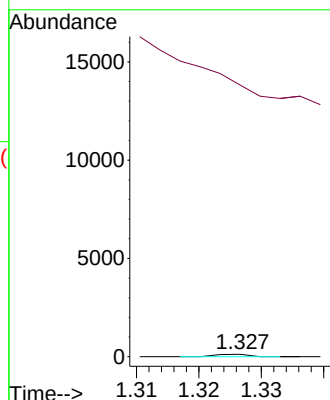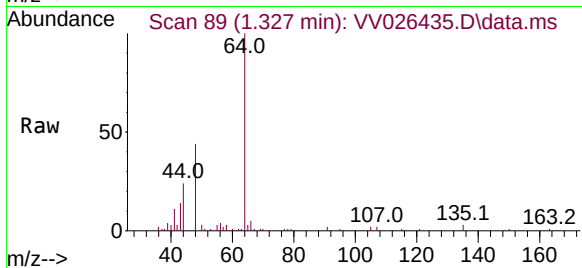

#6

Bromomethane

Concen: 10.139 ug/L

RT: 1.584 min Scan# 169

Delta R.T. 0.048 min

Lab File: VV026435.D




Acq: 18 Jun 2022 20:36


Tgt Ion: 94 Resp: 135

Ion Ratio Lower Upper

94 100

96 86.3 65.7 121.9


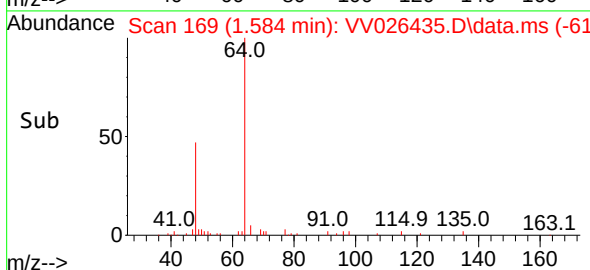
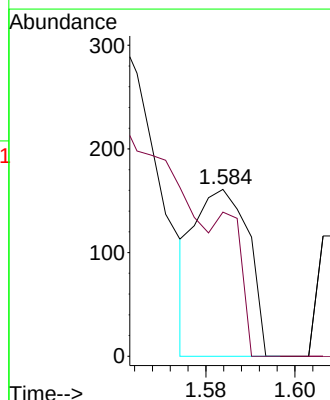
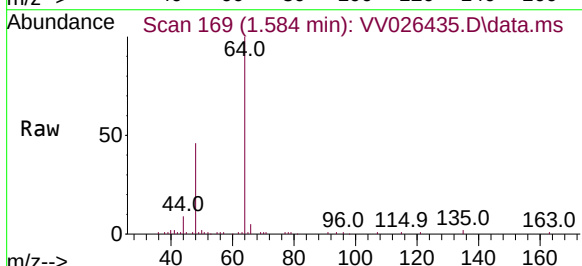




#8
Chloroethane
Concen: 14375.987 ug/L
RT: 1.529 min Scan# 11
Delta R.T. -0.068 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36




Instrument :
MSVOA_V
ClientSampleId :
BFB333


Tgt Ion: 64 Resp: 212620
Ion Ratio Lower Upper
64 100
66 5.3 24.1 44.7#

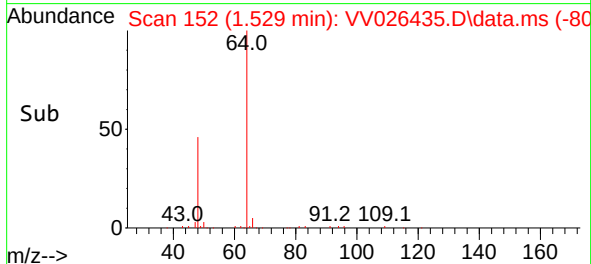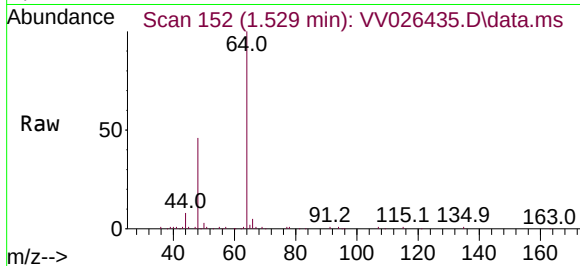

#12
1,1-Dichloroethene
Concen: 7.513 ug/L
RT: 2.130 min Scan# 339
Delta R.T. -0.000 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36

Tgt Ion: 96 Resp: 131
Ion Ratio Lower Upper
96 100
61 118.9 117.1 217.5
63 140.9 92.8 172.4

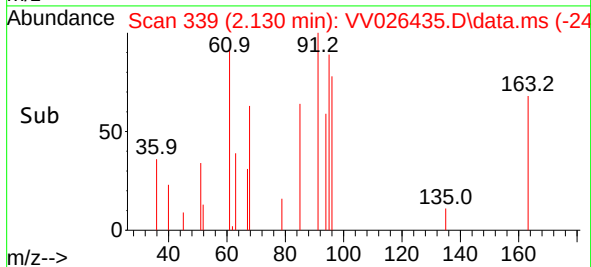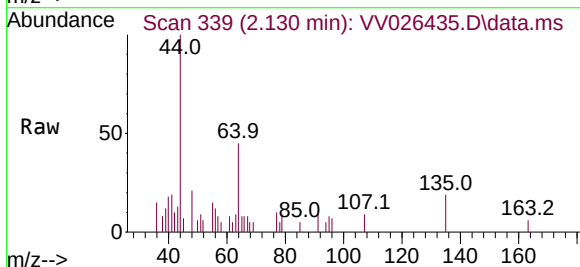



#13

Acetone

Concen: 346.429 ug/L

RT: 2.147 min Scan# 34

Delta R.T. -0.064 min

Lab File: VV026435.D

Acq: 18 Jun 2022 20:36

Instrument :

MSVOA_V

ClientSampleId :





BFB333

Tgt Ion: 43 Resp: 628

Ion Ratio Lower Upper

43 100

58 12.3 0.0 60.0

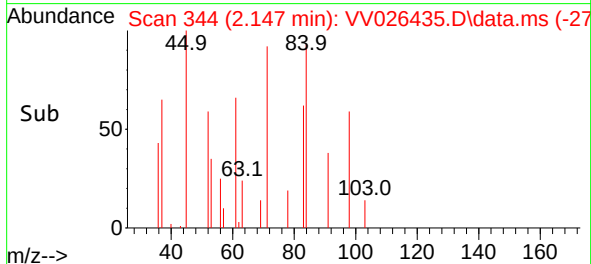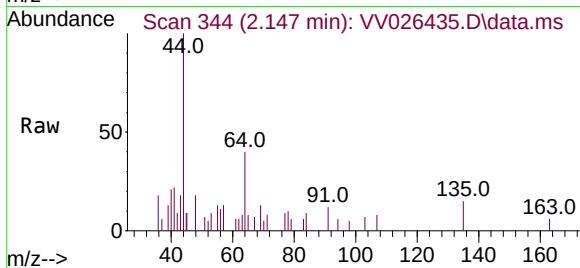

#14

Carbon disulfide

Concen: 624.544 ug/L

RT: 2.314 min Scan# 396

Delta R.T. 0.010 min

Lab File: VV026435.D




Acq: 18 Jun 2022 20:36


Tgt Ion: 76 Resp: 26851

Ion Ratio Lower Upper

76 100

78 10.3 7.7 11.5




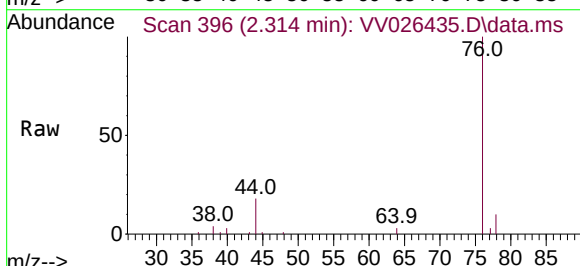




#15
Methyl Acetate
Concen: 20.232 ug/L
RT: 2.439 min Scan# 41
Delta R.T. -0.016 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36




Instrument :
MSVOA_V
ClientSampleId :
BFB333


Tgt Ion: 43 Resp: 88
Ion Ratio Lower Upper
43 100
74 0.0 21.4 32.0#

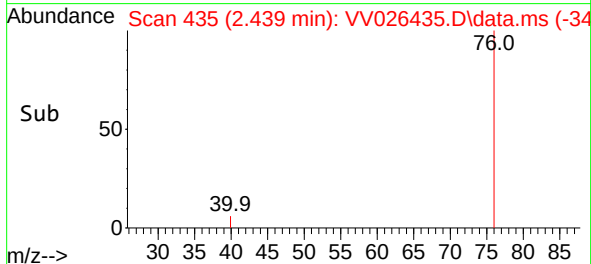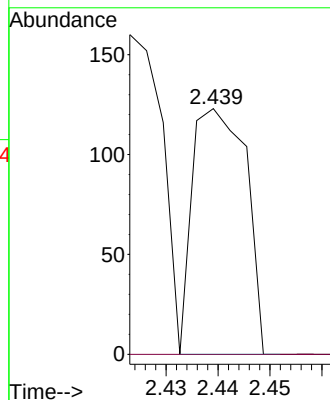

#16
Methylene chloride
Concen: 623.024 ug/L
RT: 2.526 min Scan# 462
Delta R.T. 0.010 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36

Tgt Ion: 84 Resp: 13860
Ion Ratio Lower Upper
84 100
86 62.8 44.0 81.8
49 104.0 77.3 143.7


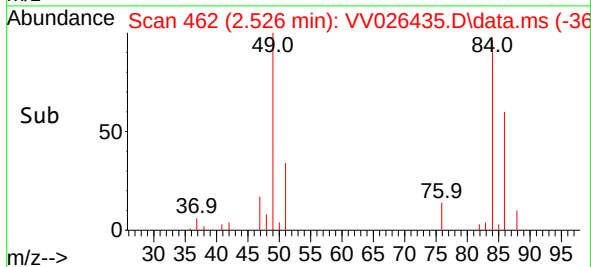
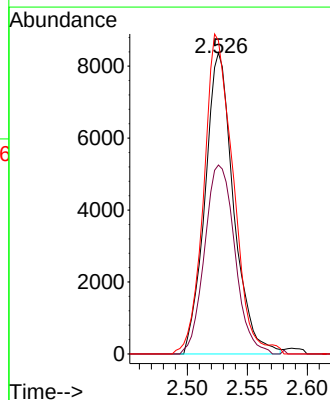
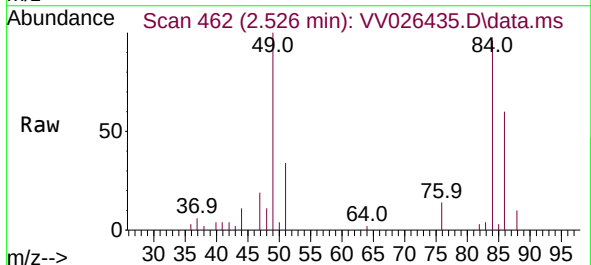




#18
 trans-1,2-Dichloroethene
 Concen: 2.720 ug/L
 RT: 2.790 min Scan# 54
 Delta R.T. 0.019 min
 Lab File: VV026435.D
 Acq: 18 Jun 2022 20:36




Instrument :
 MSVOA_V
 ClientSampleId :
 BFB333


Tgt Ion: 96 Resp: 46
 Ion Ratio Lower Upper
 96 100
 61 0.0 91.3 169.6#
 98 0.0 45.3 84.1#

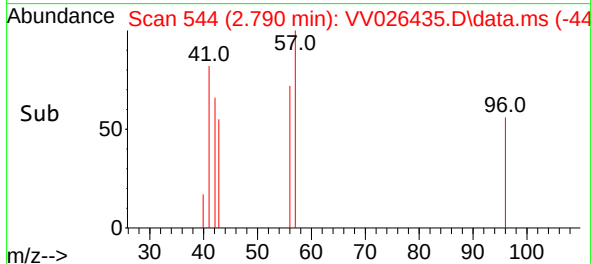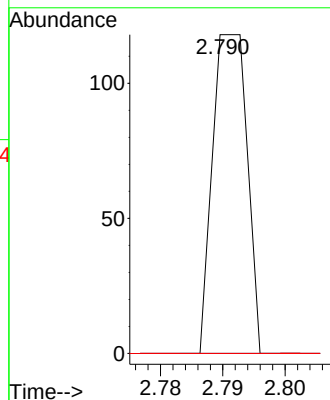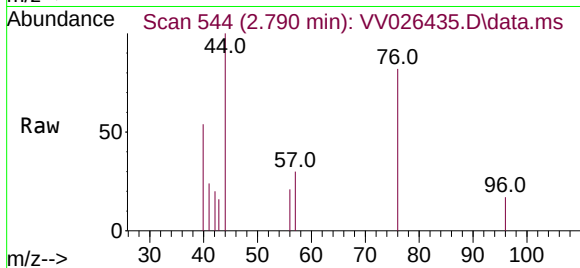

#19
 1,1-Dichloroethane
 Concen: 0.806 ug/L
 RT: 3.118 min Scan# 646
 Delta R.T. -0.080 min
 Lab File: VV026435.D
 Acq: 18 Jun 2022 20:36

Tgt Ion: 63 Resp: 26
 Ion Ratio Lower Upper
 63 100
 65 0.0 22.3 41.3#
 83 0.0 8.9 16.5#


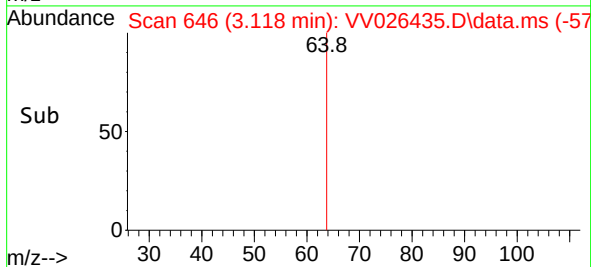
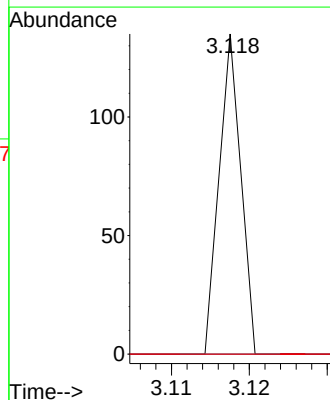
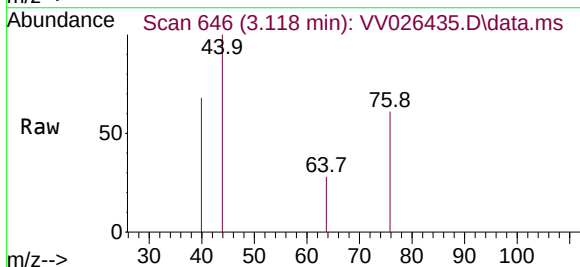


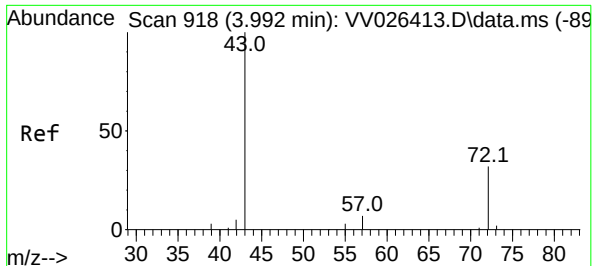

#21
2-Butanone
Concen: 8.527 ug/L
RT: 4.153 min Scan# 918
Delta R.T. 0.161 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36




Instrument :
MSVOA_V
ClientSampleId :
BFB333


Tgt Ion: 43 Resp: 20
Ion Ratio Lower Upper
43 100
72 0.0 12.7 38.0#

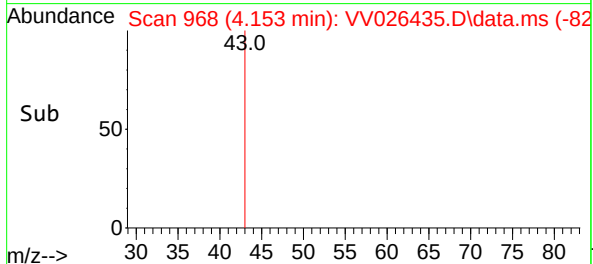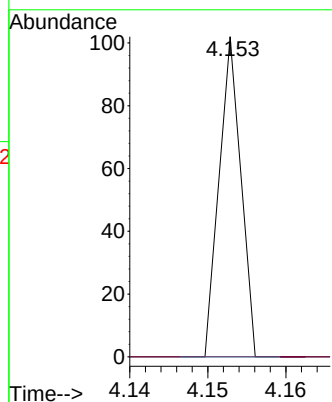

#25
Chloroform
Concen: 1.858 ug/L
RT: 4.391 min Scan# 1042
Delta R.T. 0.010 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36

Tgt Ion: 83 Resp: 65
Ion Ratio Lower Upper
83 100
85 0.0 46.5 86.3#

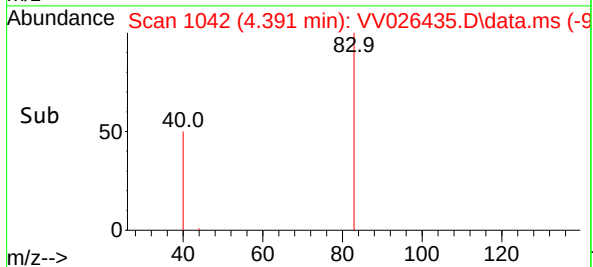
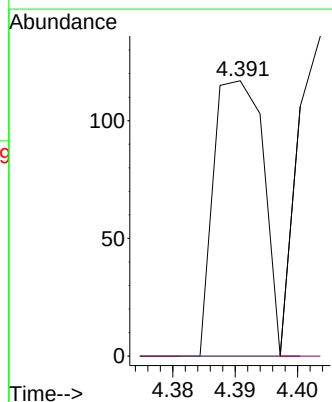
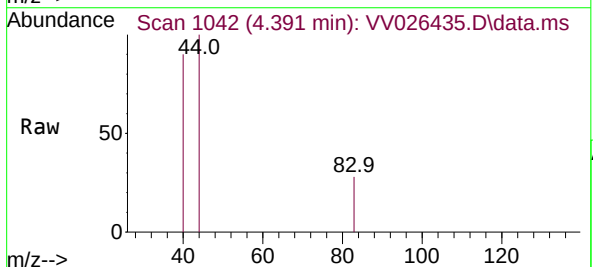


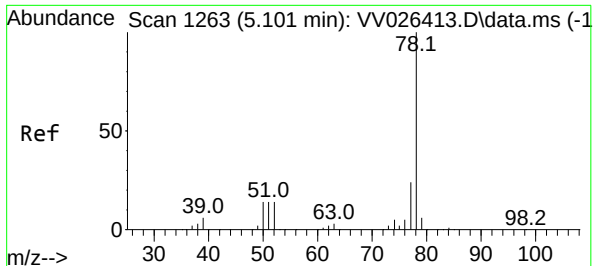

#33
Benzene
Concen: 0.327 ug/L
RT: 5.117 min Scan# 11
Delta R.T. 0.016 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36




Instrument :
MSVOA_V
ClientSampleId :
BFB333


Tgt Ion: 78 Resp: 90

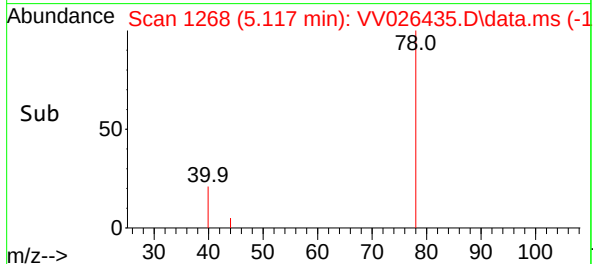

#35
Methylcyclohexane
Concen: 1.137 ug/L
RT: 6.133 min Scan# 1584
Delta R.T. 0.003 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36

Tgt Ion: 83 Resp: 118
Ion Ratio Lower Upper
83 100
55 0.0 59.3 88.9#
98 0.0 39.9 59.9#

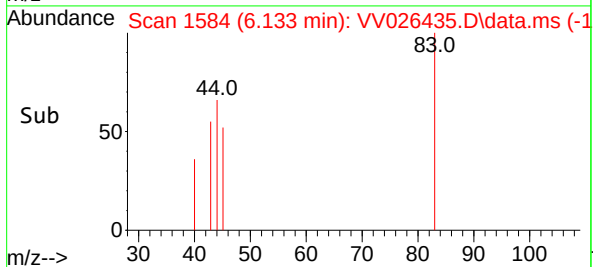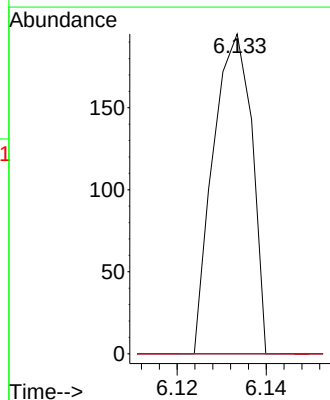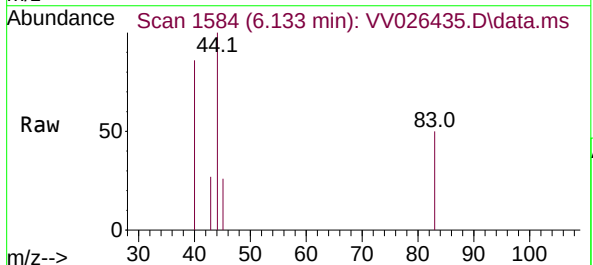

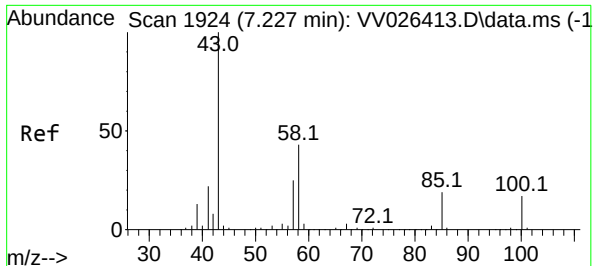

#40

4-Methyl-2-pentanone

Concen: 1.703 ug/L

RT: 7.230 min Scan# 1924

Delta R.T. 0.003 min

Lab File: VV026435.D

Acq: 18 Jun 2022 20:36





Instrument :

MSVOA_V

ClientSampleId :

BFB333

Tgt Ion: 43	Resp:	45
Ion Ratio	Lower	Upper
43	100	
58	0.0	33.3 49.9#
100	0.0	13.4 20.2#

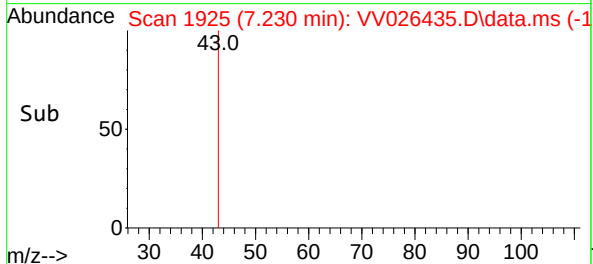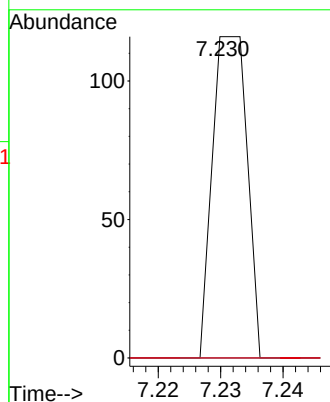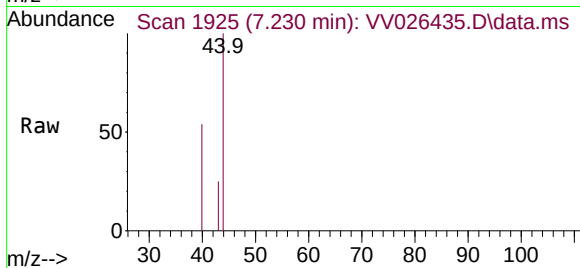

#42

Toluene

Concen: 1.837 ug/L




RT: 7.404 min Scan# 1979


Delta R.T. 0.016 min

Lab File: VV026435.D

Acq: 18 Jun 2022 20:36

Tgt Ion: 91	Resp:	531
Ion Ratio	Lower	Upper
91	100	
92	42.4	40.1 74.5


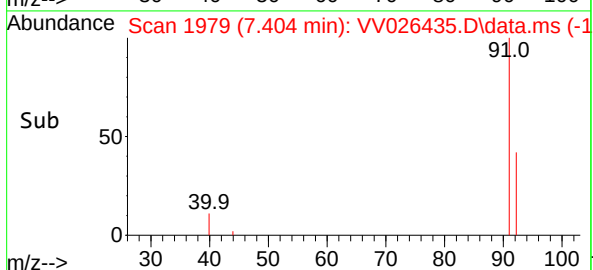
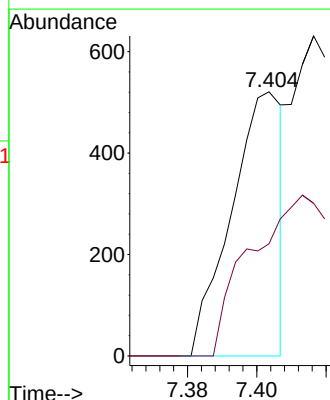
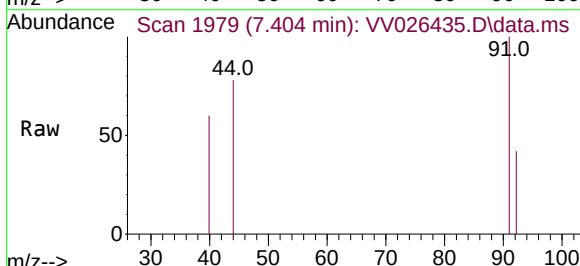




#51
Chlorobenzene
Concen: 2.358 ug/L
RT: 8.902 min Scan# 2445
Delta R.T. 0.022 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36




Instrument :
MSVOA_V
ClientSampleId :
BFB333


Tgt Ion:112 Resp: 445
Ion Ratio Lower Upper
112 100
114 0.0 22.7 42.3#
77 57.5 44.5 66.7

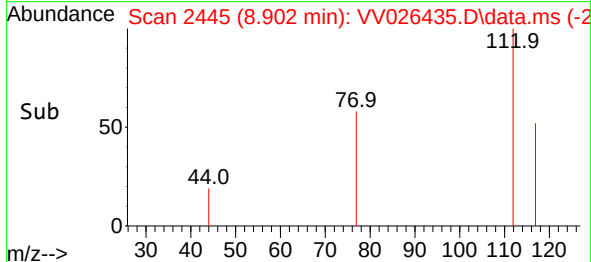

#52
Ethylbenzene
Concen: 9.718 ug/L
RT: 9.021 min Scan# 2482
Delta R.T. 0.010 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36

Tgt Ion: 91 Resp: 2816
Ion Ratio Lower Upper
91 100
106 26.7 21.6 40.0


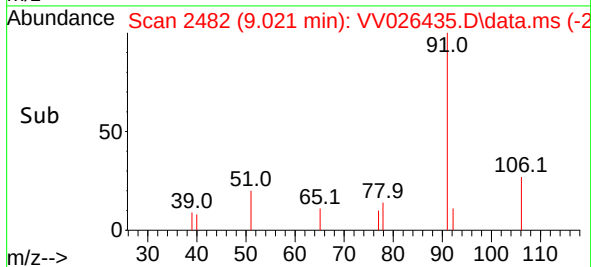

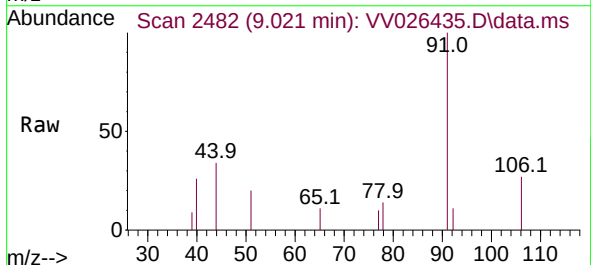


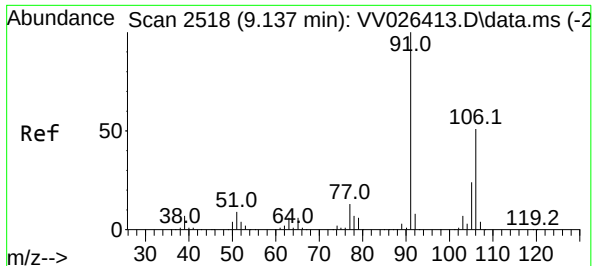

#53
m,p-Xylene
Concen: 27.090 ug/L
RT: 9.143 min Scan# 21
Delta R.T. 0.006 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36




Instrument :
MSVOA_V
ClientSampleId :
BFB333


Tgt Ion:106 Resp: 3060
Ion Ratio Lower Upper
106 100
91 159.4 141.3 262.3

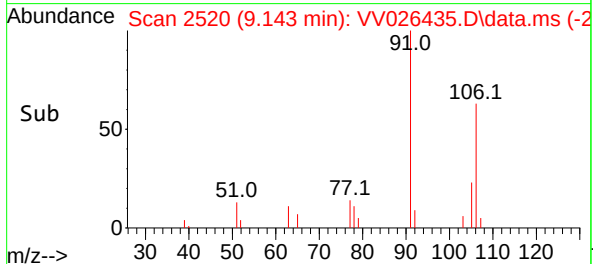

#54
o-Xylene
Concen: 9.011 ug/L
RT: 9.551 min Scan# 2647
Delta R.T. 0.010 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36

Tgt Ion:106 Resp: 986
Ion Ratio Lower Upper
106 100
91 162.8 143.3 266.1




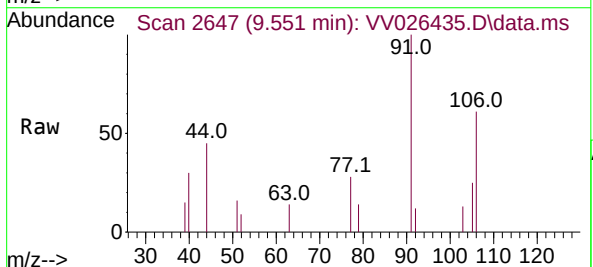


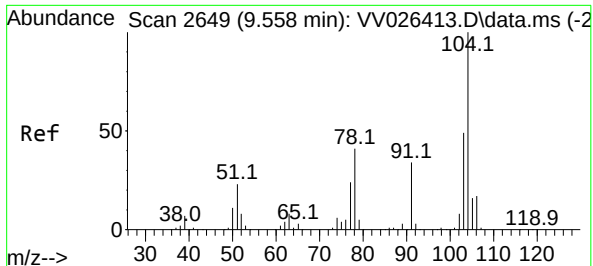

#55
Styrene
Concen: 0.805 ug/L
RT: 9.571 min Scan# 2653
Delta R.T. 0.013 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36




Instrument :
MSVOA_V
ClientSampleId :
BFB333


Tgt Ion:104 Resp: 148
Ion Ratio Lower Upper
104 100
78 78.5 29.5 54.7#

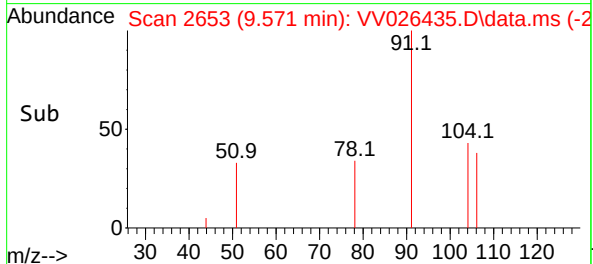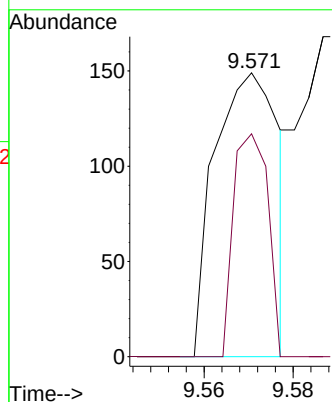

#57
1,1,2,2-Tetrachloroethane
Concen: 0.982 ug/L
RT: 10.243 min Scan# 2862
Delta R.T. 0.003 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36

Tgt Ion: 83 Resp: 47
Ion Ratio Lower Upper
83 100
85 0.0 47.1 87.5#
131 0.0 7.7 11.5#


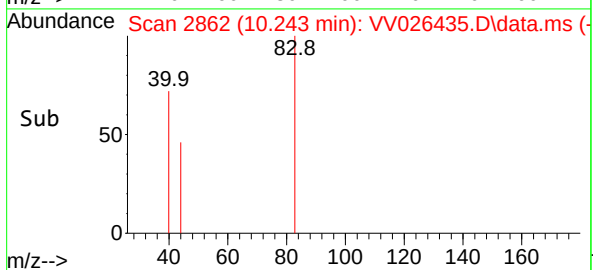

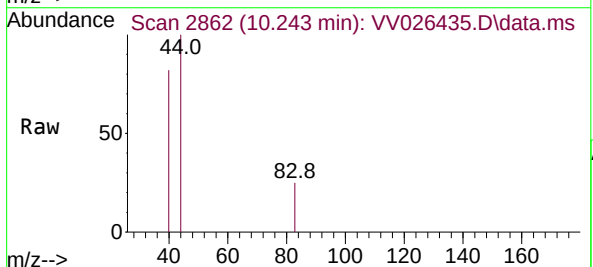




#60
Isopropylbenzene
Concen: 1.220 ug/L
RT: 9.934 min Scan# 21
Delta R.T. 0.003 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36




Instrument :
MSVOA_V
ClientSampleId :
BFB333


Tgt Ion:105 Resp: 1110
Ion Ratio Lower Upper
105 100
120 20.5 21.5 32.3#
77 21.4 12.2 18.4#

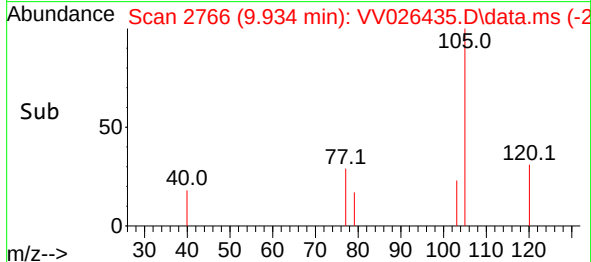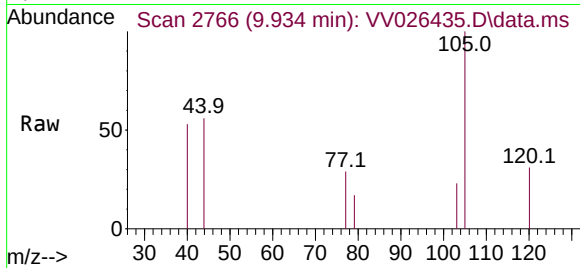

#61
1,2,3-Trichloropropane
Concen: 0.813 ug/L
RT: 10.284 min Scan# 2875
Delta R.T. 0.013 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36

Tgt Ion: 75 Resp: 90
Ion Ratio Lower Upper
75 100
77 110.0 26.9 40.3#
110 0.0 30.7 46.1#

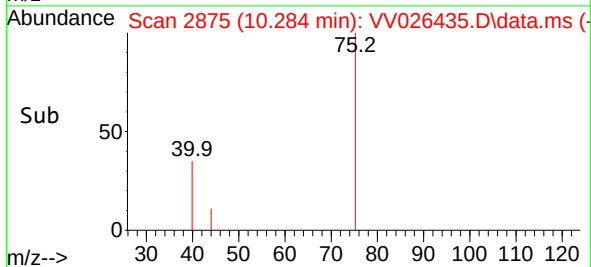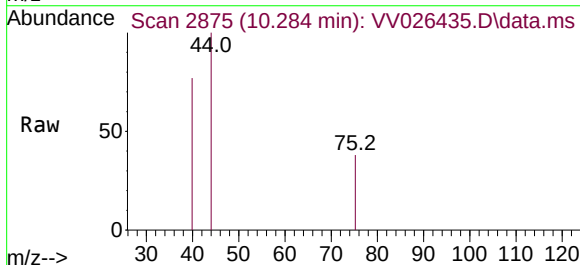



#62

1,3,5-Trimethylbenzene

Concen: 1.803 ug/L

RT: 10.545 min Scan# 2954

Delta R.T. 0.006 min

Lab File: VV026435.D

Acq: 18 Jun 2022 20:36

Instrument :

MSVOA_V

ClientSampleId :





BFB333

Tgt Ion:105 Resp: 1302

Ion Ratio Lower Upper

105 100

120 54.6 39.9 59.9

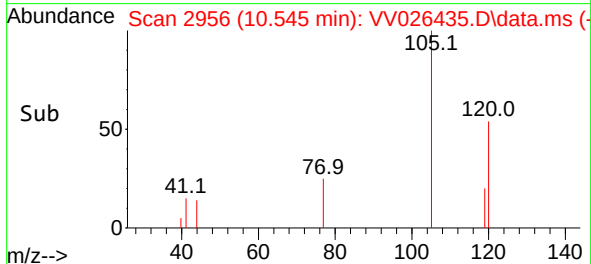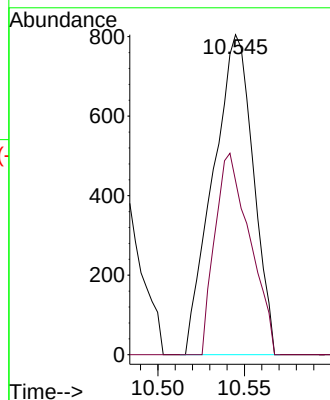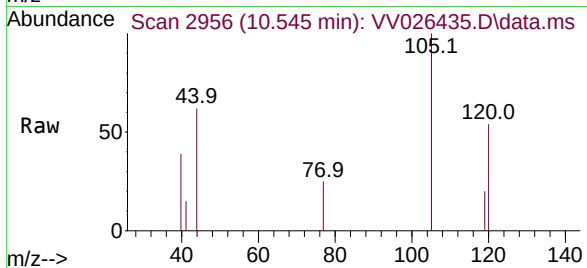

#63

1,2,4-Trimethylbenzene

Concen: 4.127 ug/L

RT: 10.918 min Scan# 3072

Delta R.T. 0.006 min

Lab File: VV026435.D




Acq: 18 Jun 2022 20:36


Tgt Ion:105 Resp: 2950

Ion Ratio Lower Upper

105 100

120 43.5 36.9 55.3


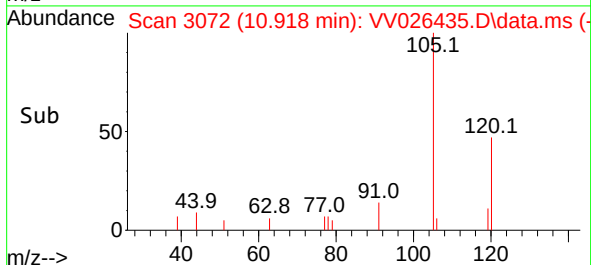
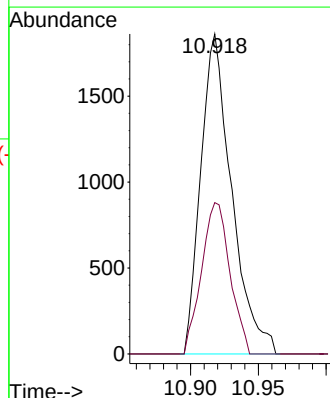
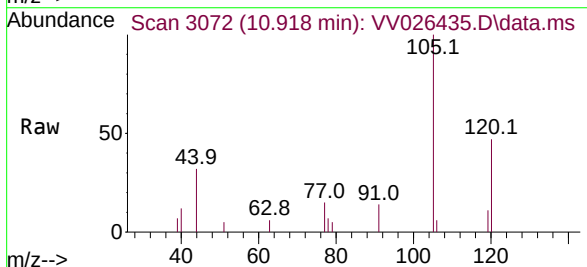




#64
1,3-Dichlorobenzene
Concen: 3.292 ug/L
RT: 11.185 min Scan# 3155
Delta R.T. 0.006 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36




Instrument :
MSVOA_V
ClientSampleId :
BFB333


Tgt Ion:146 Resp: 1472
Ion Ratio Lower Upper
146 100
111 28.4 27.8 51.6
148 39.2 44.9 83.3#

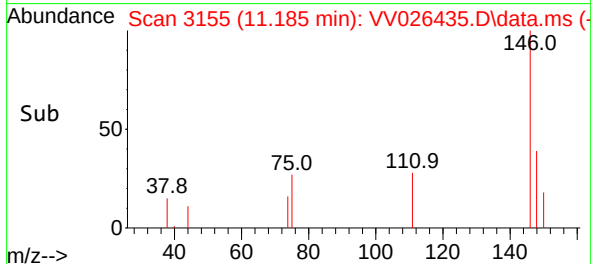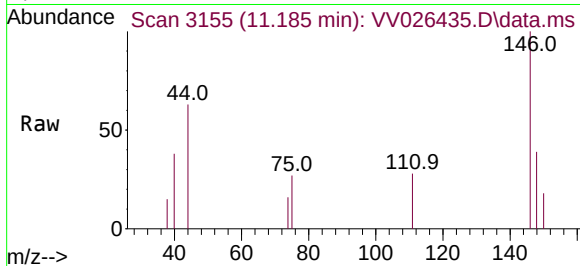

#65
1,4-Dichlorobenzene
Concen: 3.259 ug/L
RT: 11.278 min Scan# 3184
Delta R.T. 0.010 min
Lab File: VV026435.D
Acq: 18 Jun 2022 20:36

Tgt Ion:146 Resp: 1481
Ion Ratio Lower Upper
146 100
111 20.3 26.7 49.7#
148 53.0 43.3 80.3

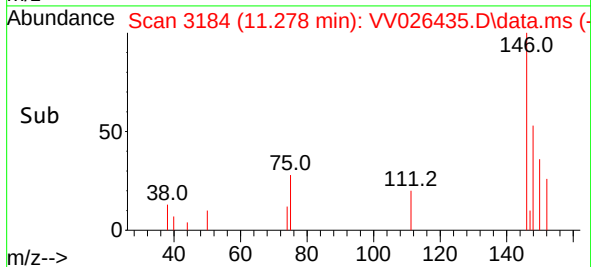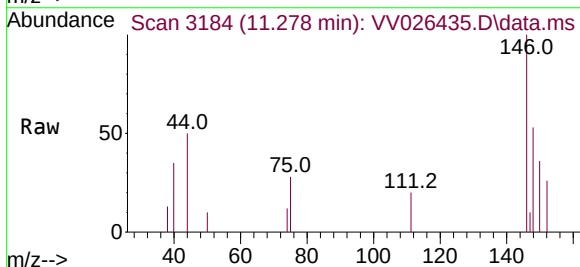



#67

1,2-Dichlorobenzene

Concen: 3.343 ug/L

RT: 11.651 min Scan# 31

Delta R.T. 0.010 min

Lab File: VV026435.D

Acq: 18 Jun 2022 20:36

Instrument :

MSVOA_V

ClientSampleId :

BFB333





Tgt Ion:146 Resp: 1324

Ion Ratio Lower Upper

146 100

111 40.5 33.8 50.8

148 60.9 51.7 77.5

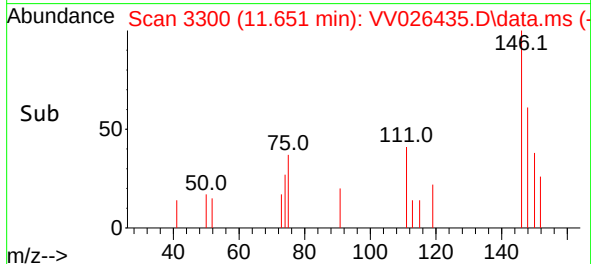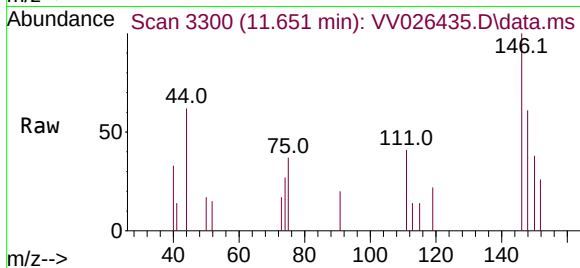

#68

1,2-Dibromo-3-chloropropane

Concen: 18.144 ug/L

RT: 12.654 min Scan# 3612

Delta R.T. 0.228 min

Lab File: VV026435.D

Acq: 18 Jun 2022 20:36




Tgt Ion: 75 Resp: 356


Ion Ratio Lower Upper

75 100

155 0.0 63.7 95.5#

157 0.0 85.0 127.6#


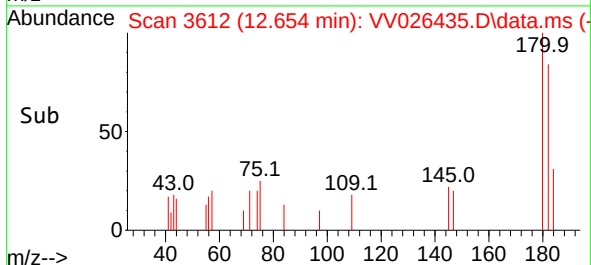
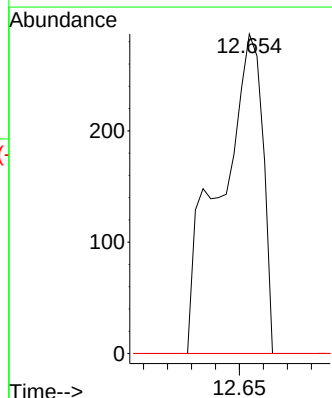
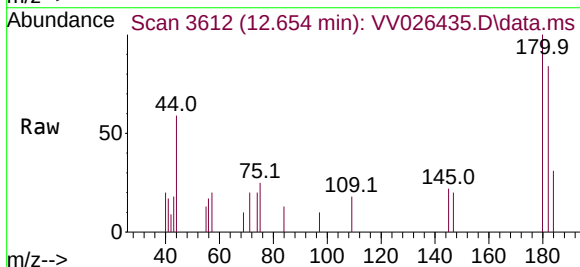




#69
 1,3,5-Trichlorobenzene
 Concen: 6.375 ug/L
 RT: 12.651 min Scan# 30
 Delta R.T. 0.010 min
 Lab File: VV026435.D
 Acq: 18 Jun 2022 20:36




Instrument :
 MSVOA_V
 ClientSampleId :
 BFB333


Tgt Ion:180	Resp:	2061
Ion Ratio	Lower	Upper
180	100	
182	76.8	75.5 113.3
184	23.1	23.7 35.5#
145	25.0	24.2 36.2

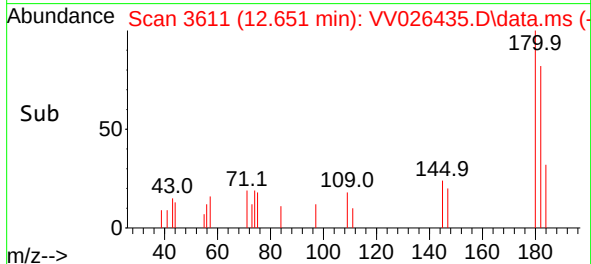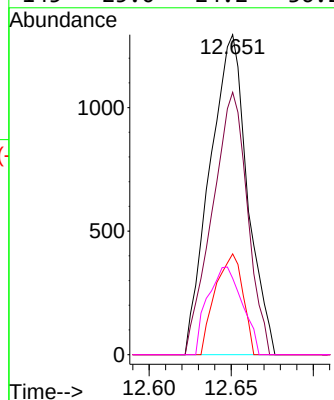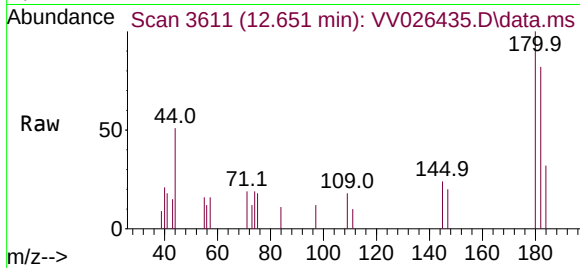

#70
 1,2,4-trichlorobenzene
 Concen: 10.207 ug/L
 RT: 13.262 min Scan# 3801
 Delta R.T. 0.003 min
 Lab File: VV026435.D
 Acq: 18 Jun 2022 20:36

Tgt Ion:180	Resp:	2434
Ion Ratio	Lower	Upper
180	100	
182	99.0	76.2 114.2
145	31.9	23.9 35.9

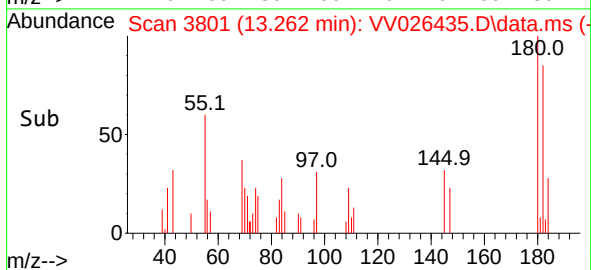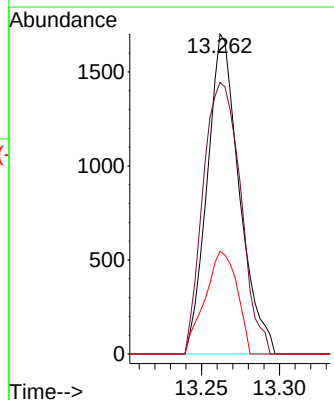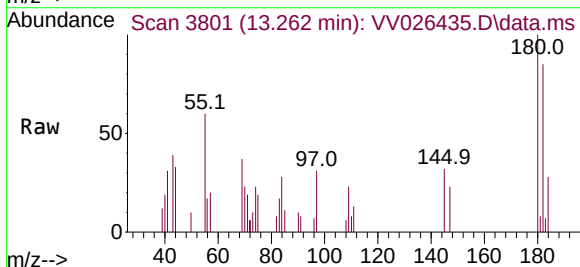



#71

Naphthalene

Concen: 21.148 ug/L

RT: 13.506 min Scan# 31

Delta R.T. 0.006 min

Lab File: VV026435.D

Acq: 18 Jun 2022 20:36

Instrument :

MSVOA_V

ClientSampleId :

BFB333





Tgt Ion:128 Resp: 7002

Ion Ratio Lower Upper

128 100

129 11.0 8.7 13.1

127 14.4 10.6 16.0

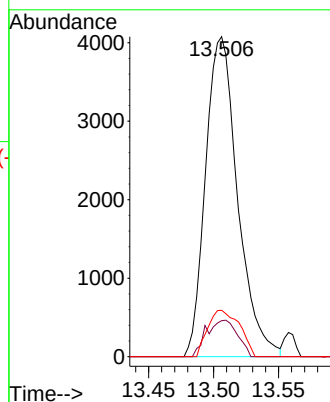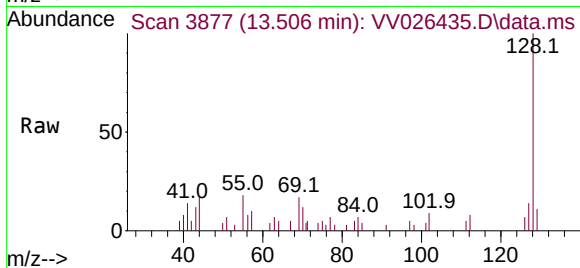

#72

1,2,3-Trichlorobenzene

Concen: 17.652 ug/L

RT: 13.747 min Scan# 3952

Delta R.T. 0.006 min

Lab File: VV026435.D

Acq: 18 Jun 2022 20:36

Tgt Ion:180 Resp: 3524

Ion Ratio Lower Upper

180 100

182 90.1 77.9 116.9

145 34.4 26.7 40.1

