




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
 Data File : VV026422.D
 Acq On : 18 Jun 2022 13:59
 Operator : SY/MD
 Sample : N3345-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK6

Manual IntegrationsAPPROVED

Quant Time: Jun 20 01:29:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 20 01:25:22 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/20/2022
 Supervised By :Mahesh Dadoda 06/20/2022

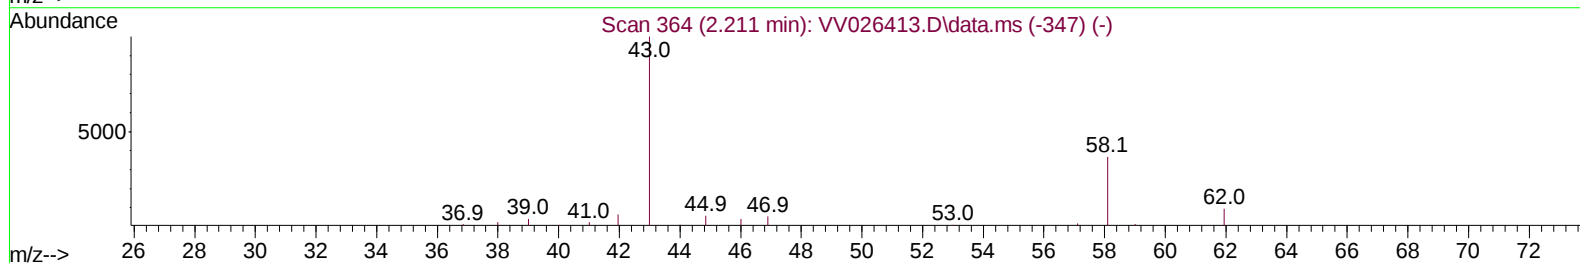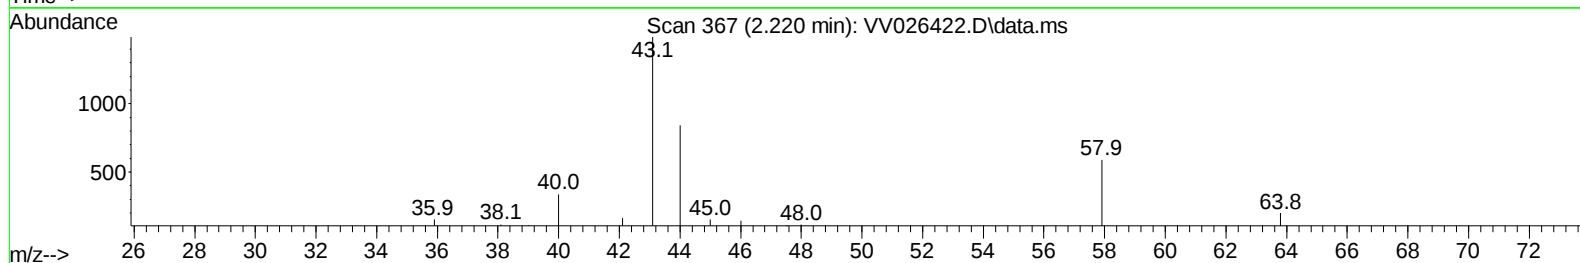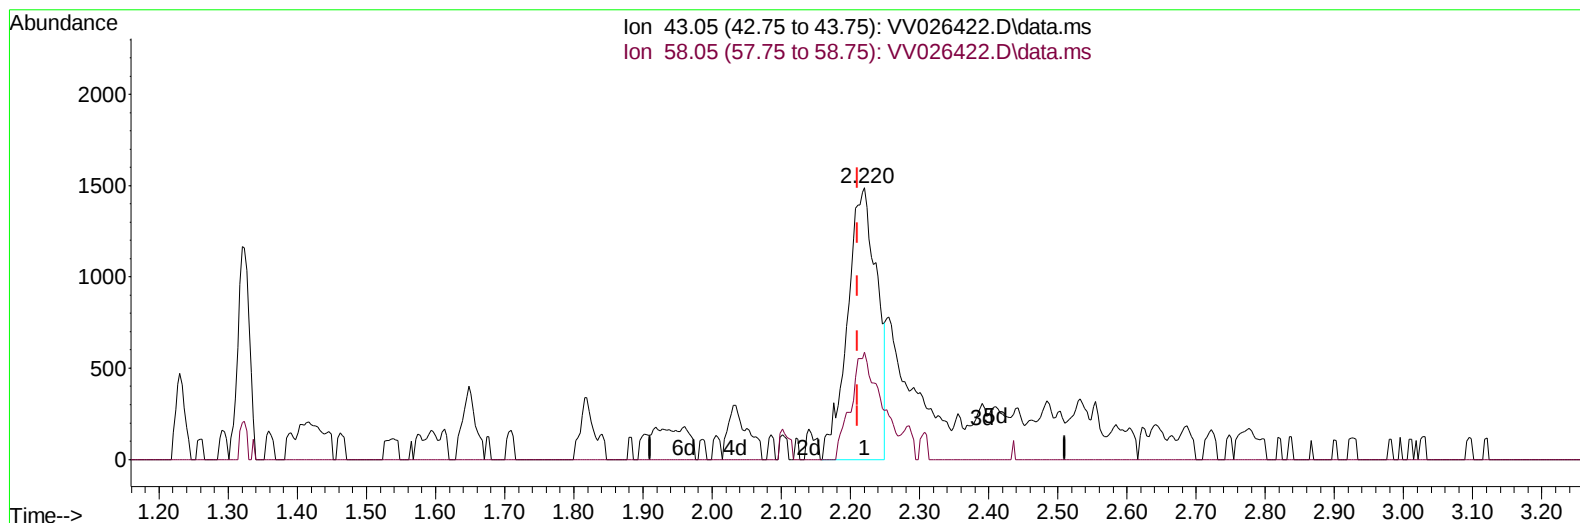

TIC: VV026422.D\data.ms

(13) Acetone (T)

2.220min (+ 0.010) 3.39 ug/L

response 4416

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	39.90
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
 Data File : VV026422.D
 Acq On : 18 Jun 2022 13:59
 Operator : SY/MD
 Sample : N3345-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK6

Manual IntegrationsAPPROVED

Quant Time: Jun 20 01:29:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 20 01:25:22 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/20/2022
 Supervised By :Mahesh Dadoda 06/20/2022

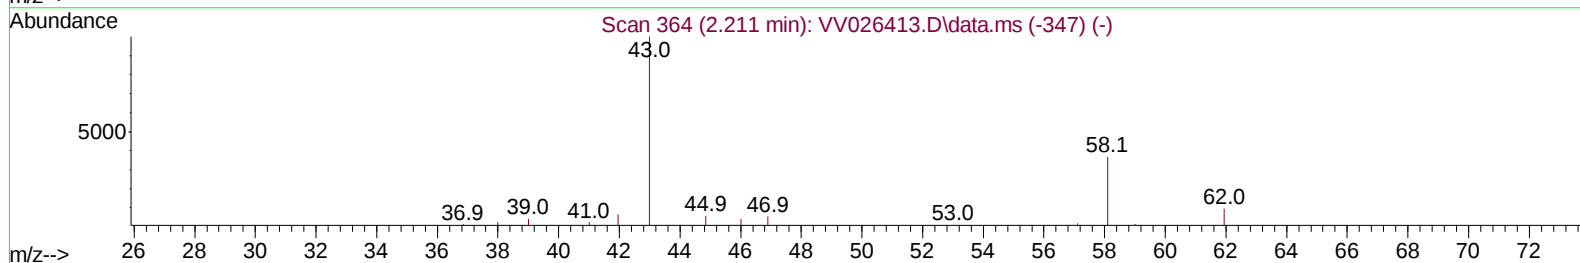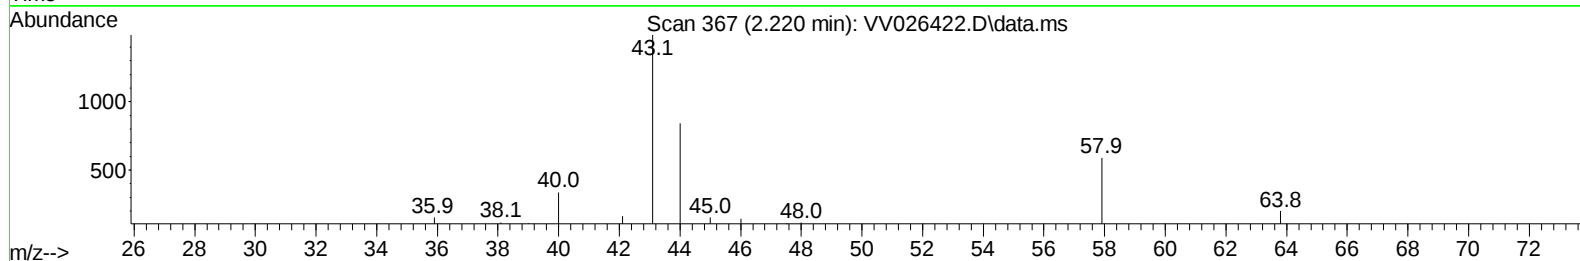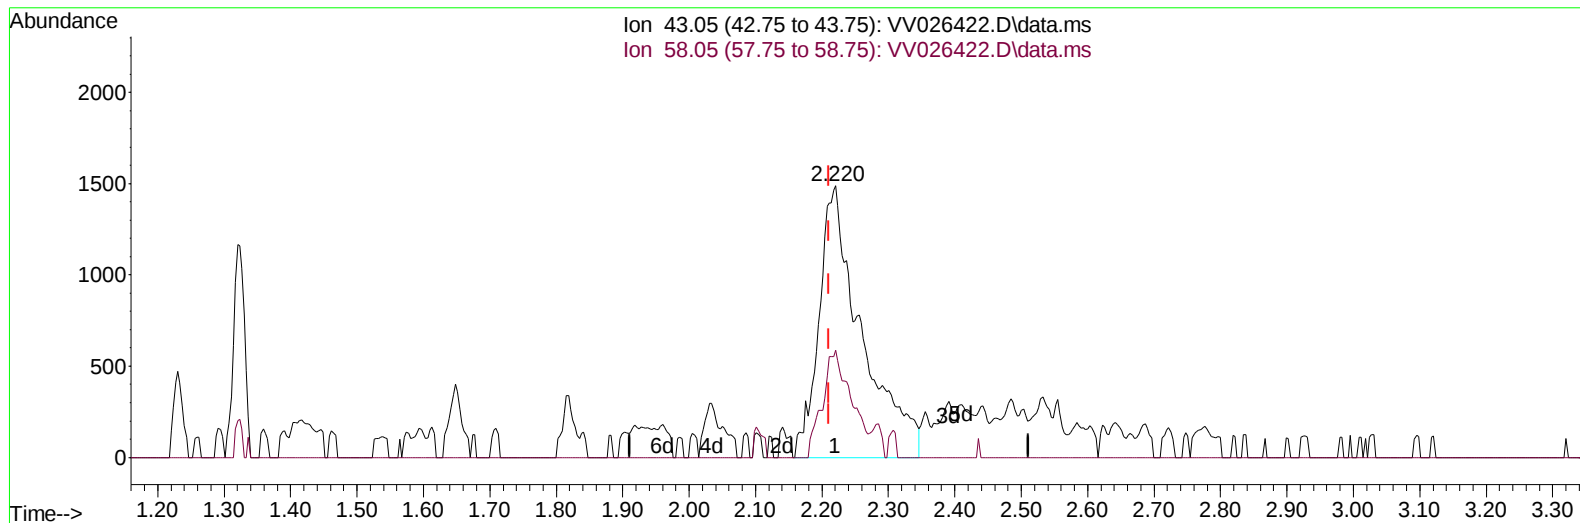

TIC: VV026422.D\data.ms

(13) Acetone (T)

2.220min (+ 0.010) 5.07 ug/L m

response 6619

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	26.62
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
 Data File : VV026422.D
 Acq On : 18 Jun 2022 13:59
 Operator : SY/MD
 Sample : N3345-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK6

Manual IntegrationsAPPROVED

Quant Time: Jun 20 01:29:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 20 01:25:22 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/20/2022
 Supervised By :Mahesh Dadoda 06/20/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	198596	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	186502	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	77325	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	78260	4.537	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	90.800%	
7) Chloroethane-d5	1.584	69	65003	4.793	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	95.800%	
11) 1,1-Dichloroethene-d2	2.121	63	112773	3.807	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	76.200%	
20) 2-Butanone-d5	3.925	46	84632	50.282	ug/L	0.01
Spiked Amount 50.000	Range 40	- 130	Recovery	=	100.560%	
24) Chloroform-d	4.362	84	138918	5.495	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	109.800%	
26) 1,2-Dichloroethane-d4	5.044	65	55557	5.194	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	103.800%	
32) Benzene-d6	5.060	84	269739	5.410	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	108.200%	
36) 1,2-Dichloropropane-d6	6.076	67	80049	5.501	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	110.000%	
41) Toluene-d8	7.320	98	226531	4.983	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	99.600%	
43) trans-1,3-Dichloroprop...	7.629	79	17546	3.718	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	74.400%	
46) 2-Hexanone-d5	8.092	63	65856	46.200	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	92.400%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	48007	5.355	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	107.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	69741	5.855	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	117.200%	
Target Compounds						
					Qvalue	
13) Acetone	2.220	43	6619m	5.074	ug/L	
14) Carbon disulfide	2.307	76	10978	0.355	ug/L #	95
25) Chloroform	4.388	83	60126	2.388	ug/L	100
33) Benzene	5.117	78	2359	0.049	ug/L	100
38) Bromodichloromethane	6.526	83	873	0.058	ug/L #	89
42) Toluene	7.400	91	10494	0.209	ug/L	98
53) m,p-Xylene	9.146	106	1076	0.055	ug/L	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
Data File : VV026422.D
Acq On : 18 Jun 2022 13:59
Operator : SY/MD
Sample : N3345-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK6

Manual IntegrationsAPPROVED

Quant Time: Jun 20 01:29:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 20 01:25:22 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/20/2022
Supervised By :Mahesh Dadoda 06/20/2022

