




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
 Data File : VV026431.D
 Acq On : 18 Jun 2022 18:35
 Operator : SY/MD
 Sample : N3358-18
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4T1

Manual IntegrationsAPPROVED

Quant Time: Jun 20 01:31:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 20 01:25:22 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/20/2022
 Supervised By :Mahesh Dadoda 06/20/2022

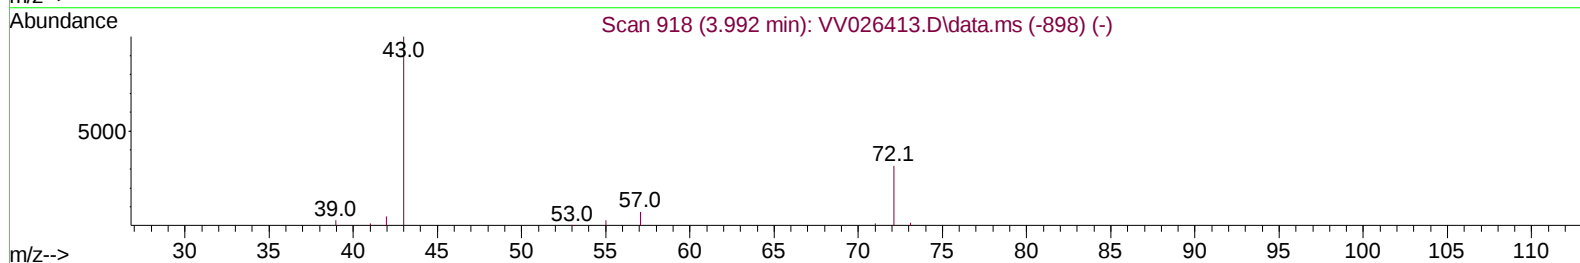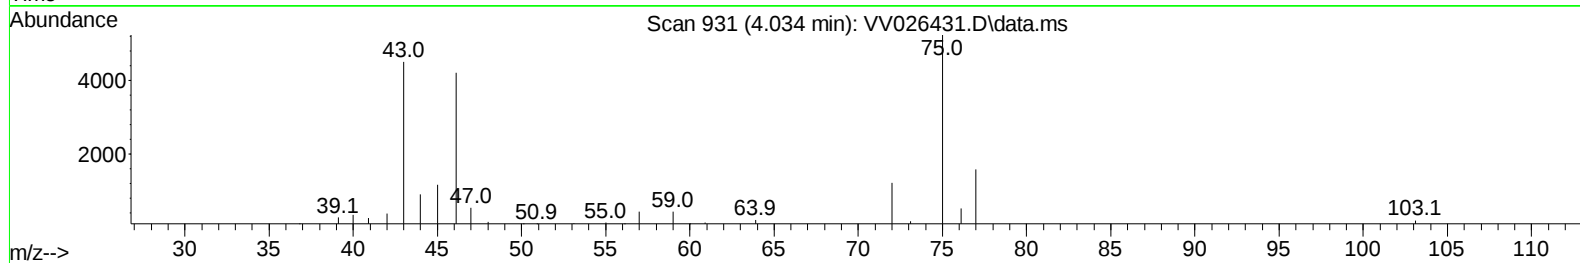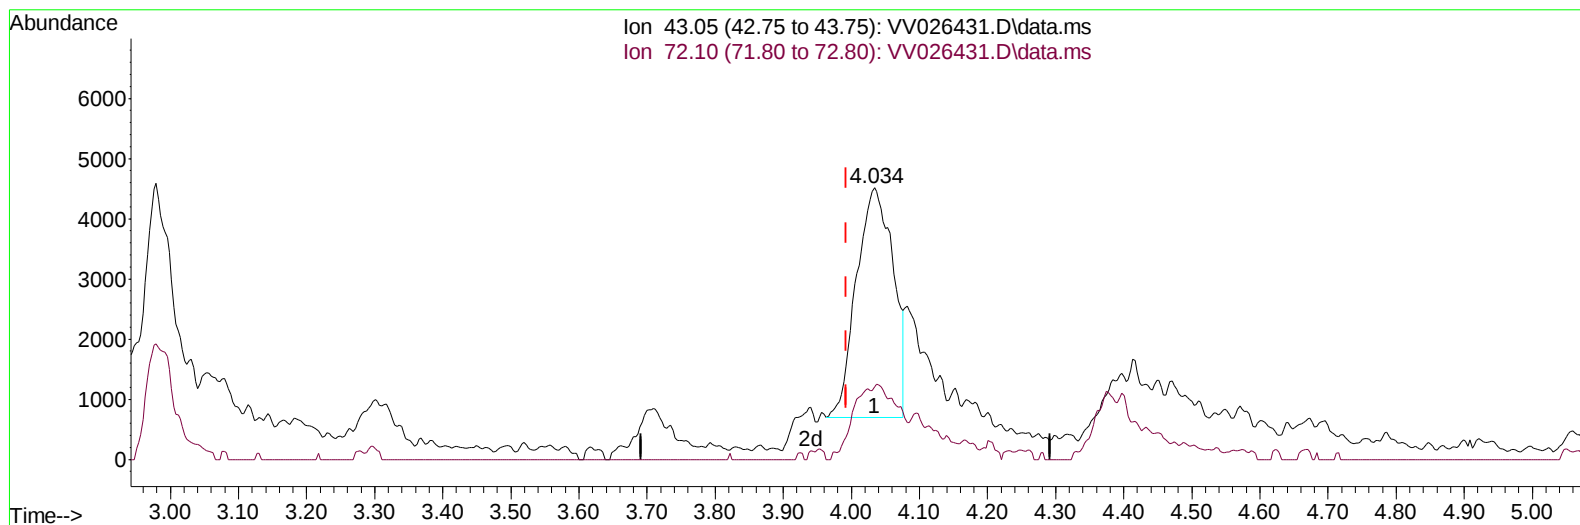

TIC: VV026431.D\data.ms

(21) 2-Butanone (T)

4.034min (+ 0.042) 6.18 ug/L

response 14339

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	15.92
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
 Data File : VV026431.D
 Acq On : 18 Jun 2022 18:35
 Operator : SY/MD
 Sample : N3358-18
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4T1

Manual IntegrationsAPPROVED

Quant Time: Jun 20 01:31:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 20 01:25:22 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/20/2022
 Supervised By :Mahesh Dadoda 06/20/2022

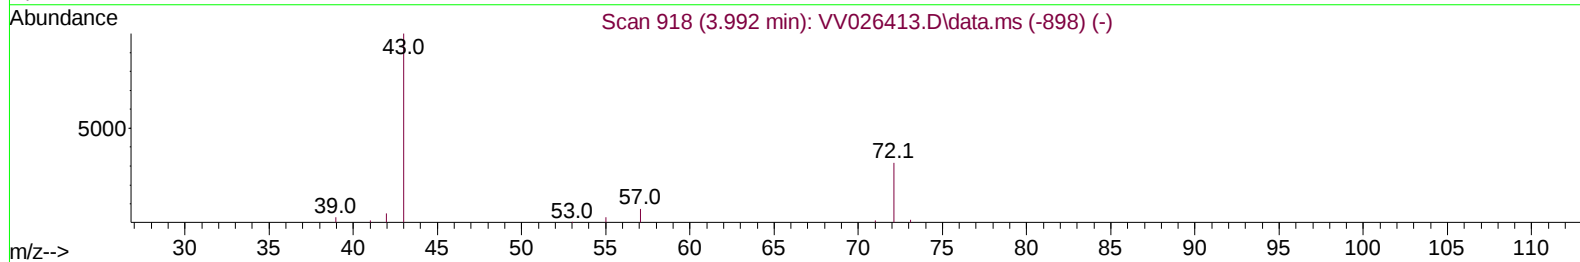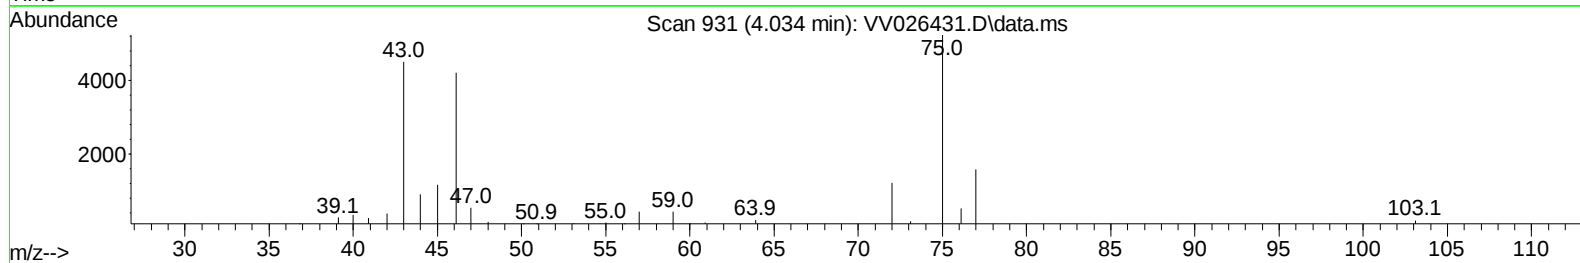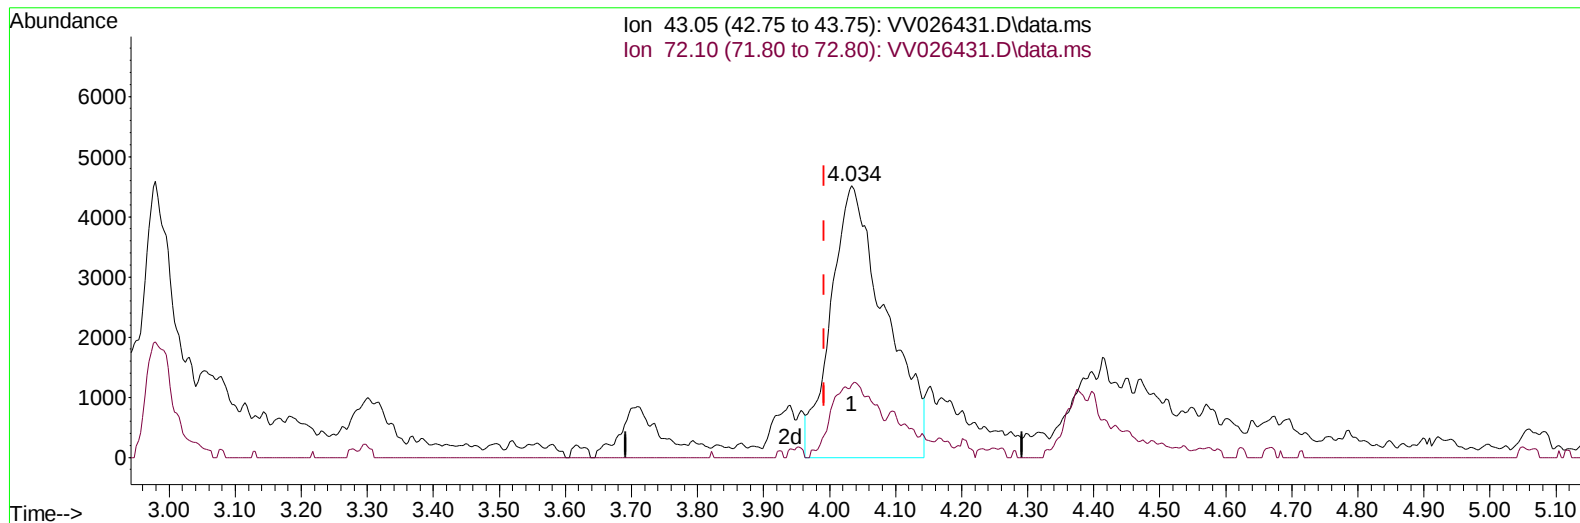

TIC: VV026431.D\data.ms

(21) 2-Butanone (T)

4.034min (+ 0.042) 11.21 ug/L m

response 26035

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	8.77#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
 Data File : VV026431.D
 Acq On : 18 Jun 2022 18:35
 Operator : SY/MD
 Sample : N3358-18
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4T1

Manual IntegrationsAPPROVED

Quant Time: Jun 20 01:31:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 20 01:25:22 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/20/2022
 Supervised By :Mahesh Dadoda 06/20/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.629	114	273205	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	247357	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	125038	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.327	65	101017	4.257	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	85.200%	
7) Chloroethane-d5	1.587	69	71326	3.823	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	76.400%	
11) 1,1-Dichloroethene-d2	2.127	63	122007	2.994	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	59.800%#	
20) 2-Butanone-d5	3.931	46	109404	47.249	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130	Recovery	=	94.500%	
24) Chloroform-d	4.365	84	159785	4.594	ug/L	0.01
Spiked Amount 5.000	Range 70	- 125	Recovery	=	91.800%	
26) 1,2-Dichloroethane-d4	5.047	65	63618	4.323	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	86.400%	
32) Benzene-d6	5.063	84	331128	5.007	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	100.200%	
36) 1,2-Dichloropropane-d6	6.079	67	97588	5.056	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	101.200%	
41) Toluene-d8	7.320	98	329057	5.457	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	109.200%	
43) trans-1,3-Dichloroprop...	7.625	79	30309	4.843	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	96.800%	
46) 2-Hexanone-d5	8.092	63	118215	62.529	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	125.060%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	62263	5.237	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	104.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	102535	5.324	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	106.400%	
Target Compounds						
						Qvalue
13) Acetone	2.220	43	146652	81.727	ug/L	57
14) Carbon disulfide	2.314	76	557105	13.091	ug/L	99
15) Methyl Acetate	2.462	43	84777	19.690	ug/L	93
19) 1,1-Dichloroethane	3.211	63	39445	1.236	ug/L	96
21) 2-Butanone	4.034	43	26035m	11.213	ug/L	
33) Benzene	5.114	78	113979	1.797	ug/L	100
40) 4-Methyl-2-pentanone	7.233	43	231574	37.970	ug/L	99
42) Toluene	7.394	91	74225	1.113	ug/L	100
52) Ethylbenzene	9.018	91	15372	0.230	ug/L	99
53) m,p-Xylene	9.140	106	20002	0.767	ug/L	94
54) o-Xylene	9.548	106	12012	0.476	ug/L	96
62) 1,3,5-Trimethylbenzene	10.538	105	12567	0.238	ug/L	100
63) 1,2,4-Trimethylbenzene	10.915	105	32880	0.628	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
Data File : VV026431.D
Acq On : 18 Jun 2022 18:35
Operator : SY/MD
Sample : N3358-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4T1

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/20/2022
Supervised By :Mahesh Dadoda 06/20/2022

Quant Time: Jun 20 01:31:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 20 01:25:22 2022
Response via : Initial Calibration

