

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061822\
 Data File : VW026419.D
 Acq On : 18 Jun 2022 12:47
 Operator : SY/MD
 Sample : N3275-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jun 20 01:28:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 20 01:25:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	197345	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	179615	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	73948	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	52474	3.061	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	61.200%	
7) Chloroethane-d5	1.584	69	48102	3.569	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	71.400%	
11) 1,1-Dichloroethene-d2	2.124	63	74714	2.538	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	50.800%#	
20) 2-Butanone-d5	3.928	46	86613	51.785	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	103.580%	
24) Chloroform-d	4.362	84	114170	4.544	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.800%	
26) 1,2-Dichloroethane-d4	5.047	65	47335	4.453	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.000%	
32) Benzene-d6	5.063	84	206285	4.296	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.000%	
36) 1,2-Dichloropropane-d6	6.079	67	66112	4.717	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	94.400%	
41) Toluene-d8	7.320	98	158641	3.623	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	72.400%	
43) trans-1,3-Dichloroprop...	7.632	79	13158	2.895	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	58.000%	
46) 2-Hexanone-d5	8.095	63	65862	47.976	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	95.960%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	43795	5.073	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	101.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	55658	4.886	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.800%	
Target Compounds						
16) Methylene chloride	2.526	84	3634	0.228	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
Data File : VV026419.D
Acq On : 18 Jun 2022 12:47
Operator : SY/MD
Sample : N3275-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Jun 20 01:28:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 20 01:25:22 2022
Response via : Initial Calibration

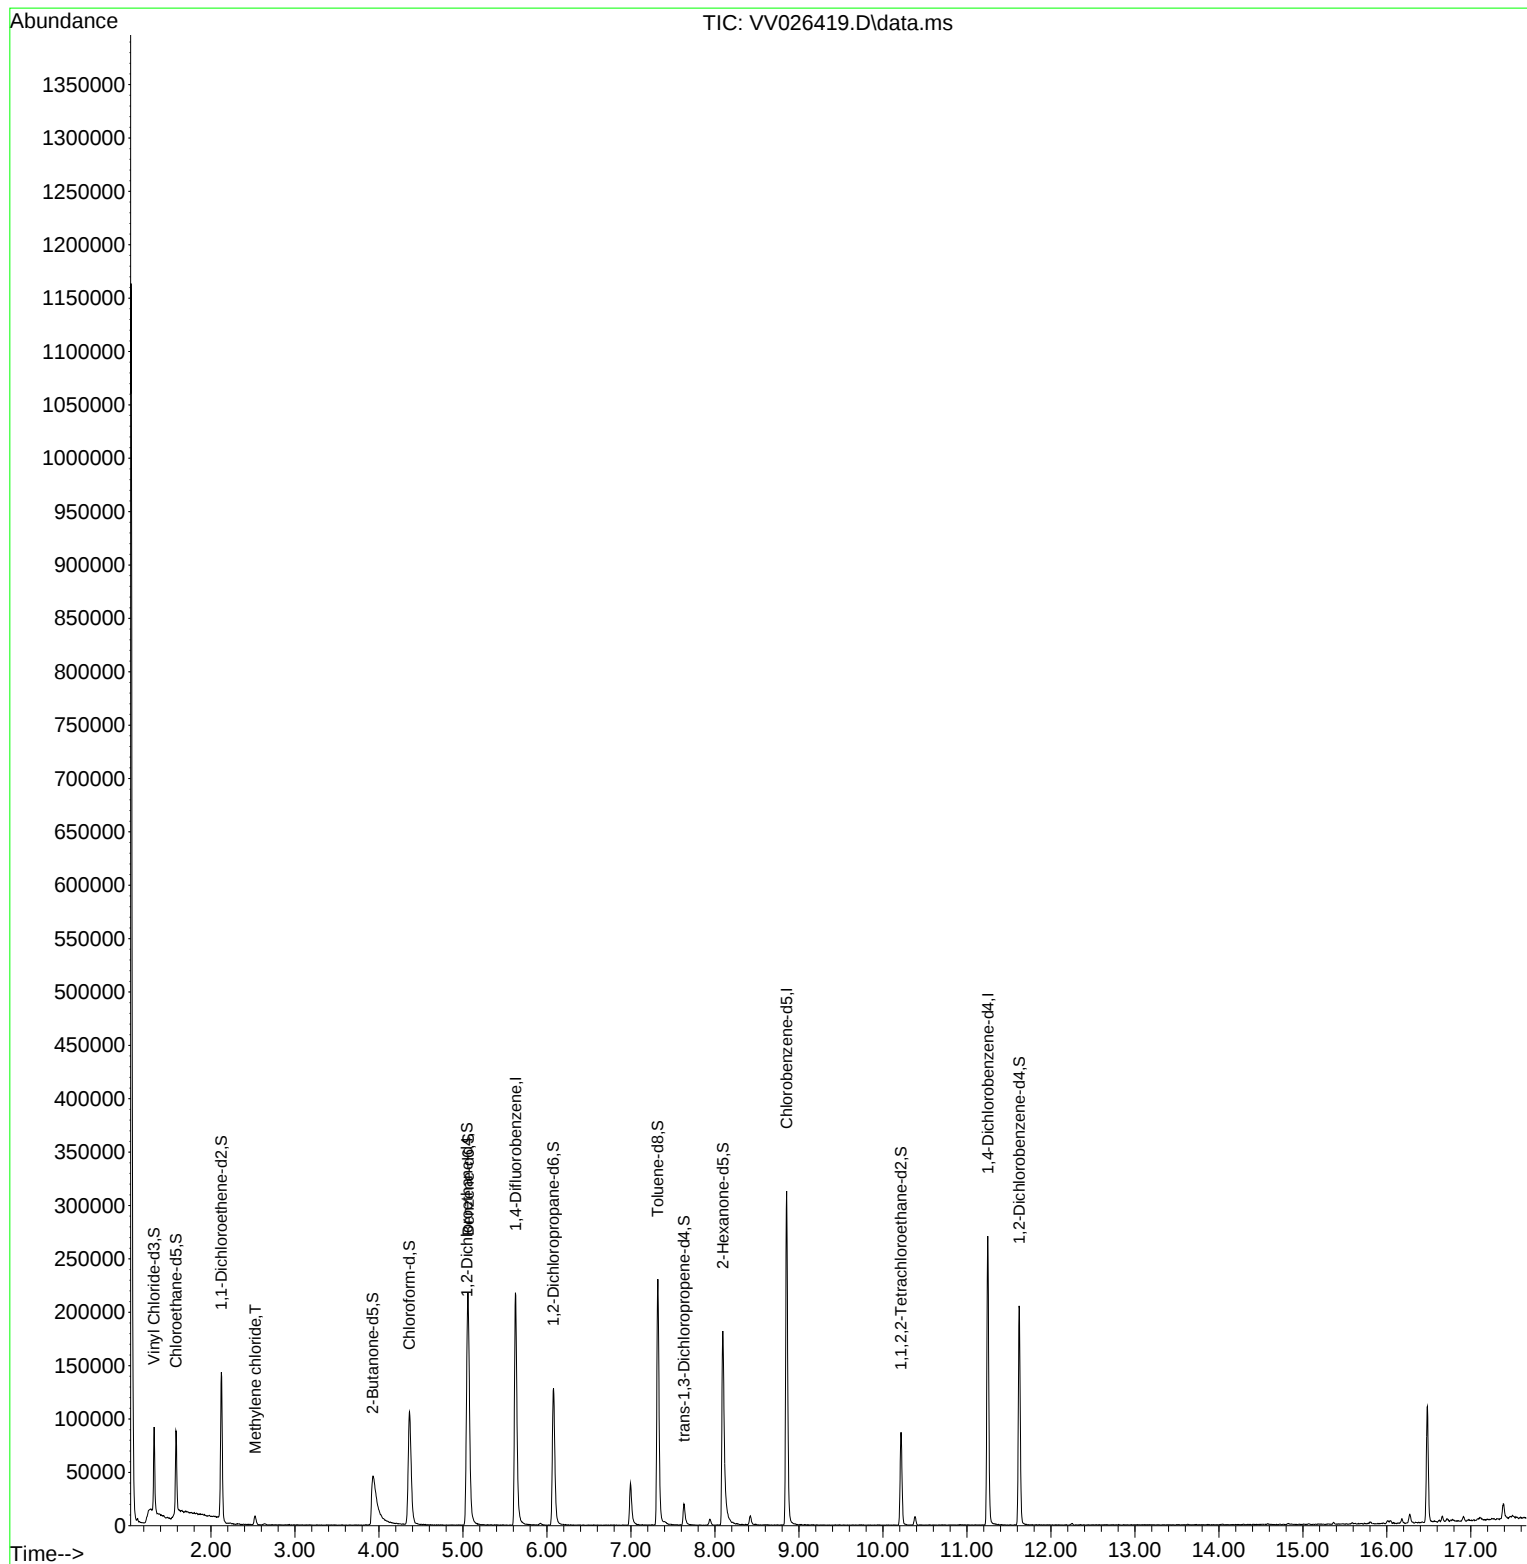

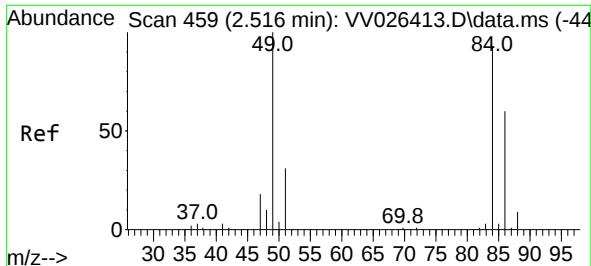

#16
Methylene chloride
Concen: 0.228 ug/L
RT: 2.526 min Scan# 4
Delta R.T. 0.009 min
Lab File: VV026419.D
Acq: 18 Jun 2022 12:47

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

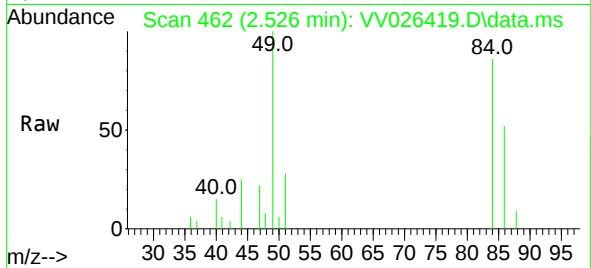

Tgt Ion: 84 Resp: 3634

Ion	Ratio	Lower	Upper
84	100		
86	59.6	44.0	81.8
49	115.6	77.3	143.7

