

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
 Data File : VV026422.D
 Acq On : 18 Jun 2022 13:59
 Operator : SY/MD
 Sample : N3345-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	54	73	77	rBV3	12612	39380	5.68%	0.729%
2	1.323	81	88	102	rVB	122082	140881	20.33%	2.606%
3	1.584	162	169	183	rBV	101839	121522	17.54%	2.248%
4	2.124	327	337	357	rVB	212238	314200	45.35%	5.813%
5	2.311	386	395	409	rVB2	9024	13980	2.02%	0.259%
6	3.925	887	897	927	rBV2	34030	135610	19.57%	2.509%
7	4.365	1016	1034	1063	rBV4	141519	454300	65.57%	8.405%
8	5.056	1232	1249	1287	rBV2	278443	692892	100.00%	12.819%
9	5.625	1414	1426	1450	rBV	222252	447706	64.61%	8.283%
10	6.076	1553	1566	1592	rBV	154345	321439	46.39%	5.947%
11	6.584	1713	1724	1740	rBV4	4563	10132	1.46%	0.187%
12	6.992	1841	1851	1874	rBV	51250	98481	14.21%	1.822%
13	7.320	1942	1953	1970	rBV	329696	577291	83.32%	10.680%
14	7.400	1972	1978	1993	rVB2	12420	23393	3.38%	0.433%
15	7.629	2038	2049	2071	rBV	27651	51712	7.46%	0.957%
16	7.941	2135	2146	2157	rBV3	5626	9749	1.41%	0.180%
17	8.095	2184	2194	2236	rBV2	185891	386520	55.78%	7.151%
18	8.854	2417	2430	2455	rBV	324715	532901	76.91%	9.859%
19	10.217	2842	2854	2867	rBV	93765	150254	21.69%	2.780%
20	10.381	2895	2905	2917	rBV2	12138	20208	2.92%	0.374%
21	11.249	3163	3175	3192	rBV	281786	441895	63.78%	8.176%
22	11.622	3279	3291	3310	rBV	256018	405766	58.56%	7.507%
23	16.484	4795	4803	4814	rVB2	9856	14899	2.15%	0.276%




Sum of corrected areas: 5405111

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
Data File : VV026422.D
Acq On : 18 Jun 2022 13:59
Operator : SY/MD
Sample : N3345-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

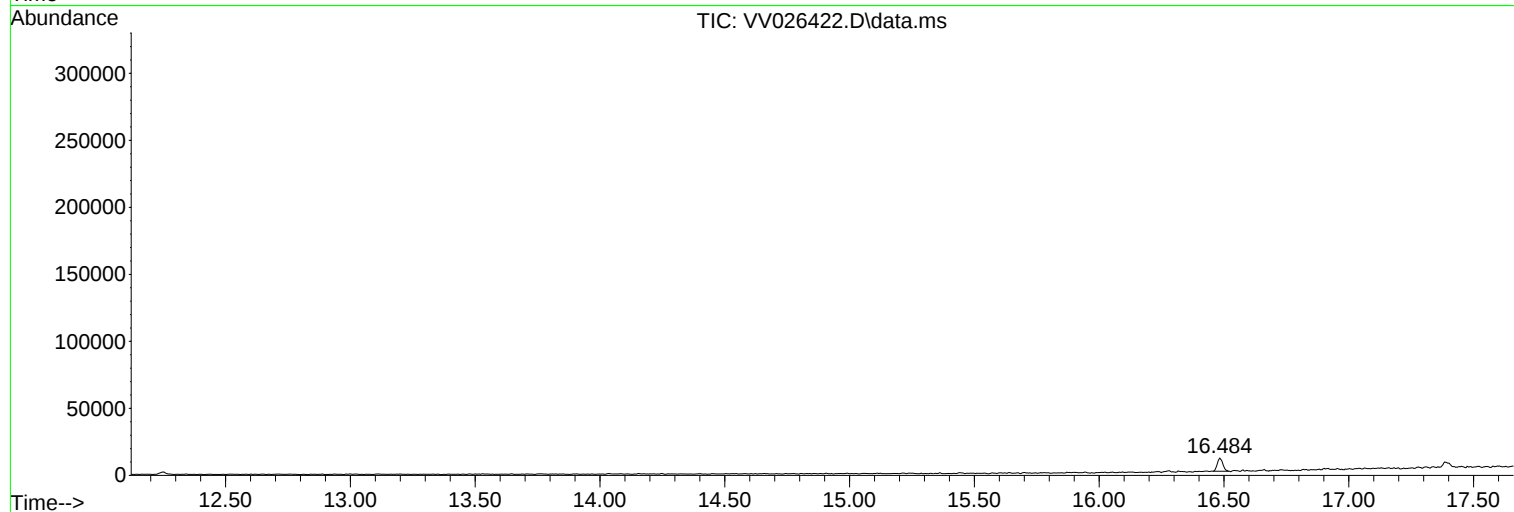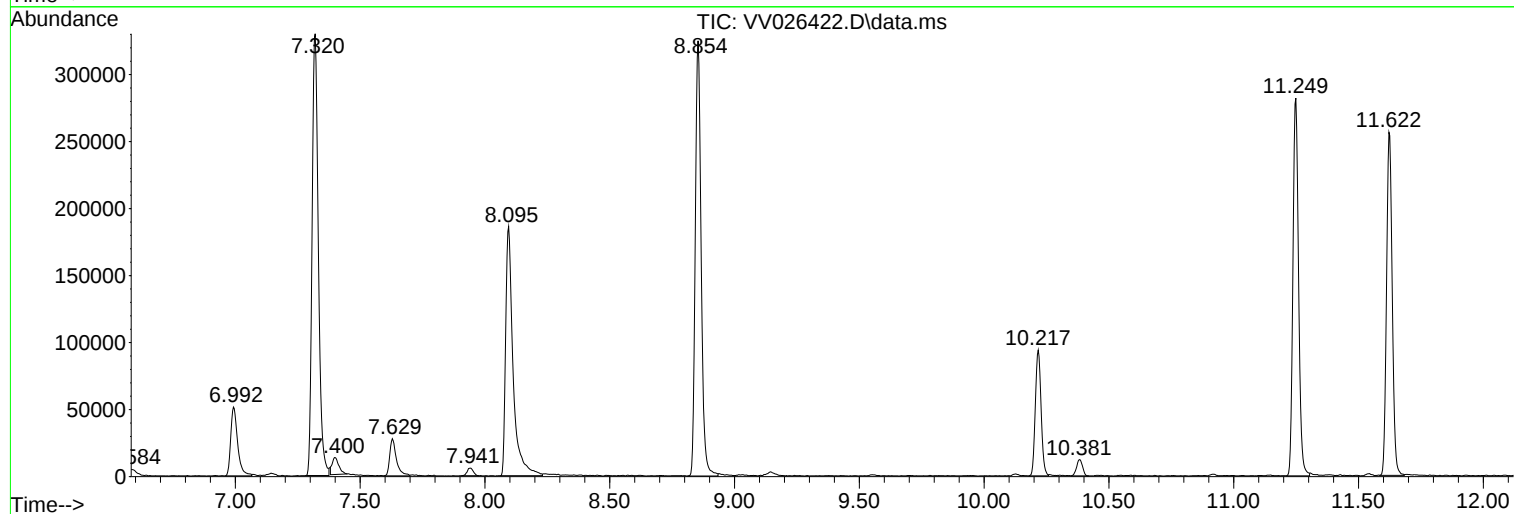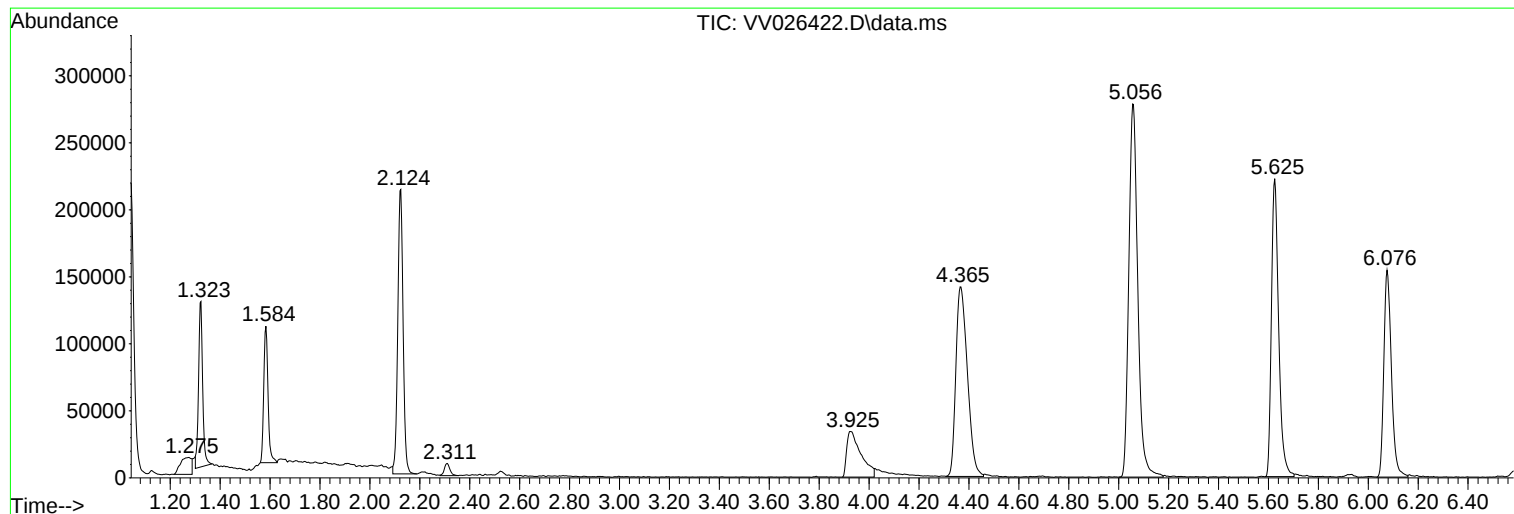

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
Data File : VV026422.D
Acq On : 18 Jun 2022 13:59
Operator : SY/MD
Sample : N3345-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
Data File : VV026422.D
Acq On : 18 Jun 2022 13:59
Operator : SY/MD
Sample : N3345-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc