

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
 Data File : VV026429.D
 Acq On : 18 Jun 2022 17:47
 Operator : SY/MD
 Sample : N3358-20
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4T3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026429.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	22	27	39	rVB	40734	42139	4.96%	0.631%
2	1.233	51	60	63	rBV	30319	37940	4.47%	0.568%
3	1.323	81	88	110	rVB	164180	190167	22.39%	2.847%
4	1.433	115	122	133	rVB	56530	66906	7.88%	1.002%
5	1.539	139	155	157	rBV2	18461	41897	4.93%	0.627%
6	1.584	162	169	183	rVB	118911	148045	17.43%	2.216%
7	2.124	327	337	358	rVB	238322	354593	41.75%	5.308%
8	3.928	887	898	942	rBV2	42258	191032	22.49%	2.860%
9	4.362	1017	1033	1063	rBV	148717	389605	45.87%	5.833%
10	5.056	1235	1249	1284	rBV2	340928	849321	100.00%	12.715%
11	5.625	1414	1426	1456	rBV	277809	570183	67.13%	8.536%
12	6.076	1554	1566	1602	rBV	186072	395737	46.59%	5.924%
13	6.992	1838	1851	1872	rBV2	66428	126496	14.89%	1.894%
14	7.320	1940	1953	1970	rBV	421017	732167	86.21%	10.961%
15	7.629	2039	2049	2069	rBV	34190	62285	7.33%	0.932%
16	8.095	2181	2194	2235	rBV	230834	483832	56.97%	7.243%
17	8.854	2418	2430	2462	rBV	400963	658843	77.57%	9.863%
18	9.143	2509	2520	2533	rBV	34015	58463	6.88%	0.875%
19	10.217	2843	2854	2871	rBV	116641	184081	21.67%	2.756%
20	11.249	3164	3175	3194	rBV	370421	567954	66.87%	8.503%
21	11.622	3280	3291	3307	rBV	329011	528093	62.18%	7.906%




Sum of corrected areas: 6679779

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
Data File : VV026429.D
Acq On : 18 Jun 2022 17:47
Operator : SY/MD
Sample : N3358-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4T3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

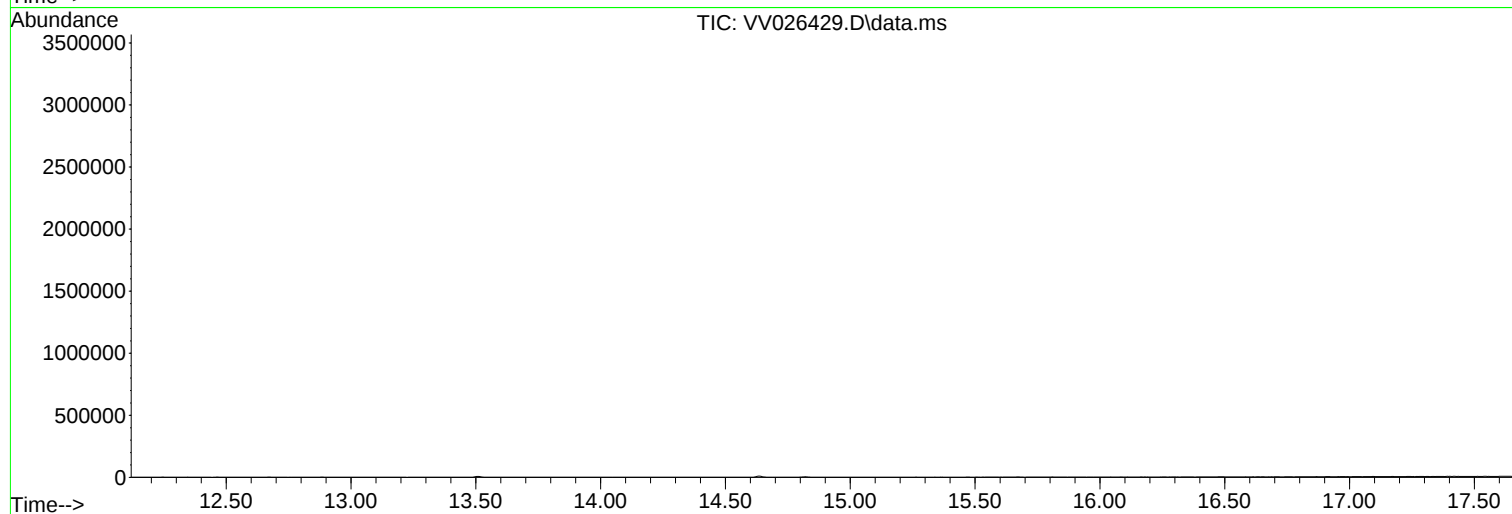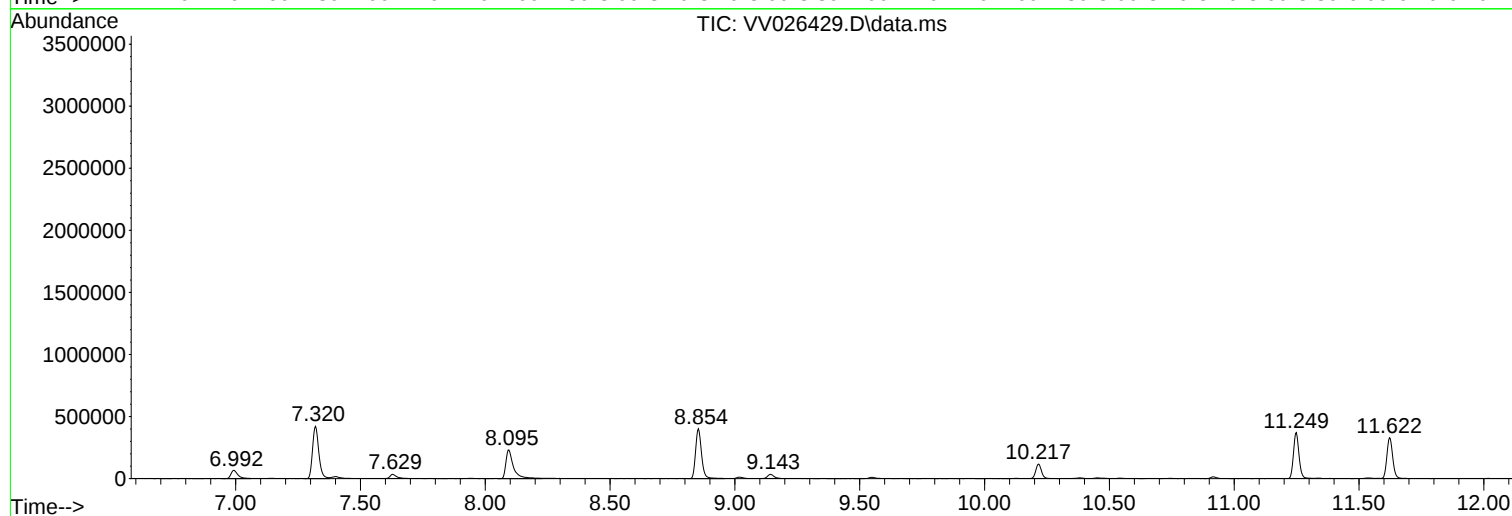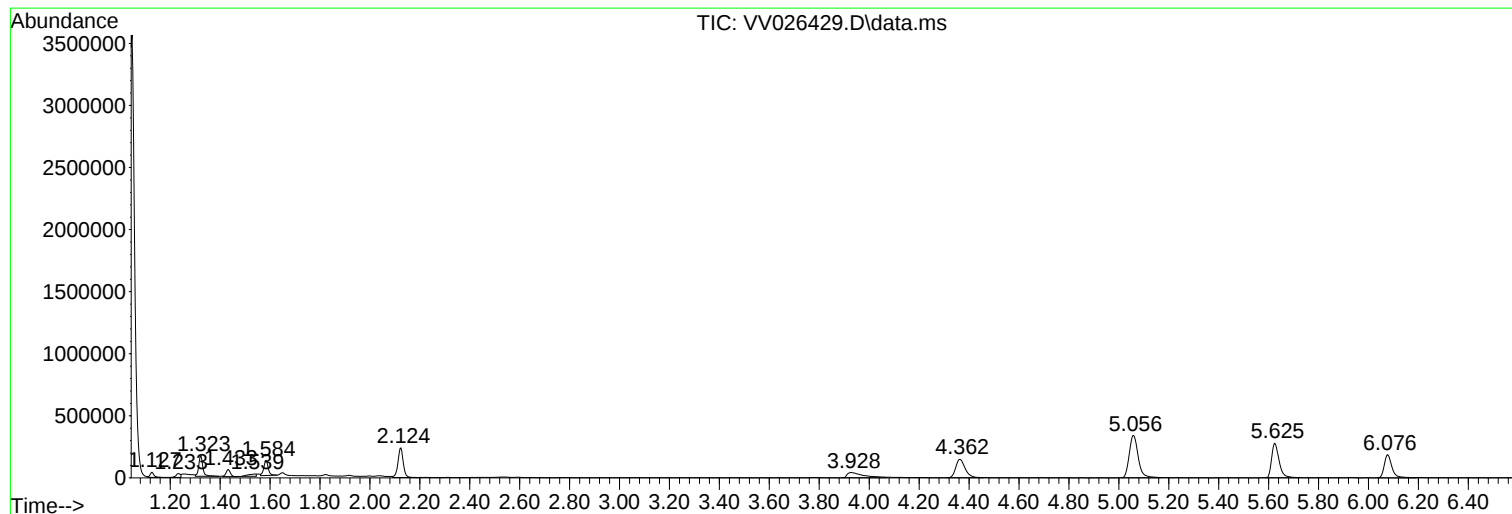

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
Data File : VV026429.D
Acq On : 18 Jun 2022 17:47
Operator : SY/MD
Sample : N3358-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4T3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
Data File : VV026429.D
Acq On : 18 Jun 2022 17:47
Operator : SY/MD
Sample : N3358-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4T3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc