


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061822\
 Data File : VV026412.D
 Acq On : 18 Jun 2022 09:17
 Operator : SY/MD
 Sample : BFB332
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB332

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Jun 21 05:26:17 2022

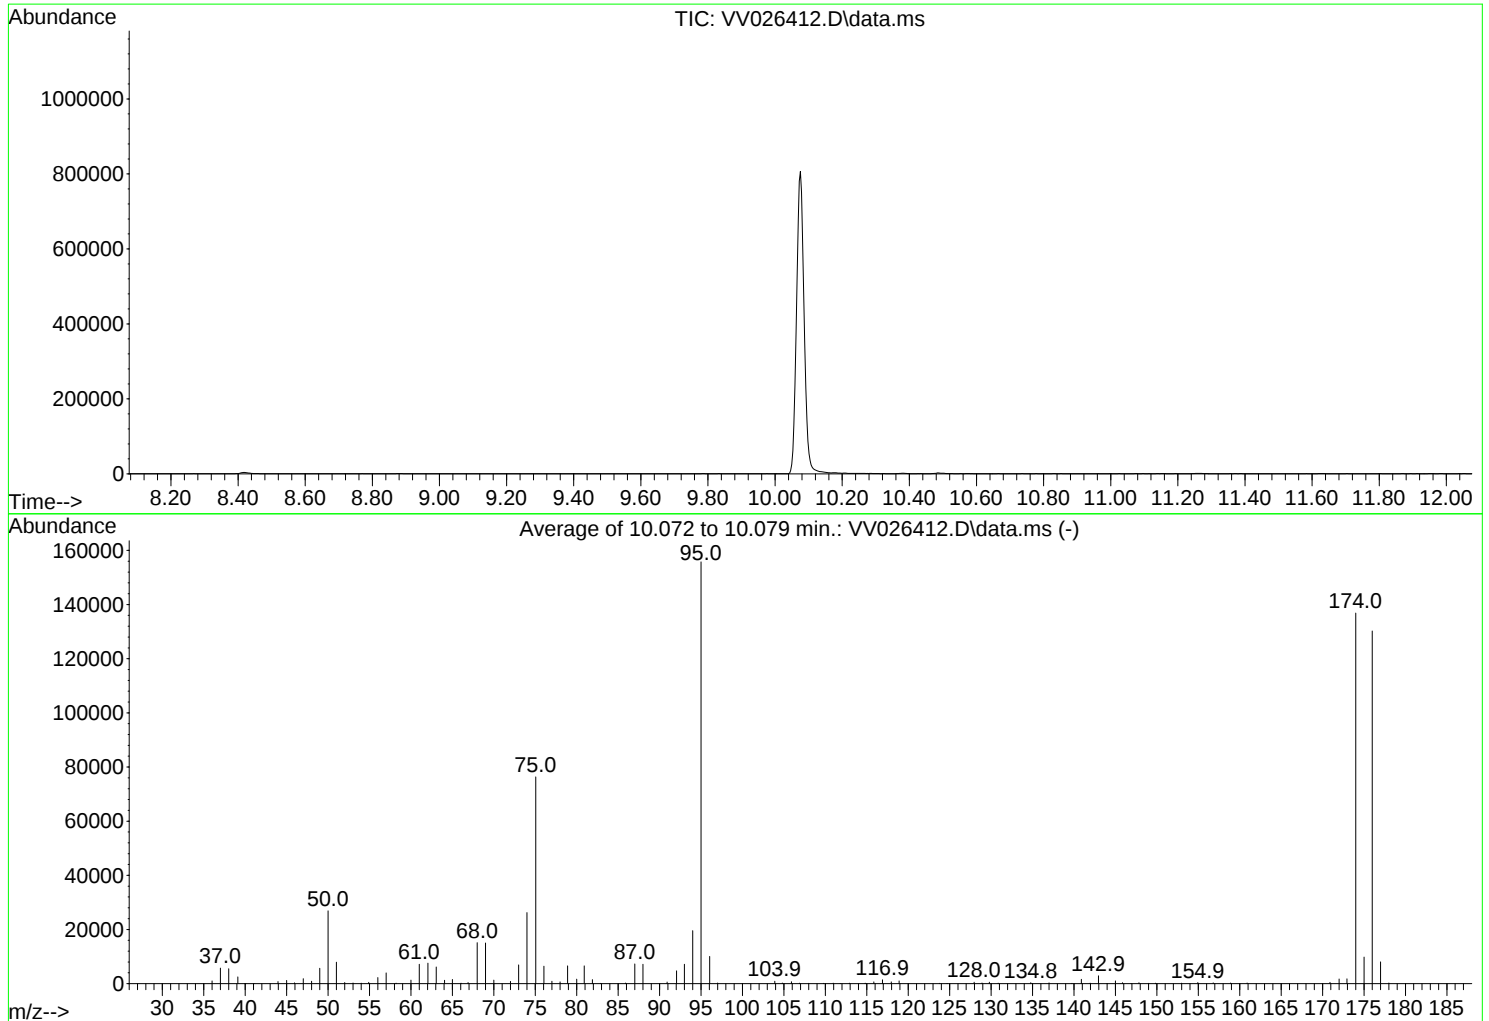

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	26904	PASS
75	95	30	80	49.0	76331	PASS
95	95	100	100	100.0	155776	PASS
96	95	5	9	6.5	10052	PASS
173	174	0.00	2	1.3	1769	PASS
174	95	50	120	87.9	136875	PASS
175	174	5	9	7.2	9844	PASS
176	174	95	105	95.2	130256	PASS
177	176	5	10	6.2	8043	PASS

m/z	Abundance
39.90	285.0
43.90	255.0

Instrument :
MSVOA_V
ClientSampleId :
BFB332

m/z	Abundance
36.00	1035.0
37.00	5687.0
38.00	5655.0
39.10	2271.0
40.20	333.0
41.10	133.0
44.00	1124.0
45.00	1272.0
46.00	351.0
47.00	1706.0
48.00	963.0
49.00	5732.0
50.00	27496.0
51.00	8018.0
52.00	441.0
53.00	207.0
54.00	198.0
54.90	441.0
56.00	2356.0
57.00	3954.0
58.20	167.0
60.00	1406.0
61.00	7483.0
62.00	7667.0
63.10	6248.0
64.00	1244.0
65.00	1491.0
66.00	122.0
66.90	429.0
68.00	15433.0
69.00	15315.0
70.00	1376.0
72.00	879.0
73.00	7056.0
74.00	26432.0
75.00	77832.0
76.00	6405.0
77.00	834.0
78.00	653.0
78.90	6661.0
80.00	1668.0
80.90	6713.0
81.90	1452.0
82.90	140.0
85.90	227.0
87.00	7385.0
88.00	6828.0
90.80	543.0
92.00	4694.0
93.00	7082.0
94.00	19736.0
95.00	156928.0
96.10	10198.0
97.00	281.0
103.90	909.0
104.80	203.0
105.90	733.0
106.90	174.0
108.00	120.0
109.80	154.0
111.00	144.0
112.90	144.0
114.80	145.0
115.90	677.0
116.90	1387.0
118.00	605.0
118.90	1000.0
123.80	148.0
128.00	513.0
129.00	238.0
129.80	574.0
130.90	230.0
134.80	358.0
137.00	232.0
139.80	119.0
140.90	1608.0
141.90	219.0
142.90	2839.0
145.00	1129.0
145.90	324.0
146.90	116.0
147.90	316.0
149.90	206.0
153.00	182.0
155.00	429.0
156.80	272.0
158.90	168.0
160.90	237.0
170.90	506.0
172.00	1632.0
172.90	1847.0
174.00	134784.0

Instrument :
MSVOA_V
ClientSampleId :
BFB332

175.00	9877.0
176.00	128312.0
177.00	8142.0
178.00	256.0

Instrument :
MSVOA_V
ClientSampleId :
BFB332

m/z	Abundance
36.00	1040.0
37.00	5931.0
38.00	5604.0
39.10	2562.0
40.00	308.0
41.00	129.0
44.00	1064.0
45.00	1222.0
45.90	334.0
47.00	1899.0
48.00	958.0
49.00	5946.0
50.00	27960.0
51.00	8174.0
52.00	456.0
53.00	233.0
54.00	196.0
54.90	503.0
56.00	2349.0
57.00	4065.0
58.20	187.0
60.00	1342.0
61.00	7371.0
62.10	7781.0
63.00	6356.0
64.10	1275.0
65.00	1635.0
66.10	174.0
66.90	422.0
68.00	15687.0
69.00	15572.0
70.00	1326.0
72.00	858.0
73.00	7189.0
74.00	27208.0
75.00	79088.0
76.10	6623.0
77.00	890.0
78.00	635.0
78.90	6786.0
80.00	1688.0
80.90	6818.0
81.90	1557.0
82.90	135.0
85.90	223.0
87.00	7502.0
88.00	7479.0
90.90	596.0
92.10	4957.0
93.00	7383.0
94.00	20344.0
95.00	161024.0
96.00	10408.0
97.00	267.0
103.90	950.0
104.80	225.0
105.90	772.0
106.90	212.0
108.00	159.0
109.80	142.0
111.00	174.0
112.90	167.0
114.80	183.0
115.90	698.0
116.90	1443.0
117.90	666.0
118.90	1057.0
123.80	140.0
124.70	122.0
127.90	562.0
128.90	225.0
129.80	559.0
130.90	216.0
134.80	347.0
137.00	272.0
139.80	130.0
140.90	1655.0
142.00	208.0
143.00	3039.0
145.00	1035.0
145.80	392.0
146.90	101.0
147.80	334.0
149.00	136.0
149.80	206.0
153.00	162.0
155.00	461.0
156.80	301.0
158.90	232.0
160.90	295.0
170.90	463.0
172.00	1761.0

Instrument :
MSVOA_V
ClientSampleId :
BFB332

172.90	1858.0
174.00	141440.0
175.00	10156.0
176.00	134592.0
177.00	8298.0
178.00	233.0

Instrument :
MSVOA_V
ClientSampleId :
BFB332

m/z	Abundance
36.00	980.0
37.00	5557.0
38.00	5189.0
39.10	2553.0
40.00	280.0
44.00	913.0
45.00	1091.0
46.00	262.0
47.00	1864.0
48.00	824.0
49.00	5351.0
50.00	25256.0
51.00	7500.0
52.00	425.0
53.00	224.0
54.00	170.0
54.90	480.0
56.00	2120.0
57.00	3809.0
58.20	166.0
60.00	1121.0
61.00	6552.0
62.10	7259.0
63.00	5827.0
64.10	1138.0
65.00	1479.0
66.10	203.0
66.90	337.0
68.00	14258.0
69.00	14212.0
70.00	1211.0
72.00	783.0
73.00	6576.0
74.00	25104.0
75.10	72072.0
76.10	6329.0
77.00	889.0
78.00	596.0
78.90	6215.0
80.00	1559.0
80.90	6152.0
81.90	1456.0
82.90	132.0
85.90	219.0
87.00	6918.0
88.00	7242.0
91.00	622.0
92.00	4540.0
93.00	6930.0
94.00	18664.0
95.00	149376.0
96.00	9550.0
97.00	249.0
103.90	813.0
104.80	244.0
105.90	711.0
106.90	222.0
108.00	164.0
109.80	109.0
110.90	163.0
111.80	119.0
112.90	183.0
114.80	235.0
115.80	669.0
116.90	1381.0
117.90	730.0
118.90	1035.0
123.80	113.0
127.90	606.0
128.80	266.0
129.80	540.0
130.80	185.0
134.80	283.0
137.00	323.0
139.70	114.0
140.90	1532.0
142.00	179.0
143.00	2782.0
144.00	130.0
145.00	925.0
145.80	399.0
147.80	345.0
149.00	151.0
149.80	197.0
153.00	140.0
154.90	442.0
156.80	288.0
158.90	260.0
160.90	262.0
170.90	385.0
172.00	1742.0
173.00	1602.0

Instrument :
MSVOA_V
ClientSampleId :
BFB332

174.00	134400.0
175.00	9498.0
176.00	127864.0
177.00	7688.0
178.00	194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB332