




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061924\
Data File : VV036130.D
Acq On : 19 Jun 2024 09:47
Operator : SY/MD
Sample : VSTDCCC025
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
LabSampleId :
VSTDCCC025

Manual IntegrationsAPPROVED

Quant Time: Jun 20 04:57:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 19 03:24:16 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/22/2024
Supervised By :Mahesh Dadoda 06/22/2024

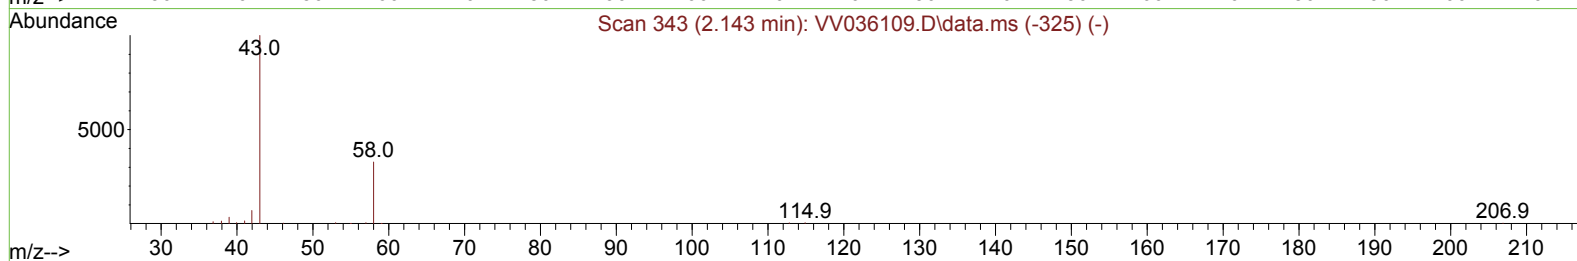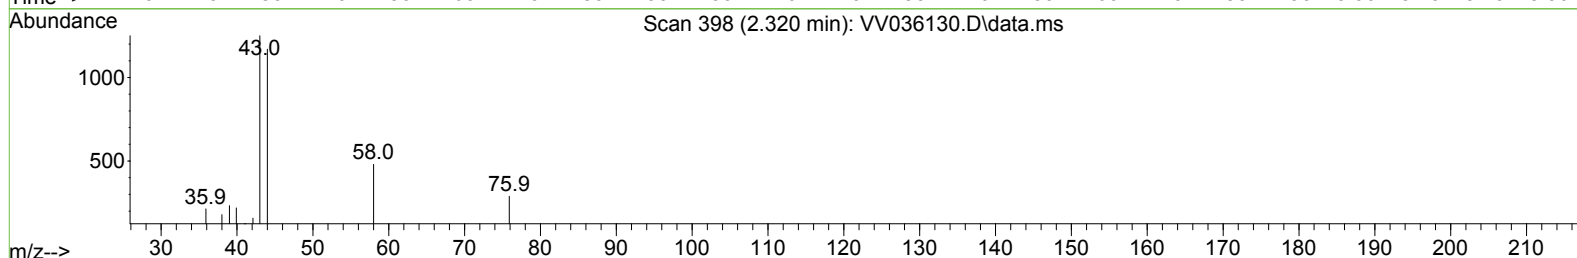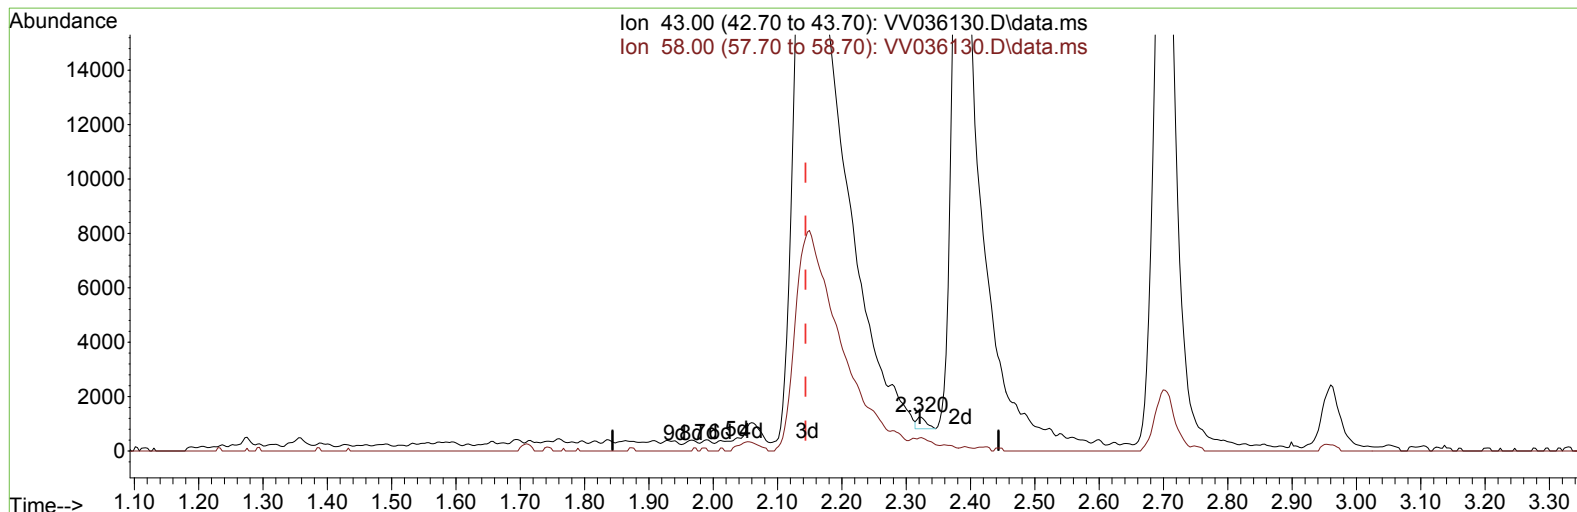

TIC: VV036130.D\data.ms

(13) Acetone (T)

2.320min (+ 0.177) 0.22 ug/L

response 440

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	12.10	11.36
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061924\
Data File : VV036130.D
Acq On : 19 Jun 2024 09:47
Operator : SY/MD
Sample : VSTDCCC025
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
LabSampleId :
VSTDCCC025

Manual IntegrationsAPPROVED

Quant Time: Jun 20 04:57:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 19 03:24:16 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/22/2024
Supervised By :Mahesh Dadoda 06/22/2024

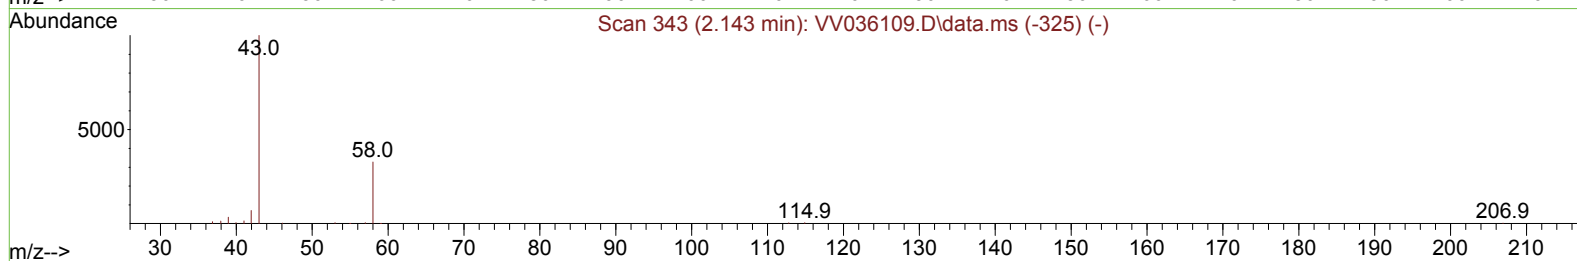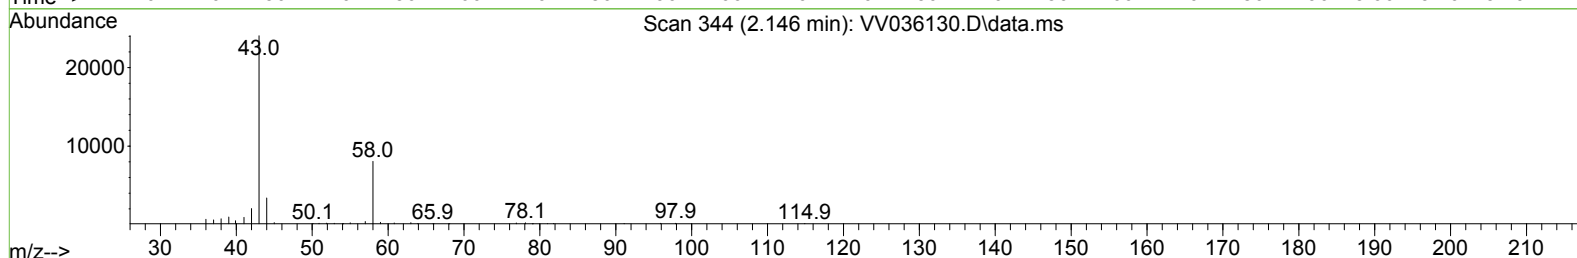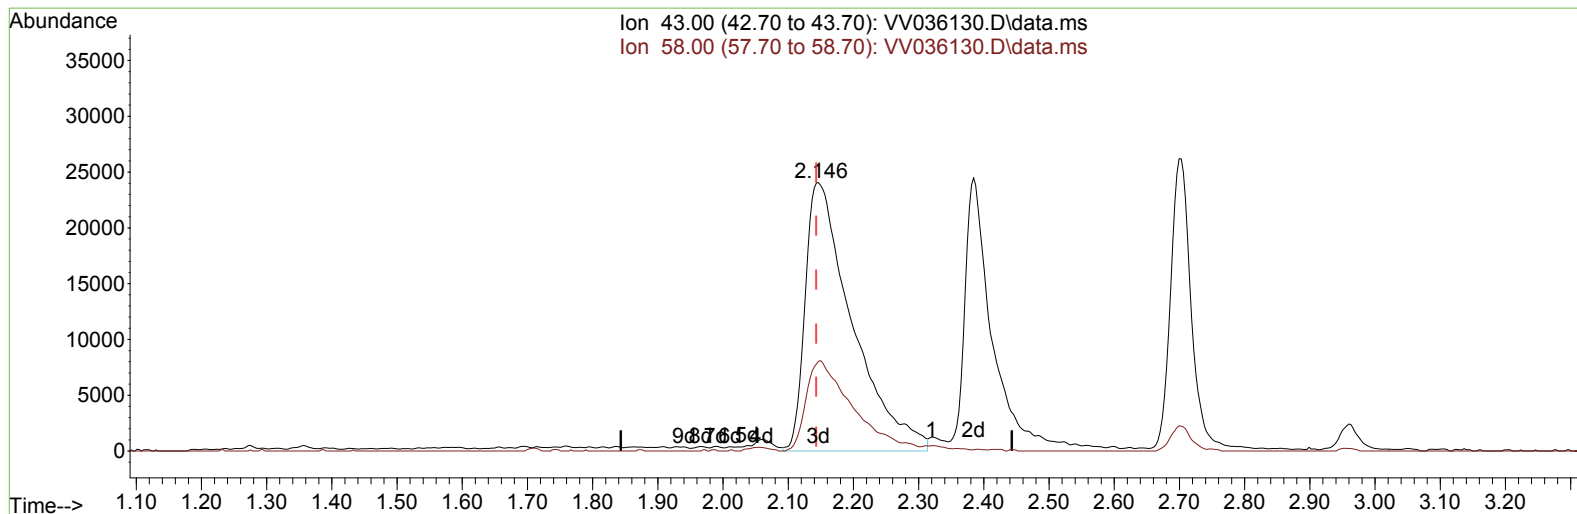

TIC: VV036130.D\data.ms

(13) Acetone (T)

2.146min (+ 0.003) 60.86 ug/L m

response 120354

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	12.10	0.04
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061924\
Data File : VV036130.D
Acq On : 19 Jun 2024 09:47
Operator : SY/MD
Sample : VSTDCCC025
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
LabSampleId :
VSTDCCC025

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/22/2024
Supervised By :Mahesh Dadoda 06/22/2024

Quant Time: Jun 20 04:57:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 19 03:24:16 2024
Response via : Initial Calibration

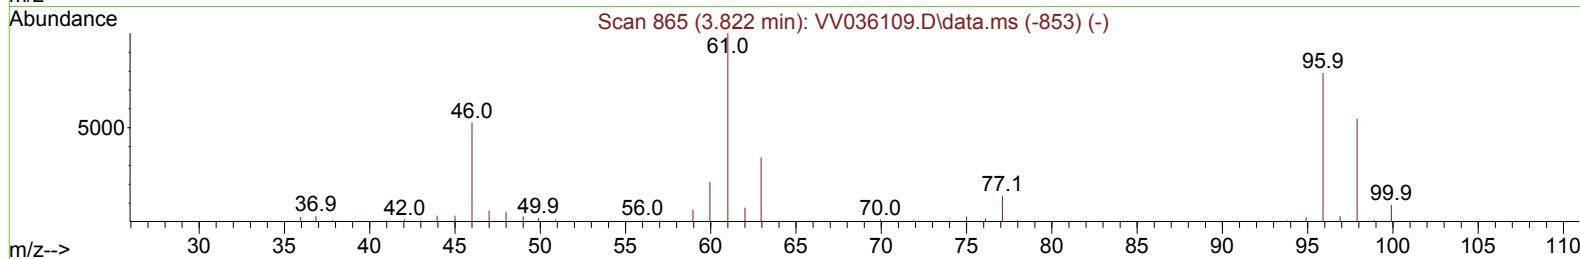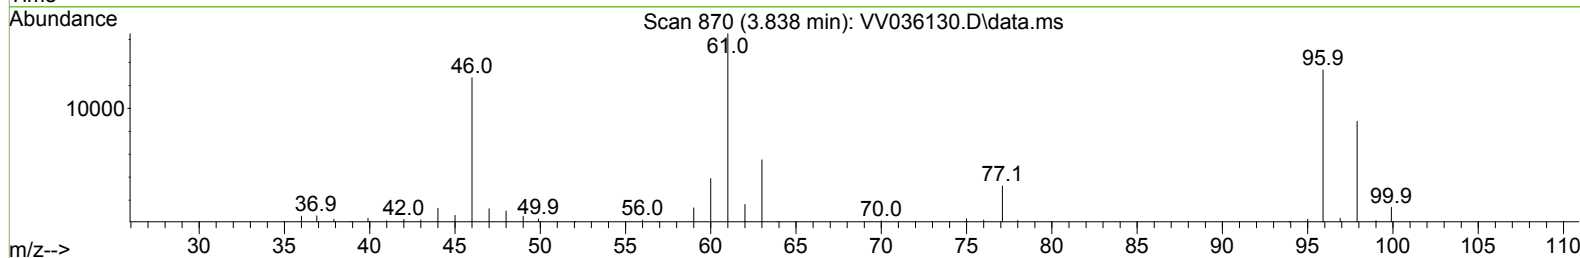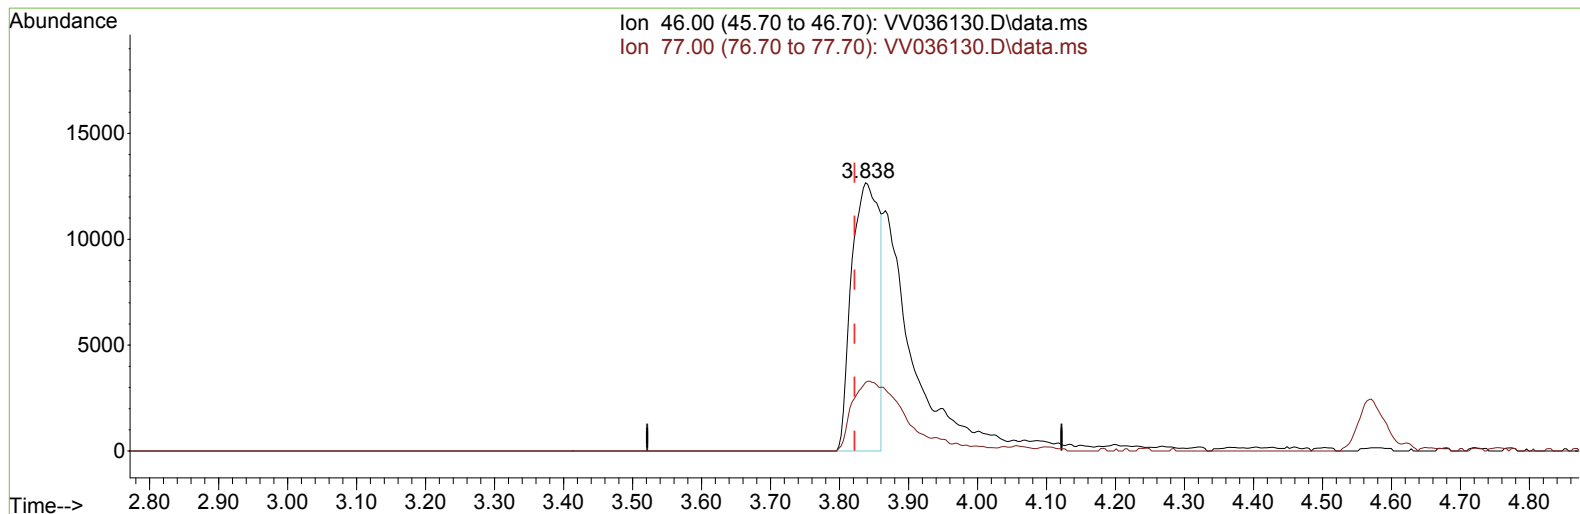

TIC: VV036130.D\data.ms

(21) 2-Butanone-d5 (S)

3.838min (+ 0.016) 27.48 ug/L

response 34880

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.90	26.09#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061924\
Data File : VV036130.D
Acq On : 19 Jun 2024 09:47
Operator : SY/MD
Sample : VSTDCCC025
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
LabSampleId :
VSTDCCC025

Manual IntegrationsAPPROVED

Quant Time: Jun 20 04:57:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 19 03:24:16 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/22/2024
Supervised By :Mahesh Dadoda 06/22/2024

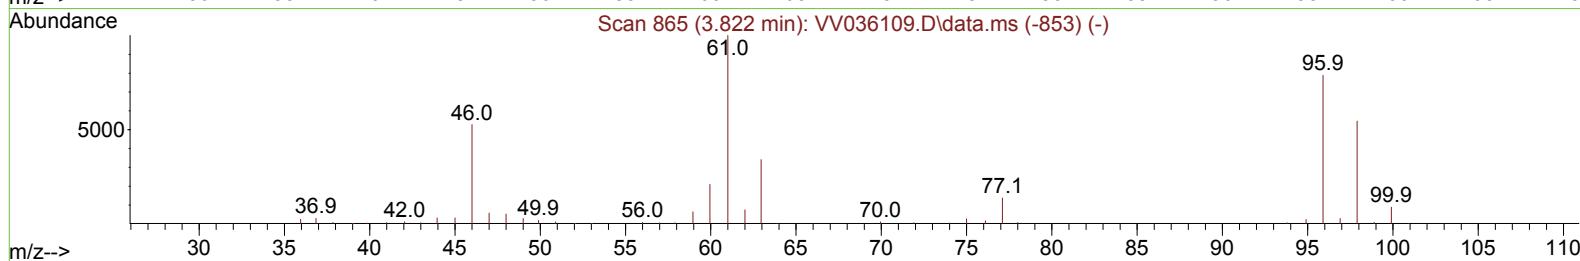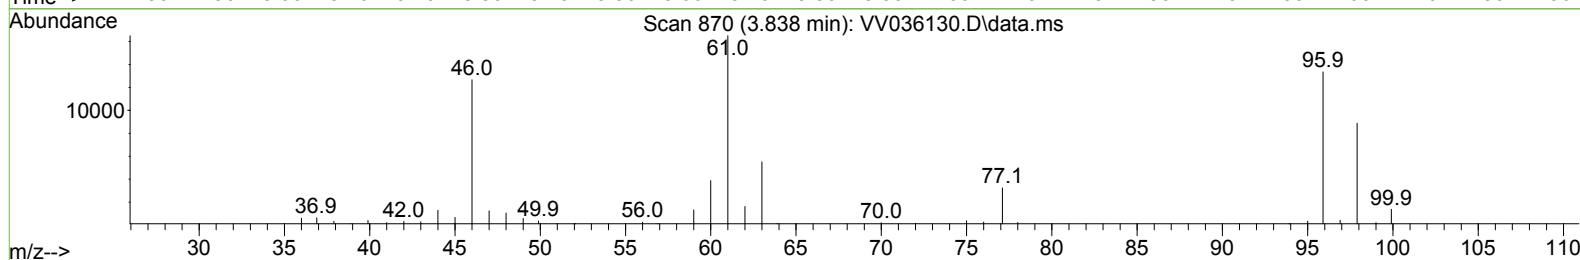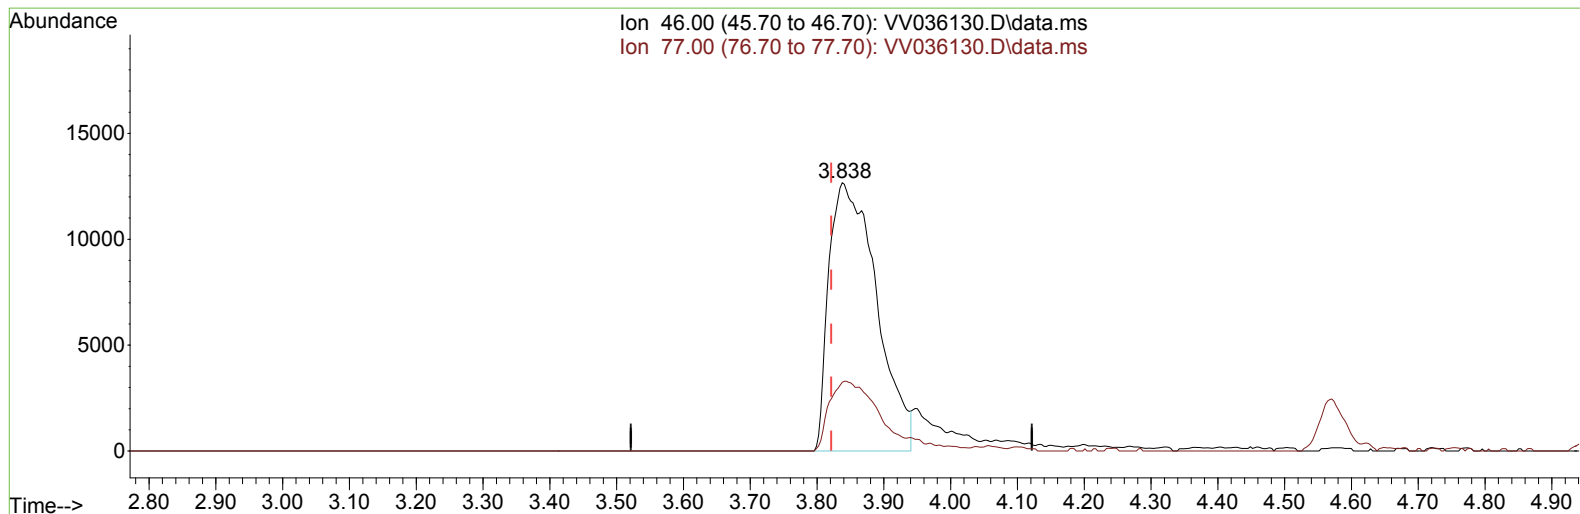

TIC: VV036130.D\data.ms

(21) 2-Butanone-d5 (S)

3.838min (+ 0.016) 49.35 ug/L m

response 62652

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.90	14.52
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061924\
 Data File : VW036130.D
 Acq On : 19 Jun 2024 09:47
 Operator : SY/MD
 Sample : VSTDCCC025
 Misc : 5.00g/10.0mL/MSVOA_V/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 LabSampleId :
 VSTDCCC025

Manual IntegrationsAPPROVED

Quant Time: Jun 20 04:57:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 19 03:24:16 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/22/2024
 Supervised By :Mahesh Dadoda 06/22/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	300956	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	308529	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	167129	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	123830	22.380	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.520%
7) Chloroethane-d5	1.526	69	102521	23.237	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.960%
11) 1,1-Dichloroethene-d2	2.050	65	56850	23.080	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	92.320%
21) 2-Butanone-d5	3.838	46	62652m	49.352	ug/L	0.02
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.700%
24) Chloroform-d	4.240	84	232462	24.296	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.200%
26) 1,2-Dichloroethane-d4	4.937	65	125439	25.005	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.000%
32) Benzene-d6	4.953	84	433908	23.660	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.640%
36) 1,2-Dichloropropane-d6	5.982	67	139755	24.198	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.800%
41) Toluene-d8	7.239	98	396751	24.518	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.080%
43) trans-1,3-Dichloroprop...	7.551	79	56994	24.068	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.280%
47) 2-Hexanone-d5	8.030	63	40869	52.230	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.460%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	109851	25.454	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.800%
66) 1,2-Dichlorobenzene-d4	11.558	152	136563	22.282	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.120%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.101	85	120507	22.207	ug/L	99
3) Chloromethane	1.211	50	150820	24.218	ug/L	100
5) Vinyl chloride	1.278	62	159711	24.360	ug/L	100
6) Bromomethane	1.484	94	104960	25.806	ug/L	100
8) Chloroethane	1.545	64	102977	25.269	ug/L	99
9) Trichlorofluoromethane	1.706	101	208636	25.625	ug/L	99
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	130836	25.320	ug/L	99
12) 1,1-Dichloroethene	2.060	96	122726	25.465	ug/L	95
13) Acetone	2.146	43	120354m	60.862	ug/L	
14) Carbon disulfide	2.230	76	406637	24.297	ug/L	99
15) Methyl Acetate	2.384	43	61393	24.977	ug/L	98
16) Methylene chloride	2.439	84	147645	21.681	ug/L	99
17) trans-1,2-Dichloroethene	2.687	96	126979	24.803	ug/L	98
18) Methyl tert-butyl Ether	2.703	73	294539	25.628	ug/L	99
19) 1,1-Dichloroethane	3.101	63	246556	25.290	ug/L	99
20) cis-1,2-Dichloroethene	3.809	96	125541	24.405	ug/L	100
22) 2-Butanone	3.908	43	88999	53.040	ug/L	87
23) Bromochloromethane	4.140	128	65658	25.446	ug/L	99
25) Chloroform	4.268	83	253747	25.302	ug/L	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061924\
 Data File : VV036130.D
 Acq On : 19 Jun 2024 09:47
 Operator : SY/MD
 Sample : VSTDCCC025
 Misc : 5.00g/10.0mL/MSVOA_V/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 LabSampleId :
 VSTDCCC025

Manual IntegrationsAPPROVED

Quant Time: Jun 20 04:57:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 19 03:24:16 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/22/2024
 Supervised By :Mahesh Dadoda 06/22/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
27) 1,2-Dichloroethane	5.037	62	168247	26.871	ug/L	100
29) Cyclohexane	4.574	56	171037	23.283	ug/L	99
30) 1,1,1-Trichloroethane	4.503	97	206739	24.511	ug/L	98
31) Carbon tetrachloride	4.725	117	181712	24.557	ug/L	100
33) Benzene	5.002	78	521804	25.859	ug/L	100
34) Trichloroethene	5.825	95	153120	24.759	ug/L	99
35) Methylcyclohexane	6.043	83	201007	23.503	ug/L	99
37) 1,2-Dichloropropane	6.088	63	137078	25.871	ug/L	99
38) Bromodichloromethane	6.429	83	180777	25.777	ug/L	99
39) cis-1,3-Dichloropropene	6.950	75	191099	24.114	ug/L	98
40) 4-Methyl-2-pentanone	7.159	43	159176	55.294	ug/L	99
42) Toluene	7.310	91	544790	26.422	ug/L	99
44) trans-1,3-Dichloropropene	7.577	75	183199	26.763	ug/L	99
45) 1,1,2-Trichloroethane	7.767	97	114421	26.099	ug/L	99
46) Tetrachloroethene	7.902	164	107201	23.701	ug/L	99
48) 2-Hexanone	8.079	43	135017	59.994	ug/L	98
49) Dibromochloromethane	8.172	129	124395	25.926	ug/L	99
50) 1,2-Dibromoethane	8.278	107	112172	26.666	ug/L	99
51) Chlorobenzene	8.808	112	346536	24.666	ug/L	100
52) Ethylbenzene	8.944	91	561114	25.435	ug/L	98
53) m,p-Xylene	9.069	106	214410	25.866	ug/L	100
54) o-Xylene	9.474	106	197063	25.210	ug/L	98
55) Styrene	9.493	104	375105	27.212	ug/L	99
57) 1,1,2,2-Tetrachloroethane	10.175	83	103795	26.441	ug/L	97
59) Bromoform	9.661	173	80396	25.508	ug/L	99
60) Isopropylbenzene	9.863	105	536536	25.023	ug/L	99
61) 1,2,3-Trichloropropane	10.207	75	106507	26.945	ug/L	97
62) 1,3,5-Trimethylbenzene	10.474	105	371370	23.885	ug/L	100
63) 1,2,4-Trimethylbenzene	10.850	105	421165	25.141	ug/L	99
64) 1,3-Dichlorobenzene	11.114	146	275223	24.442	ug/L	99
65) 1,4-Dichlorobenzene	11.204	146	285743	24.585	ug/L	99
67) 1,2-Dichlorobenzene	11.577	146	258907	24.434	ug/L	99
68) 1,2-Dibromo-3-chloropr...	12.361	75	25426	28.766	ug/L	96
69) 1,3,5-Trichlorobenzene	12.580	180	198248	23.537	ug/L	99
70) 1,2,4-trichlorobenzene	13.194	180	159223	24.008	ug/L	99
71) Naphthalene	13.435	128	306038	28.276	ug/L	99
72) 1,2,3-Trichlorobenzene	13.676	180	159927	26.426	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

