




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062124\
Data File : VV036201.D
Acq On : 21 Jun 2024 12:59
Operator : SY/MD
Sample : P2909-24
Misc : 5.00g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4DJ5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 00:11:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 20 05:02:48 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

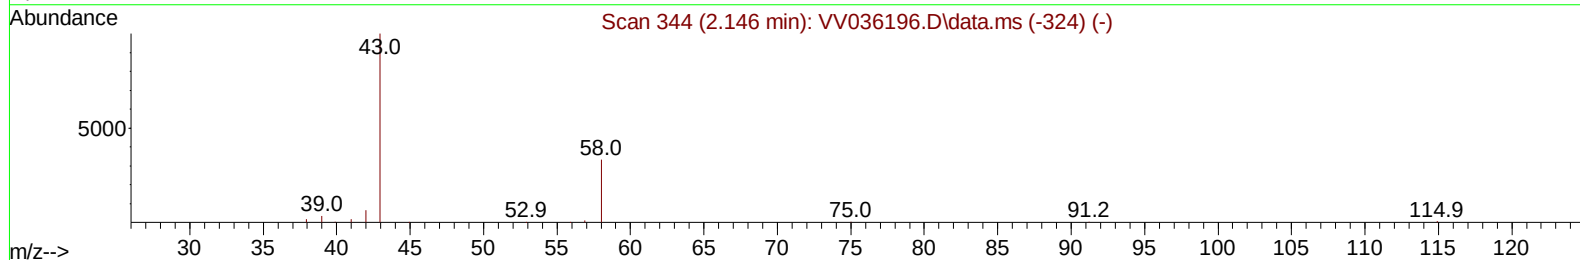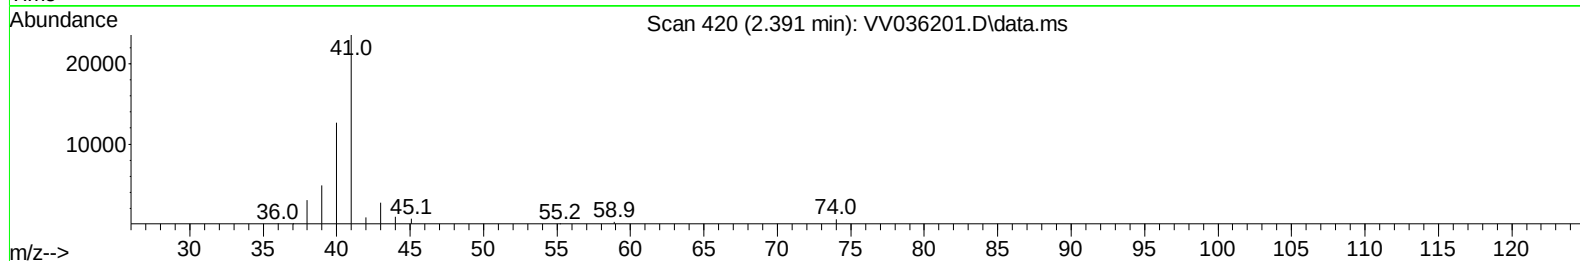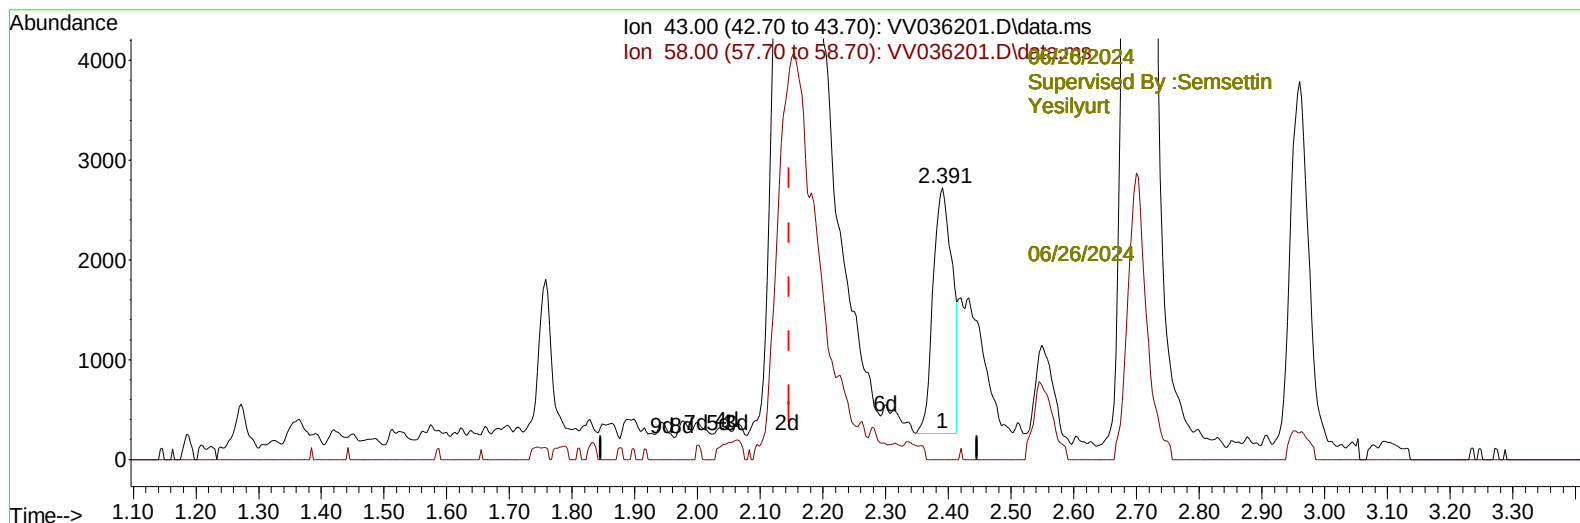

TIC: VV036201.D\data.ms

(13) Acetone (T)

2.391min (+ 0.244) 2.46 ug/L

response 5225

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	12.10	0.71
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062124\
Data File : VV036201.D
Acq On : 21 Jun 2024 12:59
Operator : SY/MD
Sample : P2909-24
Misc : 5.00g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4DJ5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 00:11:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 20 05:02:48 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

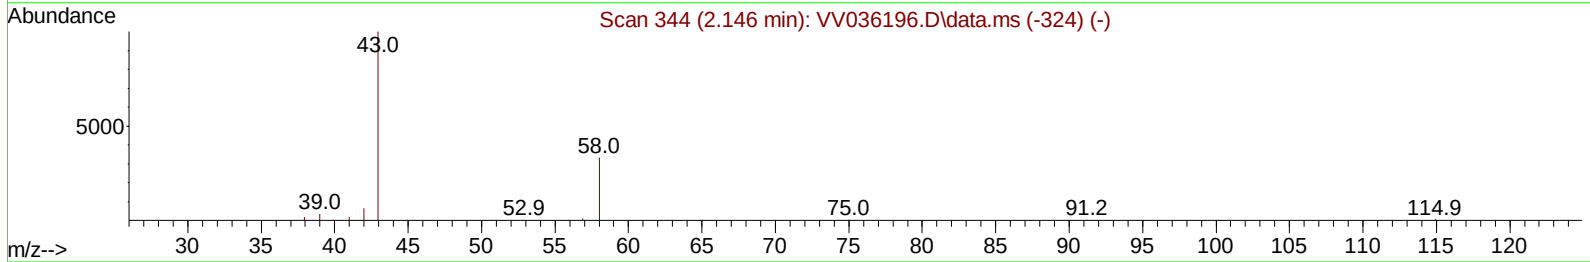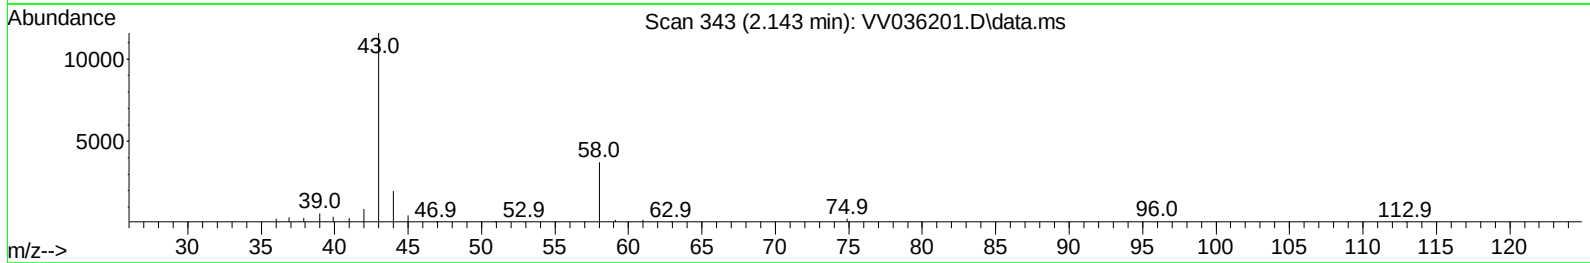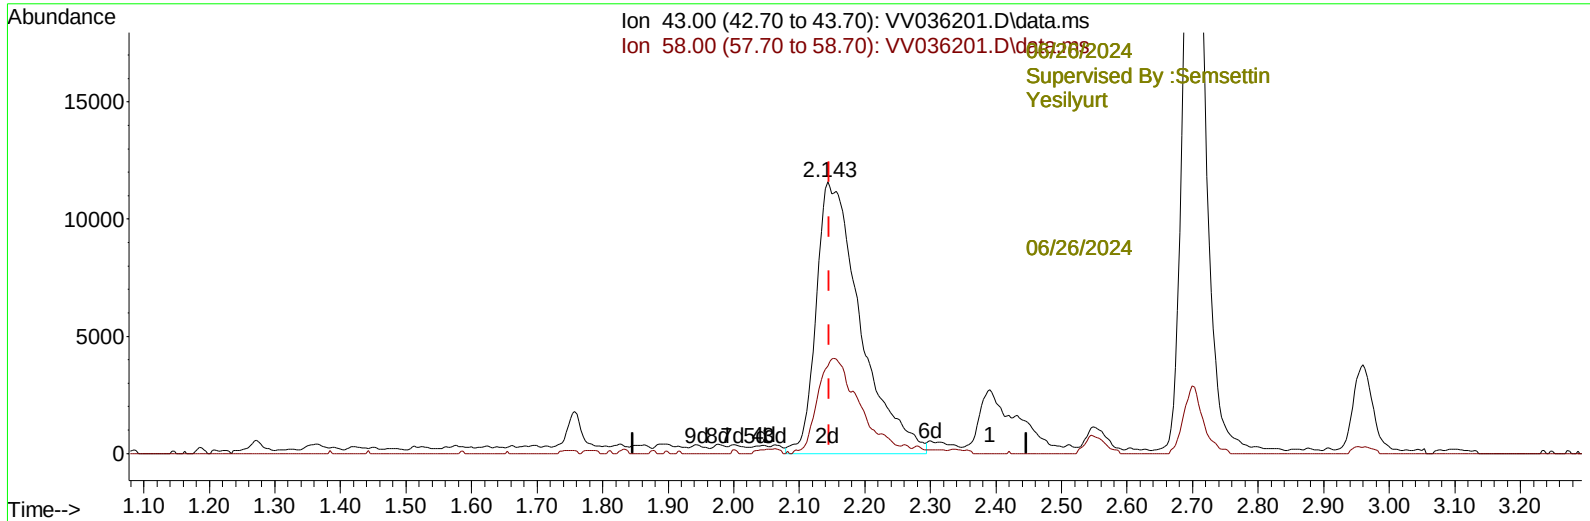

TIC: VV036201.D\data.ms

(13) Acetone (T)

2.143min (-0.003) 25.56 ug/L m

response 54205

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	12.10	0.07
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062124\
Data File : VV036201.D
Acq On : 21 Jun 2024 12:59
Operator : SY/MD
Sample : P2909-24
Misc : 5.00g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4DJ5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 00:11:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 20 05:02:48 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

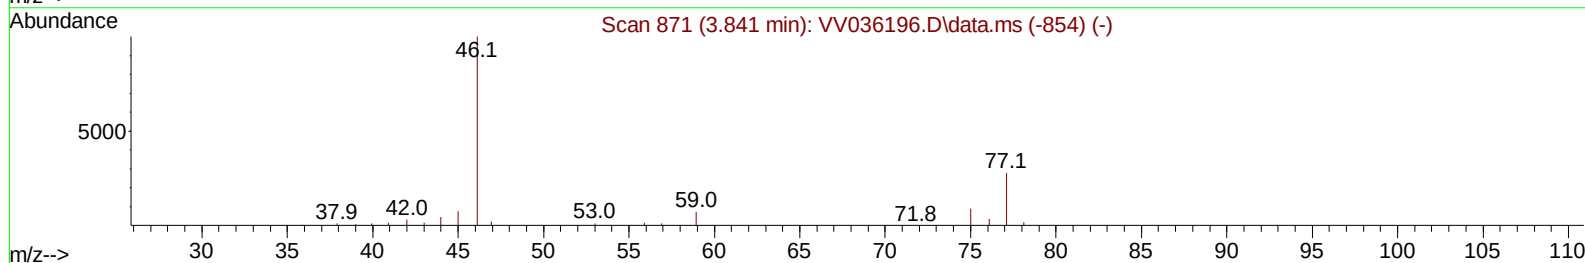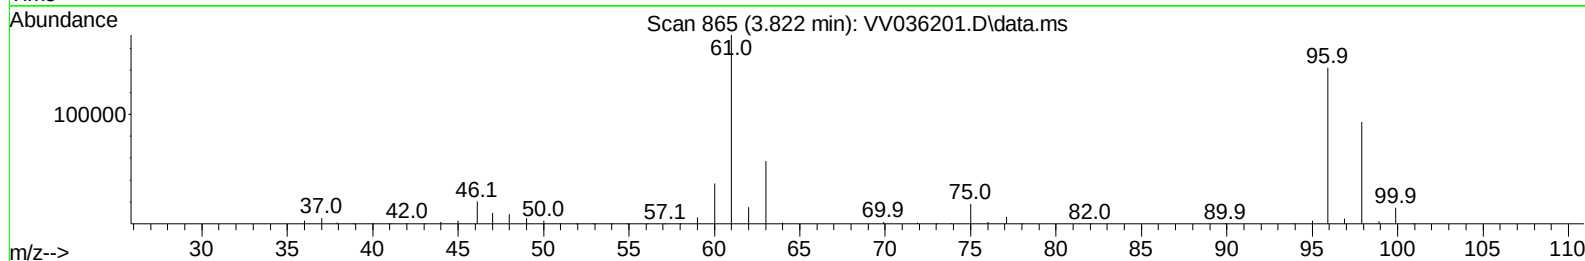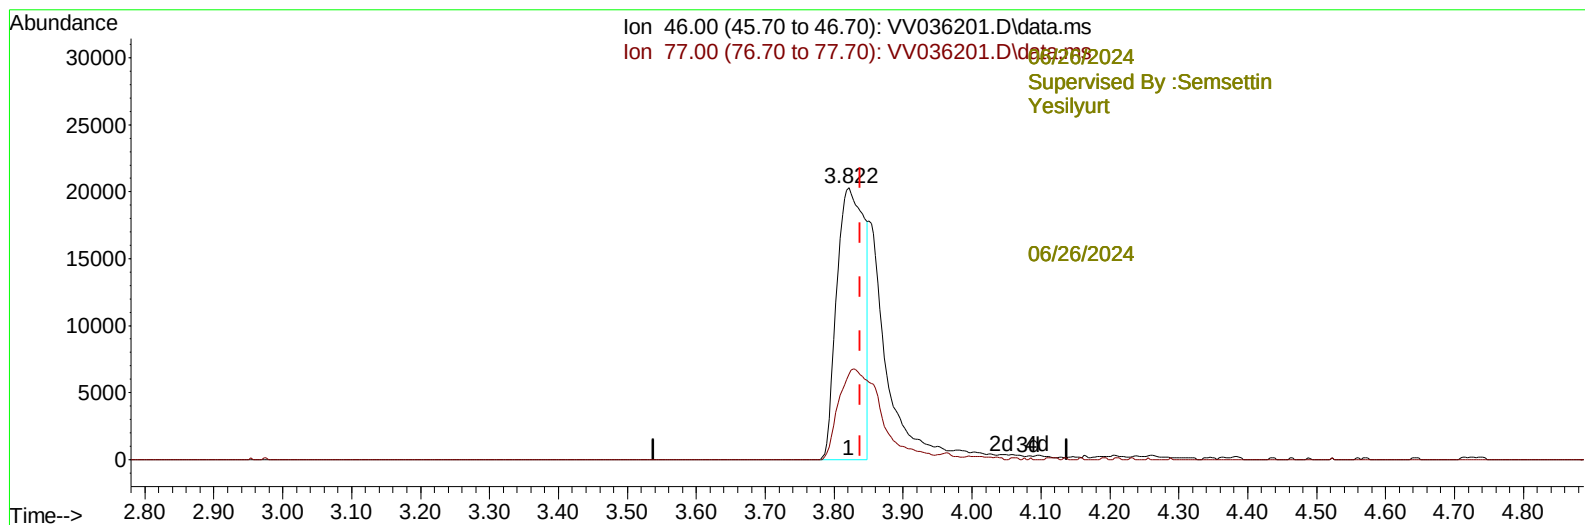

TIC: VV036201.D\data.ms

(21) 2-Butanone-d5 (S)

3.822min (-0.016) 41.09 ug/L

response 55940

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.90	51.42#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062124\
Data File : VV036201.D
Acq On : 21 Jun 2024 12:59
Operator : SY/MD
Sample : P2909-24
Misc : 5.00g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4DJ5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 00:11:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 20 05:02:48 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

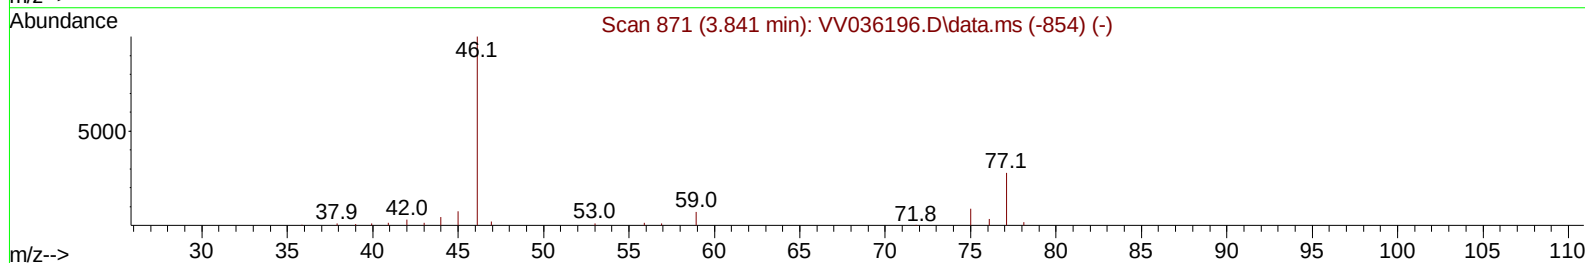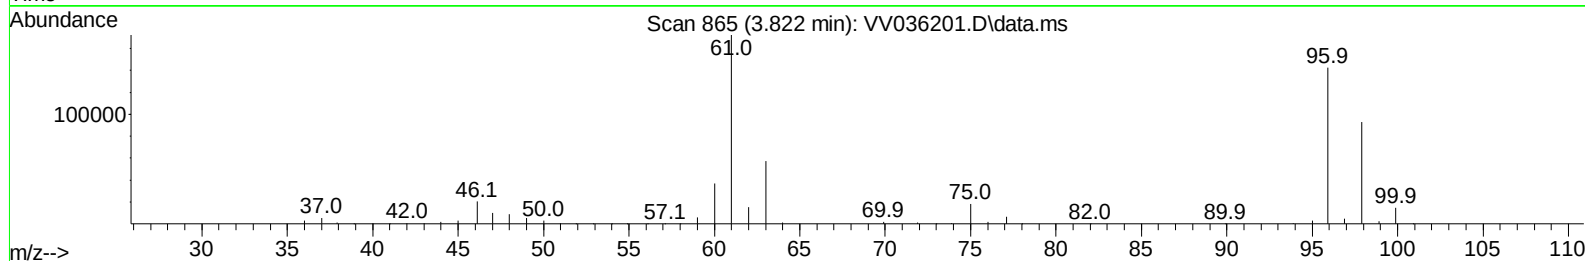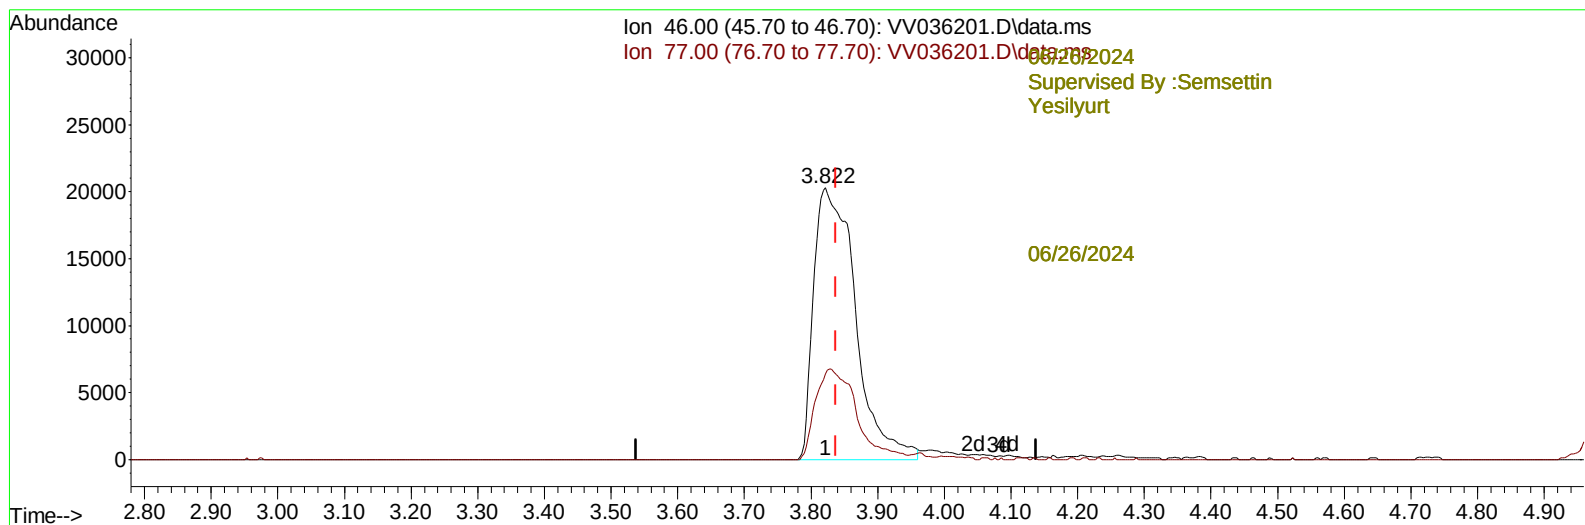

TIC: VV036201.D\data.ms

(21) 2-Butanone-d5 (S)

3.822min (-0.016) 64.72 ug/L m

response 88112

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.90	32.65#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062124\
 Data File : VV036201.D
 Acq On : 21 Jun 2024 12:59
 Operator : SY/MD
 Sample : P2909-24
 Misc : 5.00g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4DJ5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 00:11:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 20 05:02:48 2024
 Response via : Initial Calibration

Reviewed By :Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
-----06/26/2024							Supervised By :Semsettin Yesilyurt
Internal Standards							
1) 1,4-Difluorobenzene	5.529	114	322763	25.000	ug/L	0.00	
28) Chlorobenzene-d5	8.783	117	325727	25.000	ug/L	0.00	
58) 1,4-Dichlorobenzene-d4	11.181	152	181396	25.000	ug/L	0.00	
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.272	65	112870	19.021	ug/L	0.00	06/26/2024
Spiked Amount 25.000	Range 30	- 150	Recovery	=	76.080%		
7) Chloroethane-d5	1.526	69	99551	21.040	ug/L	0.00	
Spiked Amount 25.000	Range 30	- 150	Recovery	=	84.160%		
11) 1,1-Dichloroethene-d2	2.047	65	56779	21.494	ug/L	0.00	
Spiked Amount 25.000	Range 45	- 110	Recovery	=	85.960%		
21) 2-Butanone-d5	3.822	46	88112m	64.718	ug/L	-0.02	
Spiked Amount 50.000	Range 20	- 135	Recovery	=	129.440%		
24) Chloroform-d	4.243	84	265722	25.895	ug/L	0.00	
Spiked Amount 25.000	Range 40	- 150	Recovery	=	103.600%		
26) 1,2-Dichloroethane-d4	4.937	65	134147	24.934	ug/L	0.00	
Spiked Amount 25.000	Range 70	- 130	Recovery	=	99.720%		
32) Benzene-d6	4.953	84	452692	23.381	ug/L	0.00	
Spiked Amount 25.000	Range 20	- 135	Recovery	=	93.520%		
36) 1,2-Dichloropropane-d6	5.985	67	150249	24.642	ug/L	0.00	
Spiked Amount 25.000	Range 70	- 120	Recovery	=	98.560%		
41) Toluene-d8	7.239	98	424963	24.875	ug/L	0.00	
Spiked Amount 25.000	Range 30	- 130	Recovery	=	99.520%		
43) trans-1,3-Dichloroprop...	7.551	79	67063	26.825	ug/L	0.00	
Spiked Amount 25.000	Range 30	- 135	Recovery	=	107.280%		
47) 2-Hexanone-d5	8.030	63	60730	73.514	ug/L	0.00	
Spiked Amount 50.000	Range 20	- 135	Recovery	=	147.020%#		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	130835	28.715	ug/L	0.00	
Spiked Amount 25.000	Range 45	- 120	Recovery	=	114.880%		
66) 1,2-Dichlorobenzene-d4	11.558	152	159850	24.030	ug/L	0.00	
Spiked Amount 25.000	Range 75	- 120	Recovery	=	96.120%		
Target Compounds							Qvalue
12) 1,1-Dichloroethene	2.060	96	339955	65.774	ug/L #	78	
13) Acetone	2.143	43	54205m	25.559	ug/L		
16) Methylene chloride	2.439	84	323104	44.240	ug/L	98	
17) trans-1,2-Dichloroethene	2.683	96	265080	48.281	ug/L	95	
18) Methyl tert-butyl Ether	2.703	73	386782	31.380	ug/L	99	
19) 1,1-Dichloroethane	3.101	63	472000	45.143	ug/L	99	
20) cis-1,2-Dichloroethene	3.805	96	575180	104.258	ug/L	98	
22) 2-Butanone	3.889	43	467447	259.761	ug/L #	70	
25) Chloroform	4.269	83	832950	77.444	ug/L	99	
27) 1,2-Dichloroethane	5.037	62	204936	30.520	ug/L	99	
30) 1,1,1-Trichloroethane	4.506	97	3553	0.399	ug/L #	81	
31) Carbon tetrachloride	4.725	117	370291	47.400	ug/L	99	
33) Benzene	5.002	78	928189	43.570	ug/L	100	
34) Trichloroethene	5.828	95	273522	41.892	ug/L	100	
37) 1,2-Dichloropropane	6.092	63	87931	15.719	ug/L	99	
38) Bromodichloromethane	6.426	83	642946	86.838	ug/L	100	
39) cis-1,3-Dichloropropene	6.947	75	819238	97.918	ug/L	100	
40) 4-Methyl-2-pentanone	7.156	43	413275	135.983	ug/L	95	

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062124\
 Data File : VV036201.D
 Acq On : 21 Jun 2024 12:59
 Operator : SY/MD
 Sample : P2909-24
 Misc : 5.00g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4DJ5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 00:11:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 20 05:02:48 2024
 Response via : Initial Calibration

Reviewed By :Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
42) Toluene	7.310	91	860102	39.511	ug/L	99	06/26/2024
44) trans-1,3-Dichloropropene	7.577	75	413818	57.262	ug/L	99	Supervised By :Semsettin
45) 1,1,2-Trichloroethane	7.767	97	144624	31.247	ug/L	99	Yesilyurt
46) Tetrachloroethene	7.902	164	271455	56.846	ug/L	98	
48) 2-Hexanone	8.075	43	350243	147.411	ug/L	94	
49) Dibromochloromethane	8.172	129	517667	102.193	ug/L	99	
50) 1,2-Dibromoethane	8.278	107	386627	87.056	ug/L	100	06/26/2024
51) Chlorobenzene	8.812	112	277508	18.710	ug/L	99	
52) Ethylbenzene	8.944	91	1187377	50.982	ug/L	99	
53) m,p-Xylene	9.069	106	912593	104.282	ug/L	99	
54) o-Xylene	9.474	106	383168	46.430	ug/L	98	
55) Styrene	9.493	104	1086666	74.669	ug/L	98	
57) 1,1,2,2-Tetrachloroethane	10.175	83	161180	38.891	ug/L	98	
59) Bromoform	9.664	173	98685	28.848	ug/L	99	
61) 1,2,3-Trichloropropane	10.207	75	283070	65.981	ug/L	98	
64) 1,3-Dichlorobenzene	11.114	146	1179682	96.525	ug/L	100	
65) 1,4-Dichlorobenzene	11.204	146	761463	60.363	ug/L	99	
67) 1,2-Dichlorobenzene	11.577	146	356681	31.014	ug/L	99	
68) 1,2-Dibromo-3-chloropr...	12.361	75	47268	49.271	ug/L	98	
70) 1,2,4-trichlorobenzene	13.194	180	201419	27.982	ug/L	100	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062124\
Data File : VV036201.D
Acq On : 21 Jun 2024 12:59
Operator : SY/MD
Sample : P2909-24
Misc : 5.00g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4DJ5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 00:11:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 20 05:02:48 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

