

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062124\
 Data File : VW036199.D
 Acq On : 21 Jun 2024 12:13
 Operator : SY/MD
 Sample : P2960-13
 Misc : 5.57g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB50

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
 Supervised By :Semsettin Yesilyurt 06/26/2024

Quant Time: Jun 21 12:37:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 20 05:02:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	391485	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	402459	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	197080	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	170792	23.730	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.920%
7) Chloroethane-d5	1.526	69	144996	25.265	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.080%
11) 1,1-Dichloroethene-d2	2.050	65	78234	24.417	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	97.680%
21) 2-Butanone-d5	3.822	46	84277m	51.035	ug/L	-0.02
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.060%
24) Chloroform-d	4.240	84	315547	25.353	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.400%
26) 1,2-Dichloroethane-d4	4.937	65	173885	26.647	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.600%
32) Benzene-d6	4.953	84	639188	26.718	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	106.880%
36) 1,2-Dichloropropane-d6	5.982	67	201442	26.739	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.960%
41) Toluene-d8	7.239	98	556758	26.376	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	105.520%
43) trans-1,3-Dichloroprop...	7.551	79	81613	26.421	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	105.680%
47) 2-Hexanone-d5	8.030	63	66181	64.839	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	129.680%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	155255	27.578	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	110.320%
66) 1,2-Dichlorobenzene-d4	11.558	152	208674	28.874	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	115.480%
Target Compounds						
5) Vinyl chloride	1.275	62	11819	1.386	ug/L #	78
16) Methylene chloride	2.439	84	65155	7.355	ug/L	97
20) cis-1,2-Dichloroethene	3.805	96	1129199	168.750	ug/L	99
25) Chloroform	4.269	83	8437	0.647	ug/L	87
34) Trichloroethene	5.831	95	73091	9.060	ug/L	98
46) Tetrachloroethene	7.902	164	1087466	184.311	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062124\
Data File : VV036199.D
Acq On : 21 Jun 2024 12:13
Operator : SY/MD
Sample : P2960-13
Misc : 5.57g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BHB50

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

Quant Time: Jun 21 12:37:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 20 05:02:48 2024
Response via : Initial Calibration

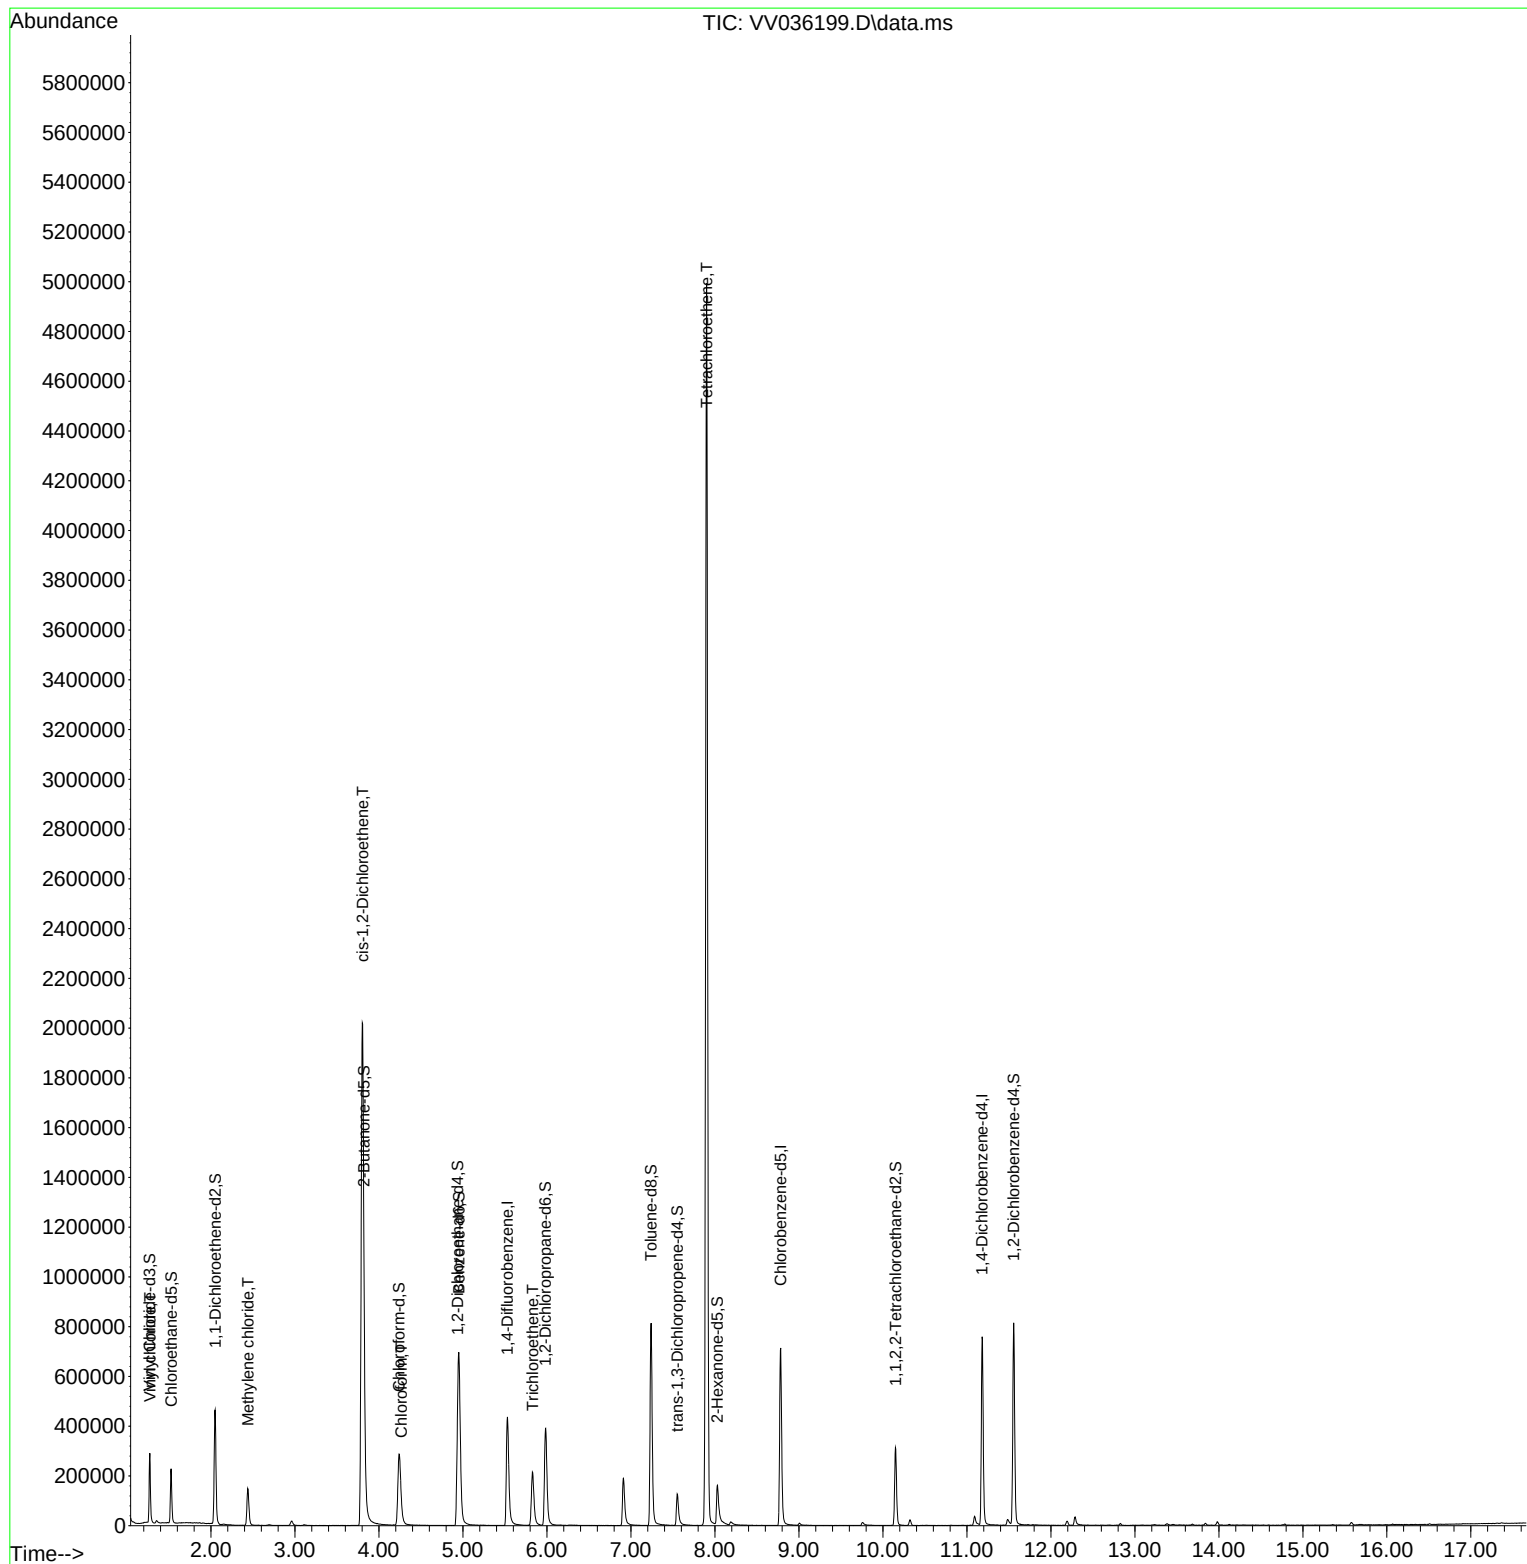

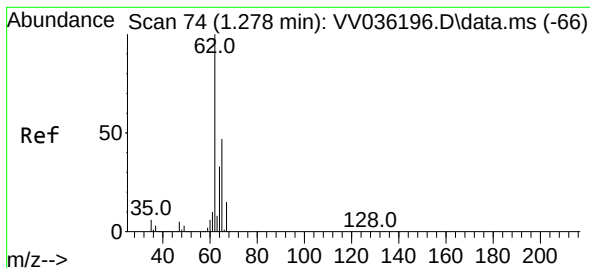





#5
 Vinyl chloride
 Concen: 1.386 ug/L
 RT: 1.275 min Scan# 74
 Delta R.T. -0.003 min
 Lab File: VV036199.D
 Acq: 21 Jun 2024 12:13

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB50

Tgt Ion: 62 Resp: 11819
 Ion Ratio Lower Upper
 62 100
 64 45.0 22.9 42.5




Manual Integrations
 APPROVED


Reviewed By :Mahesh Dadoda 06/26/2024
 Supervised By :Semsettin Yesilyurt 06/26/2024

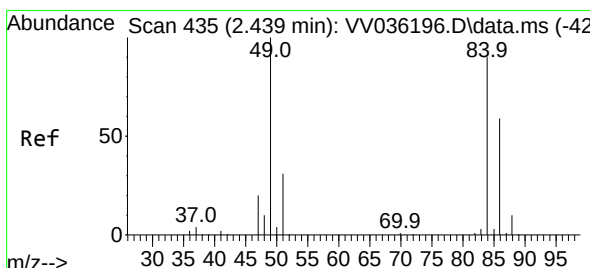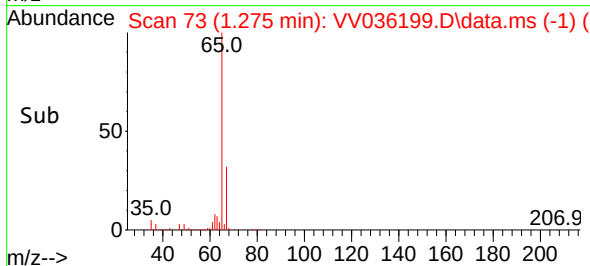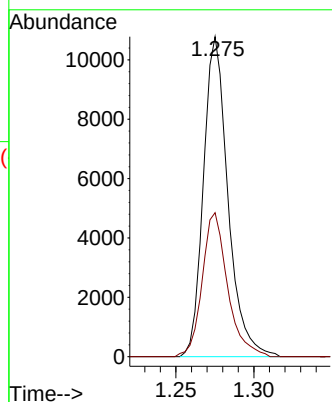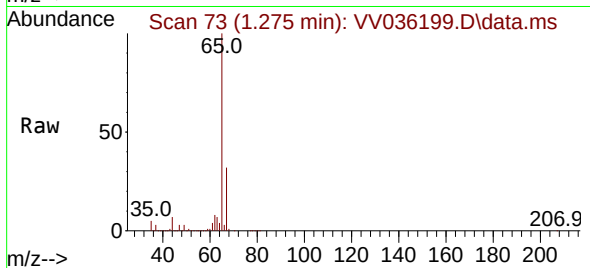

#16
 Methylene chloride
 Concen: 7.355 ug/L
 RT: 2.439 min Scan# 435
 Delta R.T. 0.000 min
 Lab File: VV036199.D
 Acq: 21 Jun 2024 12:13


Tgt Ion: 84 Resp: 65155
 Ion Ratio Lower Upper
 84 100
 86 63.2 44.6 82.8
 49 111.9 81.1 150.5

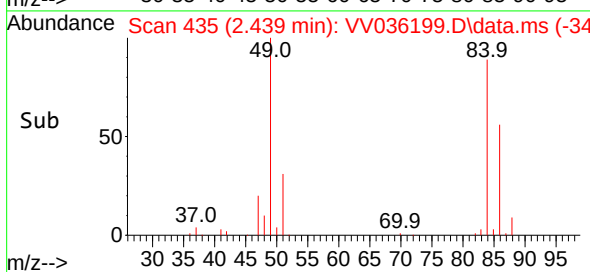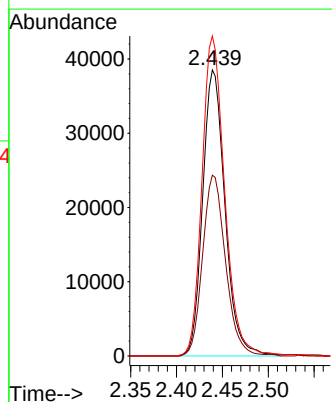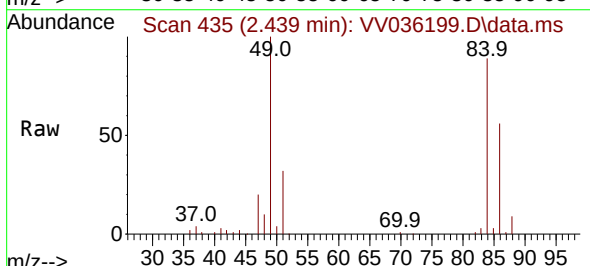

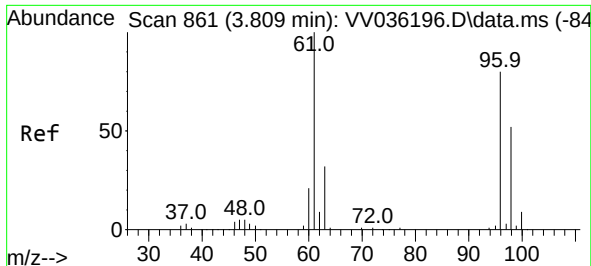

#20
cis-1,2-Dichloroethene
Concen: 168.750 ug/L
RT: 3.805 min Scan# 861
Delta R.T. -0.003 min
Lab File: VV036199.D
Acq: 21 Jun 2024 12:13




Instrument :
MSVOA_V
ClientSampleId :
BHB50

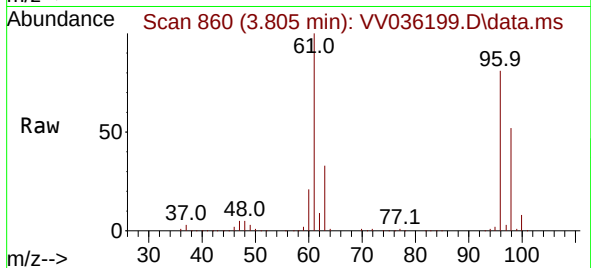

Tgt Ion: 96 Resp: 112919
Ion Ratio Lower Upper
96 100
61 123.9 87.9 163.3
98 64.1 44.4 82.5




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

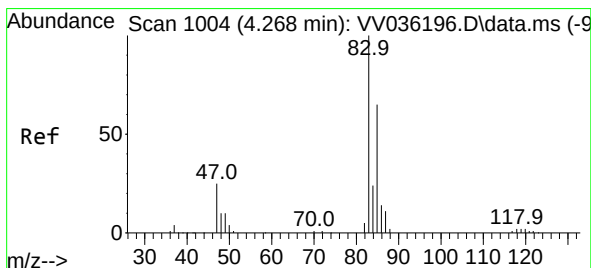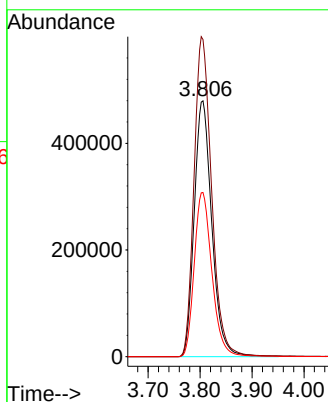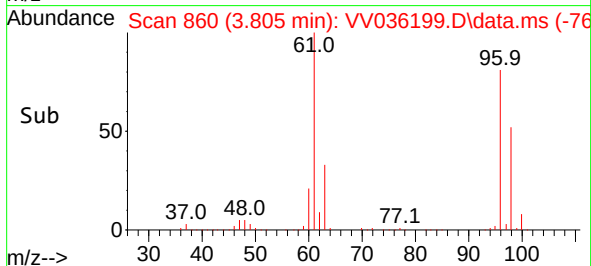

#25
Chloroform
Concen: 0.647 ug/L
RT: 4.269 min Scan# 1004
Delta R.T. 0.000 min
Lab File: VV036199.D
Acq: 21 Jun 2024 12:13

Tgt Ion: 83 Resp: 8437
Ion Ratio Lower Upper
83 100
85 75.1 45.2 84.0

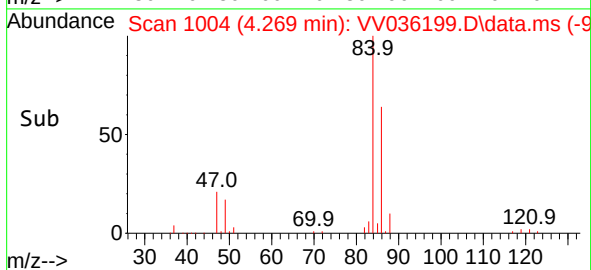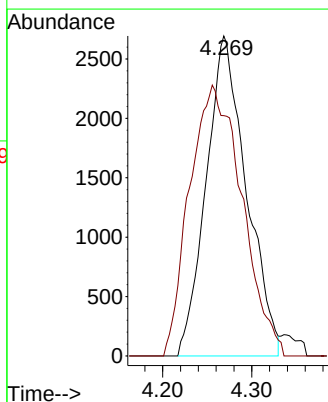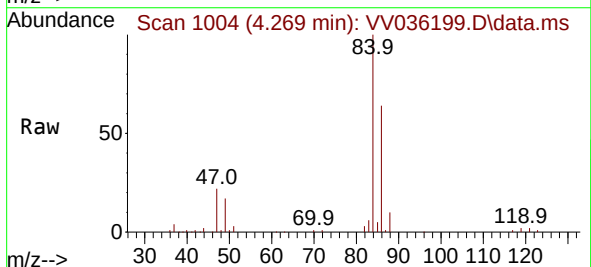

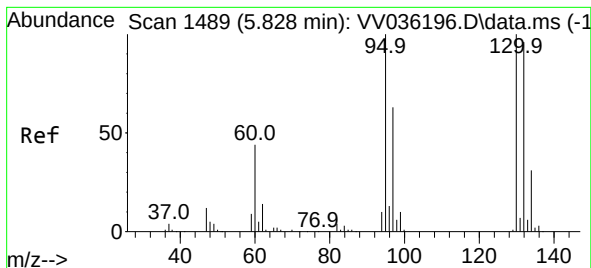

#34

Trichloroethene

Concen: 9.060 ug/L

RT: 5.831 min Scan# 1489

Delta R.T. 0.006 min

Lab File: VV036199.D


Acq: 21 Jun 2024 12:13

Instrument :

MSVOA_V

ClientSampleId :

BHB50

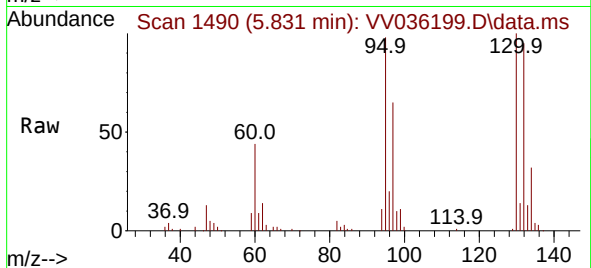

Tgt Ion: 95 Resp: 7309

Ion Ratio Lower Upper

95 100

97 66.5 44.8 83.2

132 96.3 66.8 124.2



130 101.9 70.0 130.0

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 06/26/2024

Supervised By :Semsettin Yesilyurt 06/26/2024

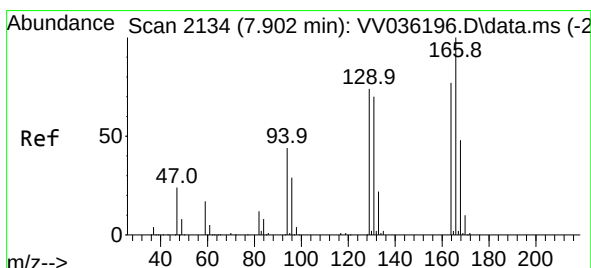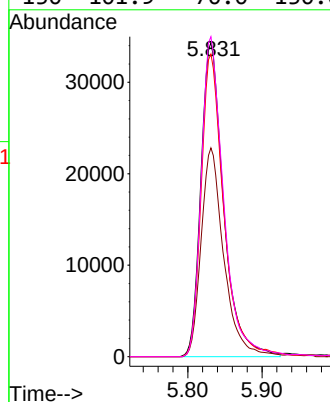

#46

Tetrachloroethene

Concen: 184.311 ug/L

RT: 7.902 min Scan# 2134

Delta R.T. 0.000 min

Lab File: VV036199.D

Acq: 21 Jun 2024 12:13

Tgt Ion:164 Resp: 1087466

Ion Ratio Lower Upper

164 100

129 96.4 64.6 120.0

131 92.9 63.2 117.4

166 127.2 89.5 166.3

