

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062124\
 Data File : VV036218.D
 Acq On : 21 Jun 2024 20:41
 Operator : SY/MD
 Sample : VV0621SBL02
 Misc : 5.00g/10.0mL/MSVOA_V/SOIL
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK330

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
 Supervised By :Semsettin Yesilyurt 06/26/2024

Quant Time: Jun 22 03:00:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 22 02:57:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	255210	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	267791	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	111523	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	93755	19.982	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.920%		
7) Chloroethane-d5	1.526	69	86822m	23.207	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	92.840%		
11) 1,1-Dichloroethene-d2	2.050	65	46208	22.122	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	88.480%		
21) 2-Butanone-d5	3.834	46	50838	47.224	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	94.440%		
24) Chloroform-d	4.243	84	190833	23.520	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	94.080%		
26) 1,2-Dichloroethane-d4	4.941	65	109889	25.832	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	103.320%		
32) Benzene-d6	4.957	84	359729	22.599	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	90.400%		
36) 1,2-Dichloropropane-d6	5.985	67	119194	23.778	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	95.120%		
41) Toluene-d8	7.243	98	288774	20.560	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	82.240%		
43) trans-1,3-Dichloroprop...	7.555	79	43095	20.967	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	83.880%		
47) 2-Hexanone-d5	8.034	63	32529	47.896	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	95.800%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	105490	28.162	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	112.640%		
66) 1,2-Dichlorobenzene-d4	11.558	152	108704	26.580	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	106.320%		
Target Compounds						Qvalue
16) Methylene chloride	2.442	84	37372	6.471	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062124\
Data File : VV036218.D
Acq On : 21 Jun 2024 20:41
Operator : SY/MD
Sample : VV0621SBL02
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 28 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
VBLK330

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024


Quant Time: Jun 22 03:00:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 22 02:57:23 2024
Response via : Initial Calibration

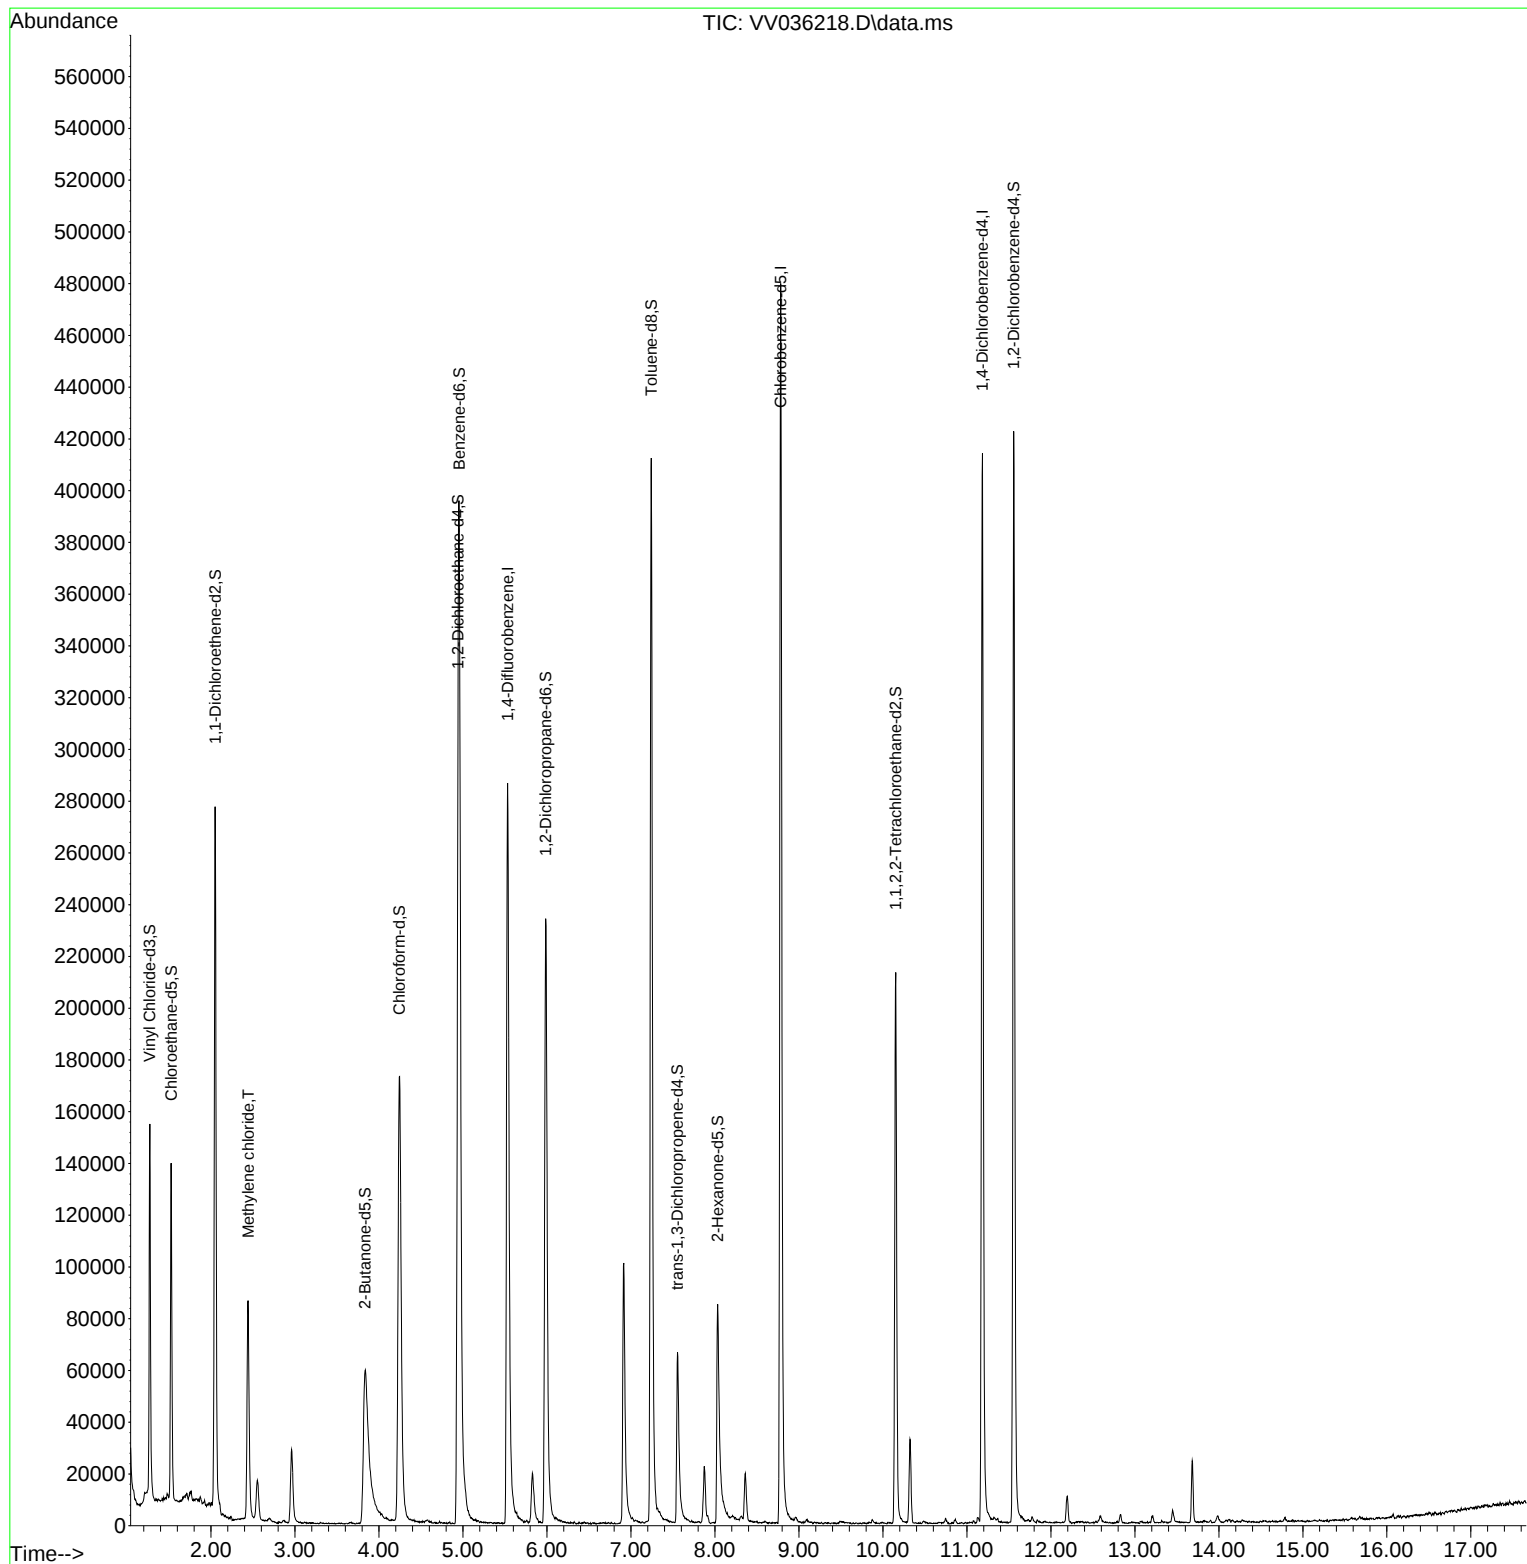

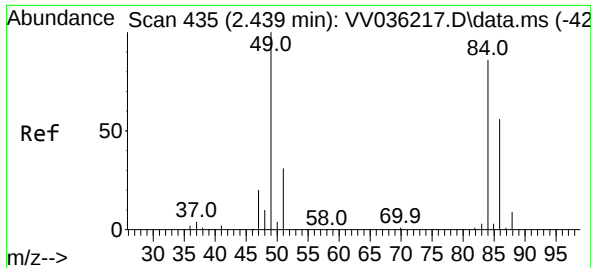

#16
Methylene chloride
Concen: 6.471 ug/L
RT: 2.442 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV036218.D
Acq: 21 Jun 2024 20:41

Instrument :
MSVOA_V
ClientSampleId :
VBLK330

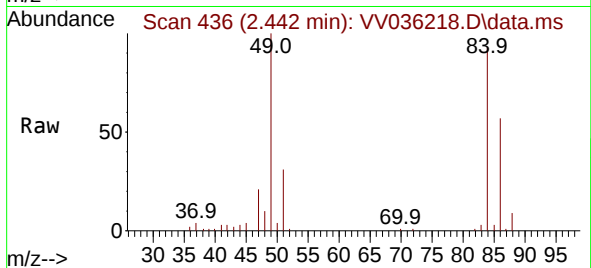

Tgt Ion: 84	Resp: 3737
Ion Ratio	Lower Upper
84 100	
86 61.5	44.6 82.8
49 108.0	81.1 150.5

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

