
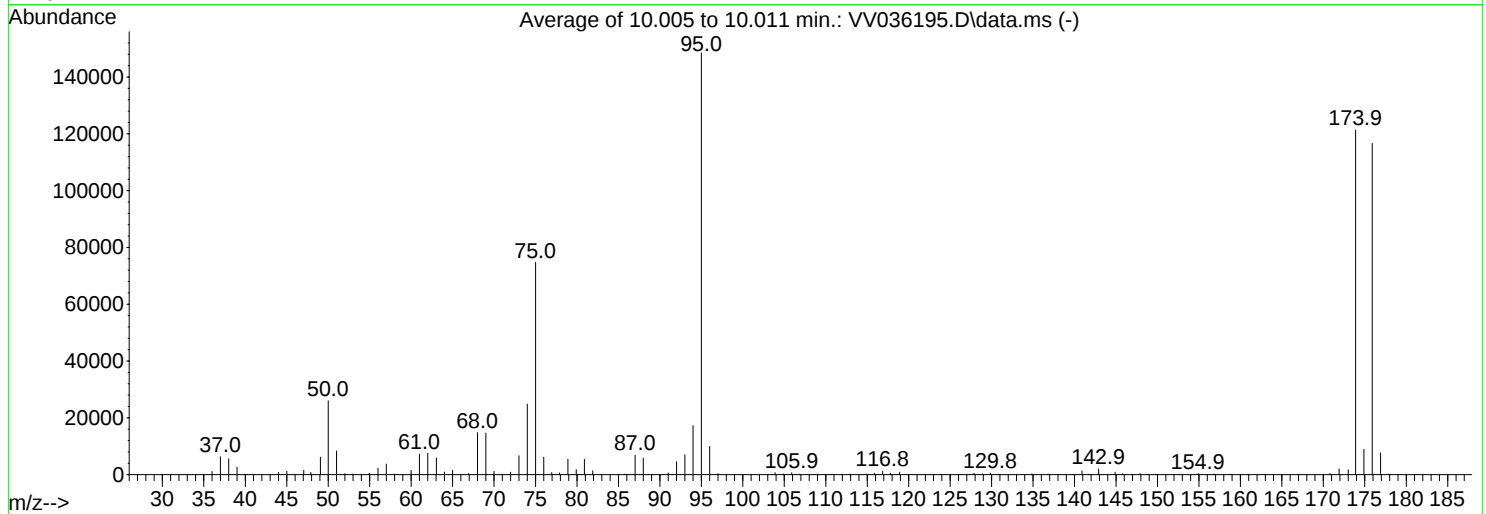


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062124\
Data File : VV036195.D
Acq On : 21 Jun 2024 08:29
Operator : SY/MD
Sample : BFB327
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB327

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Title : VOC Analysis
Last Update : Wed Jun 26 04:03:41 2024

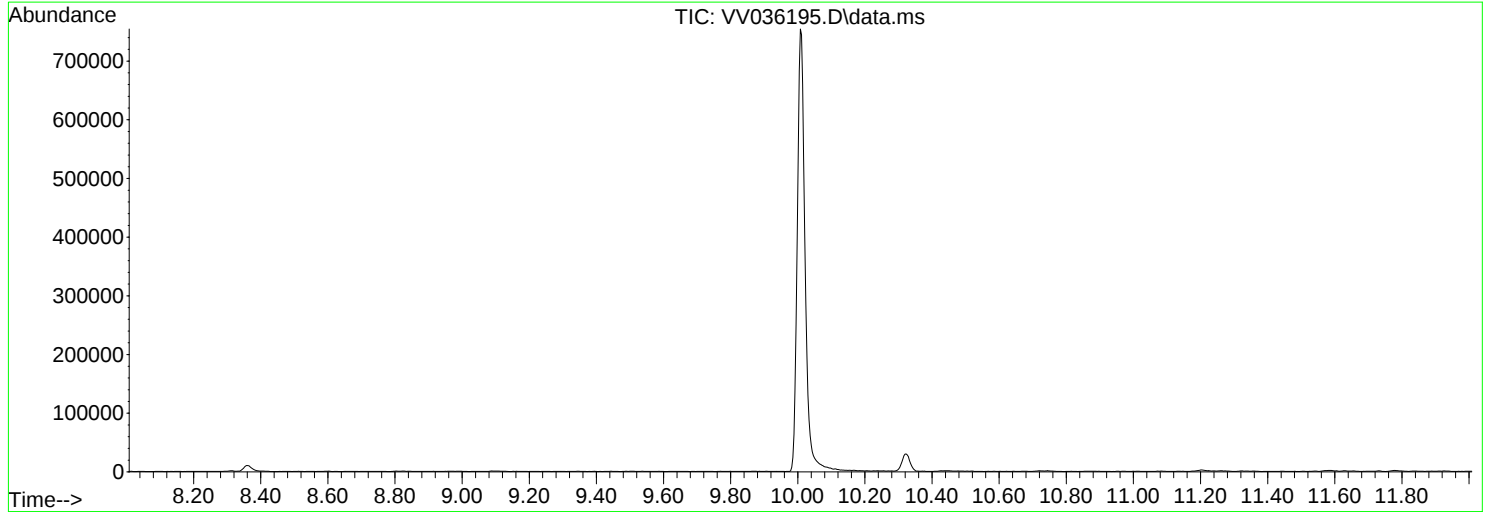

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	26040	PASS
75	95	30	80	50.3	74736	PASS
95	95	100	100	100.0	148501	PASS
96	95	5	9	6.7	9907	PASS
173	174	0.00	2	1.4	1690	PASS
174	95	50	120	81.7	121352	PASS
175	174	5	9	7.3	8901	PASS
176	174	95	101	96.1	116595	PASS
177	176	5	9	6.5	7632	PASS

m/z	Abundance
39.90	185.0
44.00	529.0
77.00	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

m/z	Abundance
36.00	1063.0
37.00	6006.0
38.00	5449.0
39.00	2546.0
39.90	350.0
44.00	1300.0
45.00	1103.0
46.00	140.0
47.00	1479.0
47.90	710.0
49.00	5881.0
50.00	24360.0
51.00	7984.0
52.00	314.0
52.80	213.0
54.90	492.0
56.00	2059.0
57.00	3634.0
58.10	223.0
60.00	1451.0
61.00	6830.0
62.00	7283.0
63.00	5706.0
64.00	981.0
65.00	1473.0
65.90	223.0
66.90	373.0
68.00	14163.0
69.00	14123.0
70.00	1113.0
70.90	127.0
72.00	826.0
73.00	6263.0
74.00	23680.0
75.00	71656.0
76.00	5895.0
77.00	812.0
77.90	556.0
78.90	5284.0
79.90	1707.0
80.90	4959.0
81.90	1269.0
82.90	130.0
85.70	149.0
87.00	6406.0
88.00	5528.0
91.00	622.0
92.00	4145.0
93.00	6778.0
94.00	16576.0
95.00	140160.0
96.00	9358.0
97.00	291.0
103.90	674.0
104.90	250.0
105.90	644.0
106.80	173.0
110.70	132.0
111.90	107.0
112.80	152.0
115.00	201.0
115.80	512.0
116.80	1098.0
117.80	492.0
118.90	802.0
123.90	108.0
127.90	515.0
128.90	248.0
129.80	518.0
130.80	173.0
134.90	258.0
136.80	248.0
140.90	1191.0
141.70	195.0
142.90	1883.0
144.90	823.0
145.80	415.0
146.90	128.0
147.90	347.0
149.70	152.0
152.70	101.0
154.90	361.0
156.90	199.0
158.80	143.0
161.00	145.0
170.80	388.0
171.90	1962.0
173.00	1567.0
173.90	111432.0
174.90	8306.0
175.90	106744.0
176.90	7149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

177.90

188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

m/z	Abundance
36.00	1150.0
37.00	6536.0
38.00	5713.0
39.00	2681.0
40.00	335.0
42.80	115.0
44.00	1334.0
45.00	1315.0
45.90	160.0
47.00	1598.0
47.90	829.0
49.00	6357.0
50.00	26888.0
51.00	8680.0
52.00	344.0
52.90	222.0
55.00	502.0
56.00	2378.0
57.00	3812.0
57.90	218.0
60.00	1596.0
61.00	7418.0
62.00	7887.0
63.00	6029.0
64.00	945.0
65.00	1584.0
66.00	189.0
66.90	385.0
68.00	15448.0
69.00	15251.0
70.00	1239.0
71.00	129.0
72.00	898.0
73.00	6857.0
74.00	25664.0
75.00	77792.0
76.00	6406.0
76.90	857.0
77.90	629.0
78.90	5590.0
79.90	1907.0
80.90	5619.0
81.90	1428.0
82.90	158.0
85.70	160.0
86.10	156.0
87.00	7145.0
88.00	6000.0
91.00	671.0
92.00	4628.0
93.00	7297.0
94.00	17880.0
95.00	154240.0
96.00	10271.0
97.00	371.0
103.90	694.0
104.90	264.0
105.90	727.0
106.90	193.0
110.80	156.0
111.90	125.0
112.90	159.0
114.90	225.0
115.90	568.0
116.90	1175.0
117.80	544.0
118.90	850.0
123.80	100.0
127.90	497.0
128.90	275.0
129.90	611.0
130.80	205.0
134.90	293.0
136.80	242.0
140.90	1390.0
141.70	191.0
142.90	2029.0
144.90	881.0
145.80	392.0
146.90	123.0
147.90	384.0
149.80	144.0
152.70	103.0
154.90	422.0
156.80	218.0
158.80	153.0
160.90	145.0
170.80	385.0
171.90	2076.0
173.00	1755.0
173.90	125944.0
174.90	9209.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

175.90	120848.0
176.90	7872.0
177.90	232.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

m/z	Abundance
36.00	1100.0
37.00	6339.0
38.00	5618.0
39.00	2607.0
40.00	306.0
42.90	134.0
44.00	1264.0
45.00	1388.0
45.90	192.0
47.10	1485.0
47.90	843.0
49.10	6208.0
50.00	26872.0
51.00	8429.0
52.00	356.0
53.00	225.0
55.00	519.0
56.00	2279.0
57.00	3658.0
57.90	205.0
60.00	1508.0
61.00	7404.0
62.00	7567.0
63.10	5870.0
64.00	842.0
65.00	1568.0
66.00	167.0
67.00	398.0
68.00	14836.0
69.00	14648.0
70.00	1141.0
71.00	104.0
72.00	889.0
73.00	6779.0
74.00	25208.0
75.00	74760.0
76.00	6118.0
76.90	910.0
77.90	639.0
78.90	5382.0
79.90	1834.0
80.90	5523.0
81.90	1416.0
82.90	148.0
85.80	171.0
87.00	7095.0
88.00	5899.0
91.00	617.0
92.00	4680.0
93.00	6971.0
94.00	17472.0
95.00	151104.0
96.00	10093.0
97.00	407.0
103.90	646.0
104.90	237.0
105.90	709.0
106.90	182.0
109.80	103.0
110.80	146.0
112.00	104.0
112.90	147.0
114.90	253.0
115.90	516.0
116.90	1132.0
117.80	527.0
118.90	854.0
123.70	104.0
127.90	451.0
128.90	256.0
129.90	611.0
130.80	200.0
134.80	287.0
136.80	206.0
139.80	102.0
140.90	1376.0
141.70	164.0
142.90	1997.0
144.90	783.0
145.80	282.0
146.80	120.0
147.90	382.0
148.80	117.0
149.90	172.0
152.70	113.0
154.90	447.0
156.70	231.0
158.80	161.0
160.80	126.0
170.80	334.0
171.90	2018.0
173.00	1749.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

173.90	126680.0
174.90	9188.0
175.90	122192.0
176.90	7875.0
177.90	253.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327