

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062218\
 Data File : VV006417.D
 Acq On : 22 Jun 2018 17:07
 Operator : SY/MD
 Sample : J3615-03 100X
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEXT9

Quant Time: Jun 23 00:19:16 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 22 23:56:13 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	291433	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	261425	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	114120	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	71118	4.47	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.40%
7) Chloroethane-d5	1.59	69	68444	5.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.40%
11) 1,1-Dichloroethene-d2	2.13	63	99747	3.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.40%
20) 2-Butanone-d5	3.97	46	224642	66.47	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	132.94%#
24) Chloroform-d	4.41	84	153789	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.80%
26) 1,2-Dichloroethane-d4	5.09	65	80408	5.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.00%
32) Benzene-d6	5.11	84	323987	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.20%
36) 1,2-Dichloropropane-d6	6.12	67	101871	5.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.80%
41) Toluene-d8	7.37	98	276463	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.20%
43) trans-1,3-Dichloropropene-	7.67	79	28683	3.39	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	67.80%
46) 2-Hexanone-d5	8.14	63	164205	45.00	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.00%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	63392	4.63	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	106720	5.39	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.80%


Target Compounds					Ovalue
33) Benzene	5.15	78	822603	11.41 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062218\
Data File : VV006417.D
Acq On : 22 Jun 2018 17:07
Operator : SY/MD
Sample : J3615-03 100X
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEXT9

Quant Time: Jun 23 00:19:16 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 22 23:56:13 2018
Response via : Initial Calibration

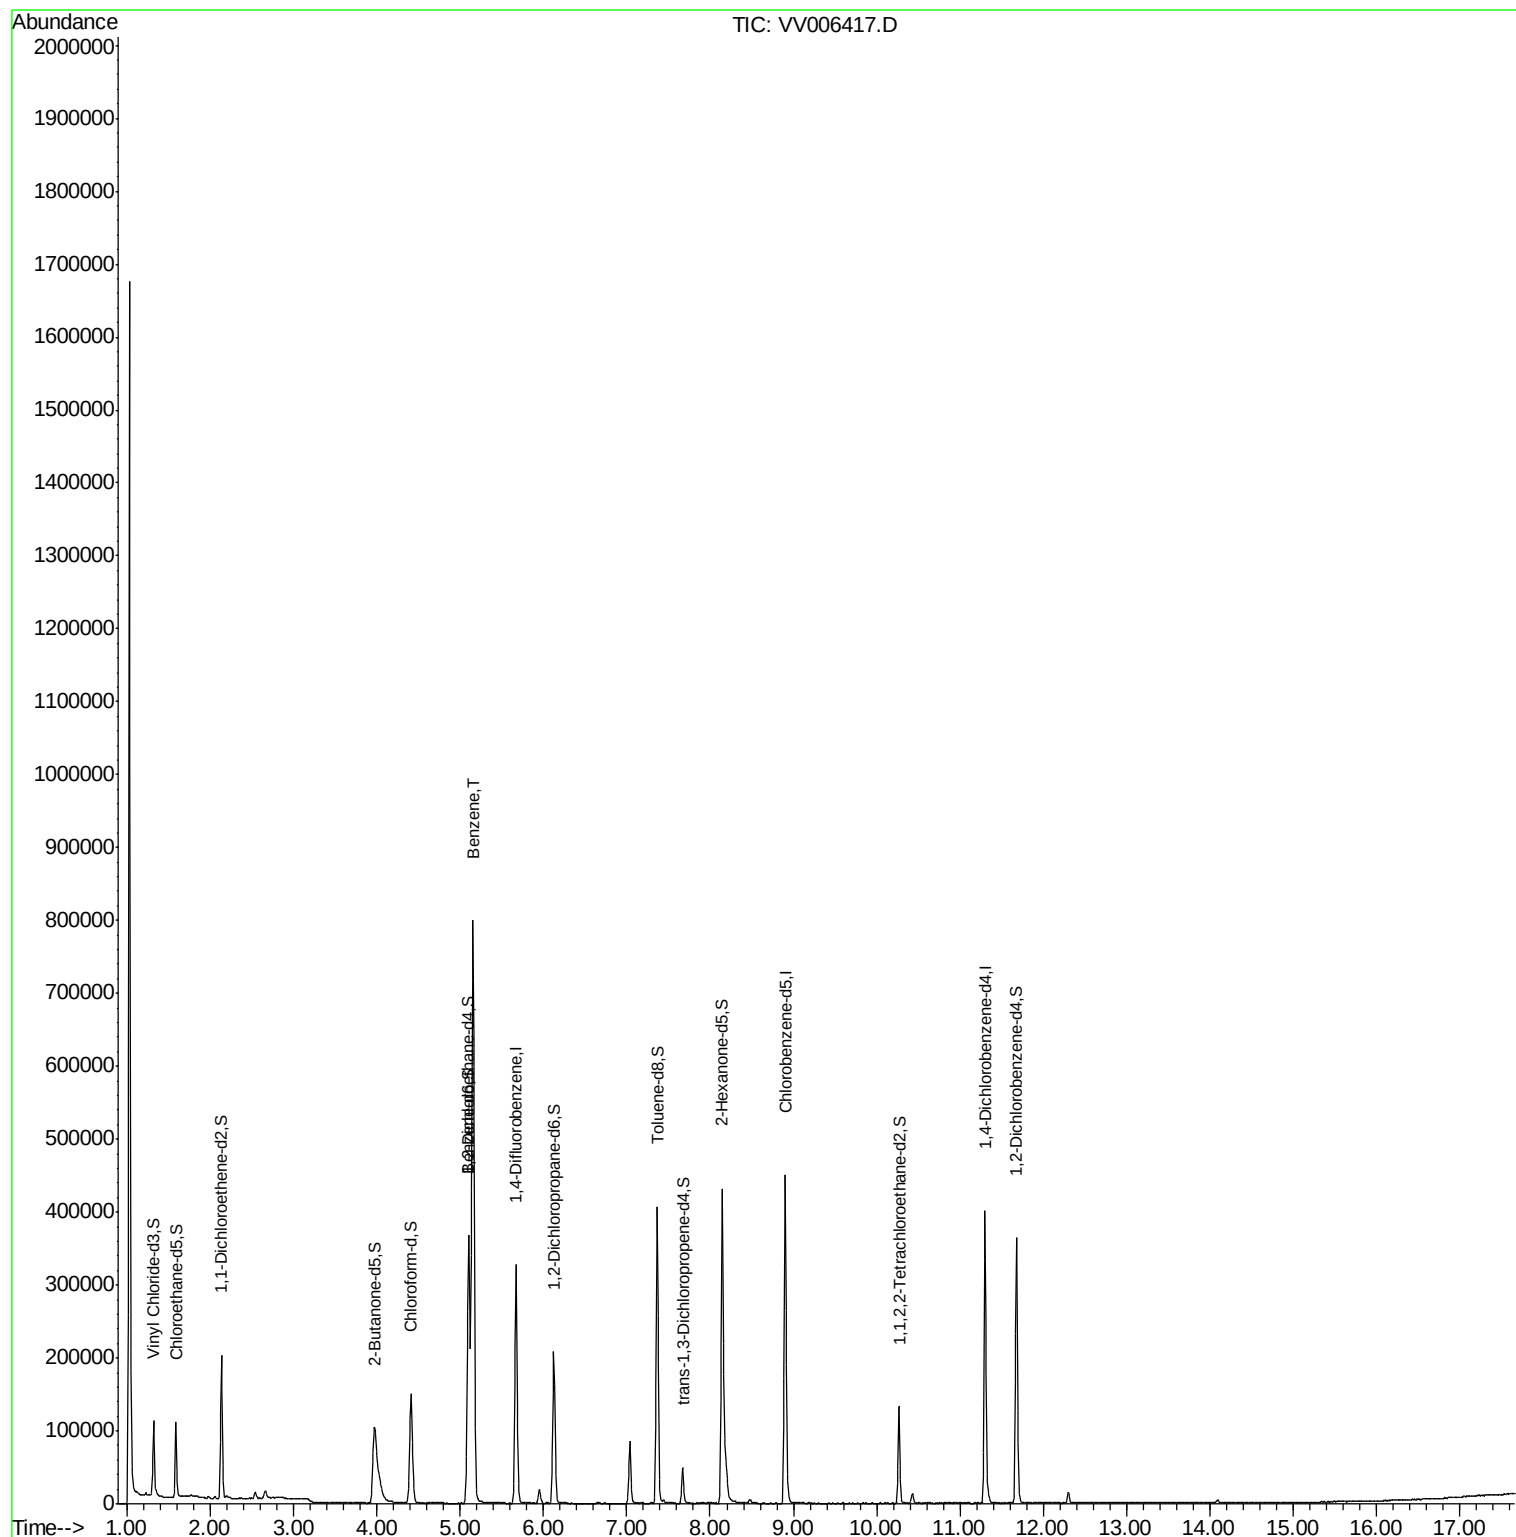

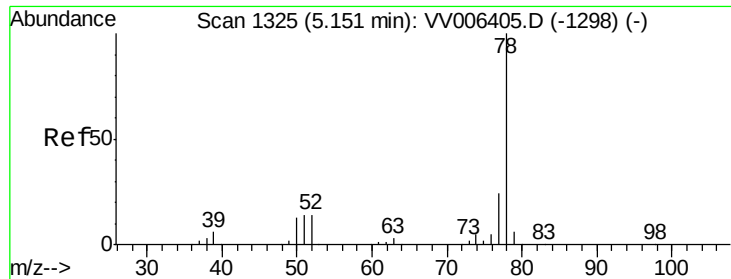

#33

Benzene

Concen: 11.41 ug/L

RT: 5.15 min Scan# 1326

Delta R.T. 0.00 min

Lab File: VV006417.D

Acq: 22 Jun 2018 17:07

Instrument :
MSVOA_V
ClientSampleId :
BEXT9

Tgt Ion: 78 Resp: 822603

