


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062524\
Data File : VV036268.D
Acq On : 25 Jun 2024 09:13
Operator : SY/MD
Sample : BFB329
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB329

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Title : VOC Analysis
Last Update : Wed Jun 26 04:03:41 2024

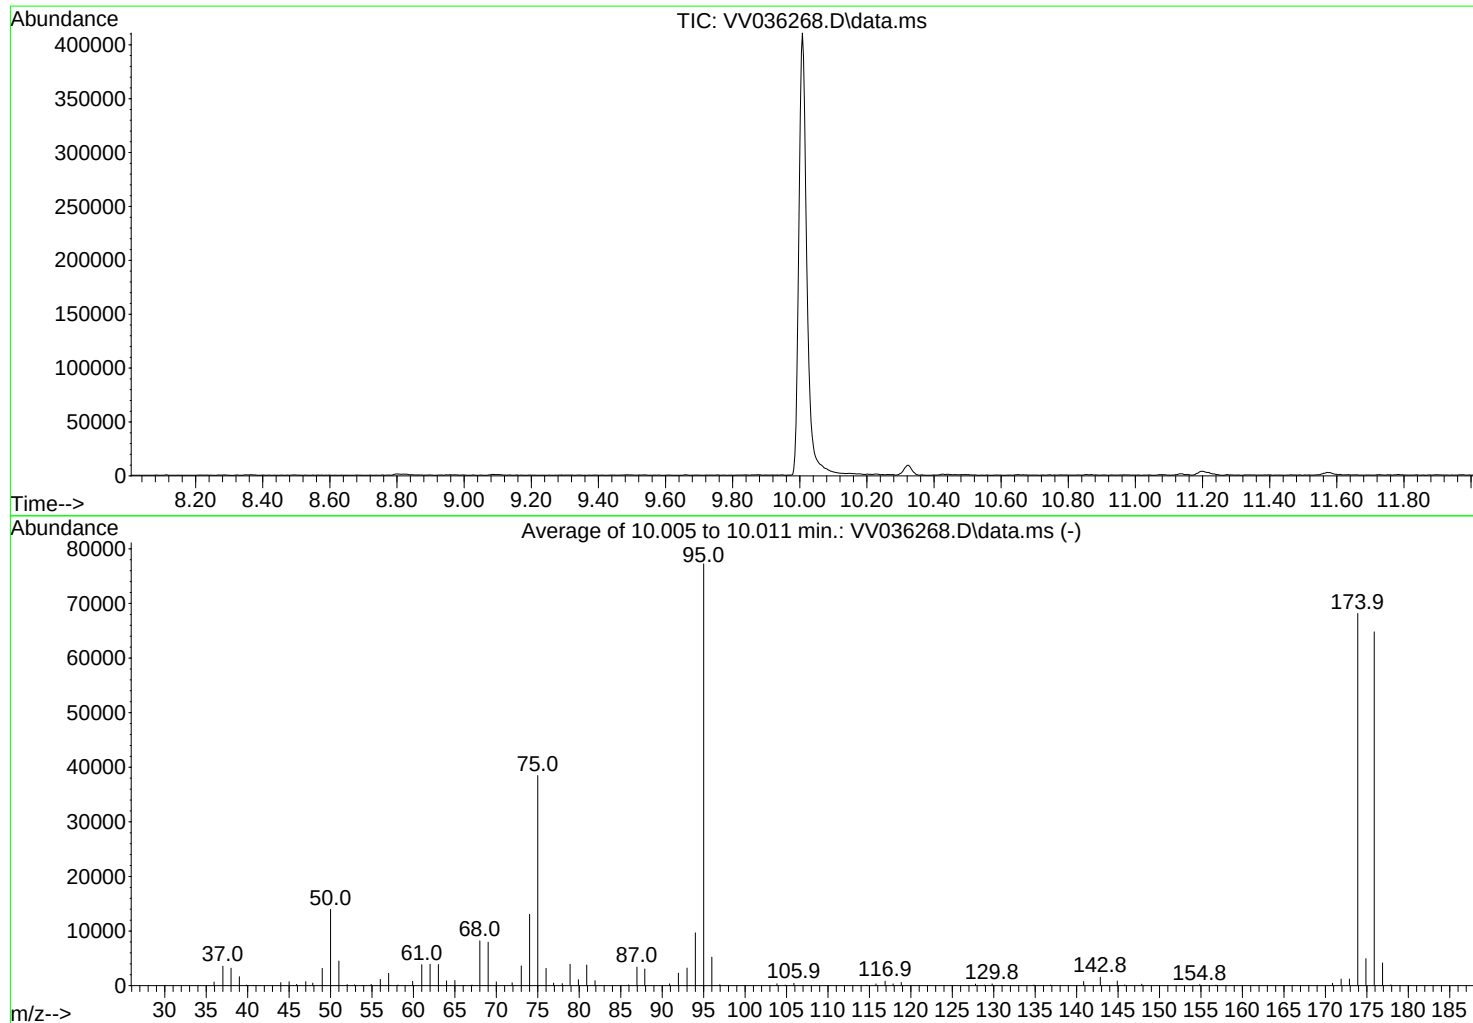

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	13970	PASS
75	95	30	80	49.8	38491	PASS
95	95	100	100	100.0	77253	PASS
96	95	5	9	6.7	5209	PASS
173	174	0.00	2	1.7	1190	PASS
174	95	50	120	88.2	68163	PASS
175	174	5	9	7.3	4965	PASS
176	174	95	101	95.0	64787	PASS
177	176	5	9	6.4	4163	PASS

m/z	Abundance
39.90	263.0
44.00	416.0
76.90	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB329

m/z	Abundance
35.90	681.0
37.00	3748.0
38.00	3359.0
39.00	1631.0
39.80	413.0
40.70	137.0
44.00	1004.0
45.00	716.0
45.90	271.0
47.00	711.0
47.80	460.0
49.00	3165.0
50.00	13888.0
51.00	4654.0
52.00	222.0
52.90	189.0
53.80	104.0
54.10	110.0
54.90	219.0
56.00	1196.0
57.00	2283.0
58.20	141.0
59.90	777.0
61.00	3968.0
62.00	4060.0
63.00	3828.0
64.00	976.0
65.00	896.0
66.00	102.0
66.90	169.0
68.00	8386.0
69.00	7990.0
70.00	708.0
71.90	595.0
73.00	3599.0
74.00	13140.0
75.00	38352.0
76.00	3203.0
76.90	596.0
78.00	375.0
78.90	4093.0
79.90	1055.0
80.90	3767.0
81.90	860.0
85.90	152.0
86.90	3401.0
87.90	3009.0
90.90	383.0
91.90	2168.0
93.00	3281.0
94.00	9646.0
95.00	76280.0
96.00	5169.0
97.00	130.0
103.90	330.0
104.80	118.0
105.90	403.0
115.80	323.0
116.90	816.0
117.80	286.0
118.80	568.0
127.80	267.0
128.80	135.0
129.80	372.0
134.90	119.0
136.80	158.0
140.80	748.0
142.90	1524.0
143.70	108.0
144.90	935.0
145.80	155.0
147.90	250.0
154.80	222.0
156.90	117.0
170.80	384.0
171.90	1056.0
172.90	1122.0
173.90	65744.0
174.90	4959.0
175.90	63304.0
176.90	4139.0
177.90	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB329

m/z	Abundance
35.90	714.0
37.00	3703.0
38.00	3295.0
39.00	1730.0
39.80	387.0
44.00	979.0
45.00	777.0
45.90	247.0
47.00	765.0
47.90	469.0
49.00	3265.0
50.00	14423.0
51.00	4645.0
52.00	211.0
52.90	150.0
53.80	102.0
54.90	247.0
56.00	1194.0
57.00	2323.0
58.20	137.0
59.90	812.0
61.00	3967.0
62.00	4067.0
63.00	4007.0
64.00	902.0
65.00	971.0
66.20	116.0
67.10	181.0
68.00	8451.0
69.00	8227.0
70.00	750.0
71.90	552.0
73.00	3722.0
74.00	13397.0
75.00	39848.0
76.00	3193.0
76.90	597.0
77.90	397.0
78.90	4045.0
79.90	1125.0
80.90	3858.0
81.90	937.0
85.90	156.0
86.90	3540.0
87.90	3096.0
90.90	349.0
92.00	2355.0
93.00	3311.0
94.00	10062.0
95.00	79992.0
96.00	5409.0
96.90	179.0
103.90	374.0
104.90	129.0
105.90	466.0
114.70	123.0
115.80	350.0
116.90	851.0
117.90	317.0
118.80	615.0
127.80	310.0
128.80	124.0
129.80	327.0
130.90	105.0
134.90	110.0
136.80	135.0
140.80	787.0
142.80	1588.0
143.70	103.0
144.90	843.0
145.80	143.0
147.90	258.0
154.90	212.0
156.80	122.0
170.90	463.0
171.90	1260.0
172.90	1224.0
173.90	70696.0
174.90	5116.0
175.90	67016.0
176.90	4287.0
177.90	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB329

m/z	Abundance
36.00	659.0
37.00	3269.0
38.00	2951.0
39.00	1553.0
39.90	336.0
44.00	966.0
45.00	685.0
45.90	197.0
47.00	736.0
47.90	470.0
49.00	3062.0
50.00	13599.0
51.00	4206.0
52.00	205.0
52.90	103.0
54.90	244.0
56.00	1059.0
57.00	2182.0
58.00	113.0
59.90	754.0
61.00	3584.0
62.00	3668.0
63.00	3794.0
64.00	804.0
65.00	976.0
67.00	196.0
68.00	7787.0
69.00	7602.0
70.00	686.0
71.90	455.0
73.00	3486.0
74.00	12661.0
75.00	37272.0
76.00	3090.0
77.00	533.0
78.00	405.0
78.90	3618.0
79.90	1107.0
80.90	3743.0
81.90	923.0
86.00	168.0
87.00	3284.0
87.90	3072.0
90.90	275.0
92.00	2362.0
93.00	3112.0
94.00	9336.0
95.00	75488.0
96.00	5050.0
97.00	190.0
103.80	395.0
104.80	130.0
105.90	442.0
106.90	109.0
114.70	119.0
115.80	323.0
116.90	829.0
117.90	338.0
118.90	546.0
127.80	290.0
128.90	112.0
129.80	247.0
130.90	121.0
134.80	108.0
136.90	108.0
140.90	729.0
142.80	1525.0
144.90	752.0
145.80	146.0
147.80	265.0
154.90	198.0
156.70	162.0
170.90	460.0
171.90	1309.0
172.90	1225.0
173.90	68048.0
174.90	4821.0
175.90	64040.0
176.90	4064.0
177.90	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB329