

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_V\DATA\VV062718\  
 Data File : VV006481.D  
 Acq On : 27 Jun 2018 15:18  
 Operator : SY/MD  
 Sample : J3673-10DL 8X  
 Misc : 25 mL/MSVOA\_V/WATER  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 DAZA5DL

Quant Time: Jun 28 01:19:25 2018  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVTR062518WMA.M  
 Quant Title : TRACE VOA SOM01.0  
 QLast Update : Thu Jun 28 01:18:56 2018  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|----------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Difluorobenzene     | 5.67  | 114  | 371119   | 5.00 | ug/L  | 0.00     |
| 28) Chlorobenzene-d5       | 8.90  | 117  | 331850   | 5.00 | ug/L  | 0.00     |
| 60) 1,4-Dichlorobenzene-d4 | 11.30 | 152  | 143177   | 5.00 | ug/L  | 0.00     |

## System Monitoring Compounds

|                                |        |       |          |          |      |        |
|--------------------------------|--------|-------|----------|----------|------|--------|
| 4) Vinyl Chloride-d3           | 1.32   | 65    | 109802   | 4.50     | ug/L | 0.00   |
| Spiked Amount                  | 5.000  | Range | 40 - 130 | Recovery | =    | 90.00% |
| 7) Chloroethane-d5             | 1.58   | 69    | 79280    | 4.03     | ug/L | 0.00   |
| Spiked Amount                  | 5.000  | Range | 65 - 130 | Recovery | =    | 80.60% |
| 11) 1,1-Dichloroethene-d2      | 2.13   | 63    | 140303   | 3.25     | ug/L | 0.00   |
| Spiked Amount                  | 5.000  | Range | 60 - 125 | Recovery | =    | 65.00% |
| 20) 2-Butanone-d5              | 3.96   | 46    | 182231   | 39.85    | ug/L | -0.01  |
| Spiked Amount                  | 50.000 | Range | 40 - 130 | Recovery | =    | 79.70% |
| 24) Chloroform-d               | 4.41   | 84    | 156145   | 3.75     | ug/L | 0.00   |
| Spiked Amount                  | 5.000  | Range | 70 - 125 | Recovery | =    | 75.00% |
| 26) 1,2-Dichloroethane-d4      | 5.09   | 65    | 78387    | 4.03     | ug/L | 0.00   |
| Spiked Amount                  | 5.000  | Range | 70 - 130 | Recovery | =    | 80.60% |
| 32) Benzene-d6                 | 5.11   | 84    | 361928   | 4.19     | ug/L | 0.00   |
| Spiked Amount                  | 5.000  | Range | 70 - 125 | Recovery | =    | 83.80% |
| 36) 1,2-Dichloropropane-d6     | 6.12   | 67    | 103821   | 4.03     | ug/L | 0.00   |
| Spiked Amount                  | 5.000  | Range | 60 - 140 | Recovery | =    | 80.60% |
| 41) Toluene-d8                 | 7.37   | 98    | 322660   | 3.94     | ug/L | 0.00   |
| Spiked Amount                  | 5.000  | Range | 70 - 130 | Recovery | =    | 78.80% |
| 43) trans-1,3-Dichloropropene- | 7.67   | 79    | 31231    | 3.29     | ug/L | 0.00   |
| Spiked Amount                  | 5.000  | Range | 55 - 130 | Recovery | =    | 65.80% |
| 46) 2-Hexanone-d5              | 8.14   | 63    | 131756   | 35.07    | ug/L | 0.00   |
| Spiked Amount                  | 50.000 | Range | 45 - 130 | Recovery | =    | 70.14% |
| 57) 1,1,2,2-Tetrachloroethane- | 10.27  | 84    | 54242    | 3.43     | ug/L | 0.00   |
| Spiked Amount                  | 5.000  | Range | 65 - 120 | Recovery | =    | 68.60% |
| 64) 1,2-Dichlorobenzene-d4     | 11.68  | 152   | 107186   | 4.03     | ug/L | 0.00   |
| Spiked Amount                  | 5.000  | Range | 80 - 120 | Recovery | =    | 80.60% |

## Target Compounds


|                            |      |    |        |              | Qvalue |
|----------------------------|------|----|--------|--------------|--------|
| 5) Vinyl chloride          | 1.33 | 62 | 9038   | 0.298 ug/L # | 76     |
| 13) Acetone                | 2.21 | 43 | 2085   | 0.744 ug/L   | 96     |
| 16) Methylene chloride     | 2.54 | 84 | 9198   | 0.350 ug/L   | 94     |
| 22) cis-1,2-Dichloroethene | 3.97 | 96 | 161556 | 5.979 ug/L   | 100    |
| 34) Trichloroethene        | 5.96 | 95 | 35067  | 1.251 ug/L   | 97     |
| 35) Methylcyclohexane      | 6.12 | 83 | 25669  | 0.630 ug/L # | 20     |
| 37) 1,2-Dichloropropane    | 6.12 | 63 | 10760  | 0.449 ug/L # | 85     |
| 48) 2-Hexanone             | 8.19 | 43 | 19027  | 2.269 ug/L # | 83     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_V\DATA\VV062718\  
Data File : VV006481.D  
Acq On : 27 Jun 2018 15:18  
Operator : SY/MD  
Sample : J3673-10DL 8X  
Misc : 25 mL/MSVOA\_V/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
DAZA5DL

Quant Time: Jun 28 01:19:25 2018  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVTR062518WMA.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Thu Jun 28 01:18:56 2018  
Response via : Initial Calibration

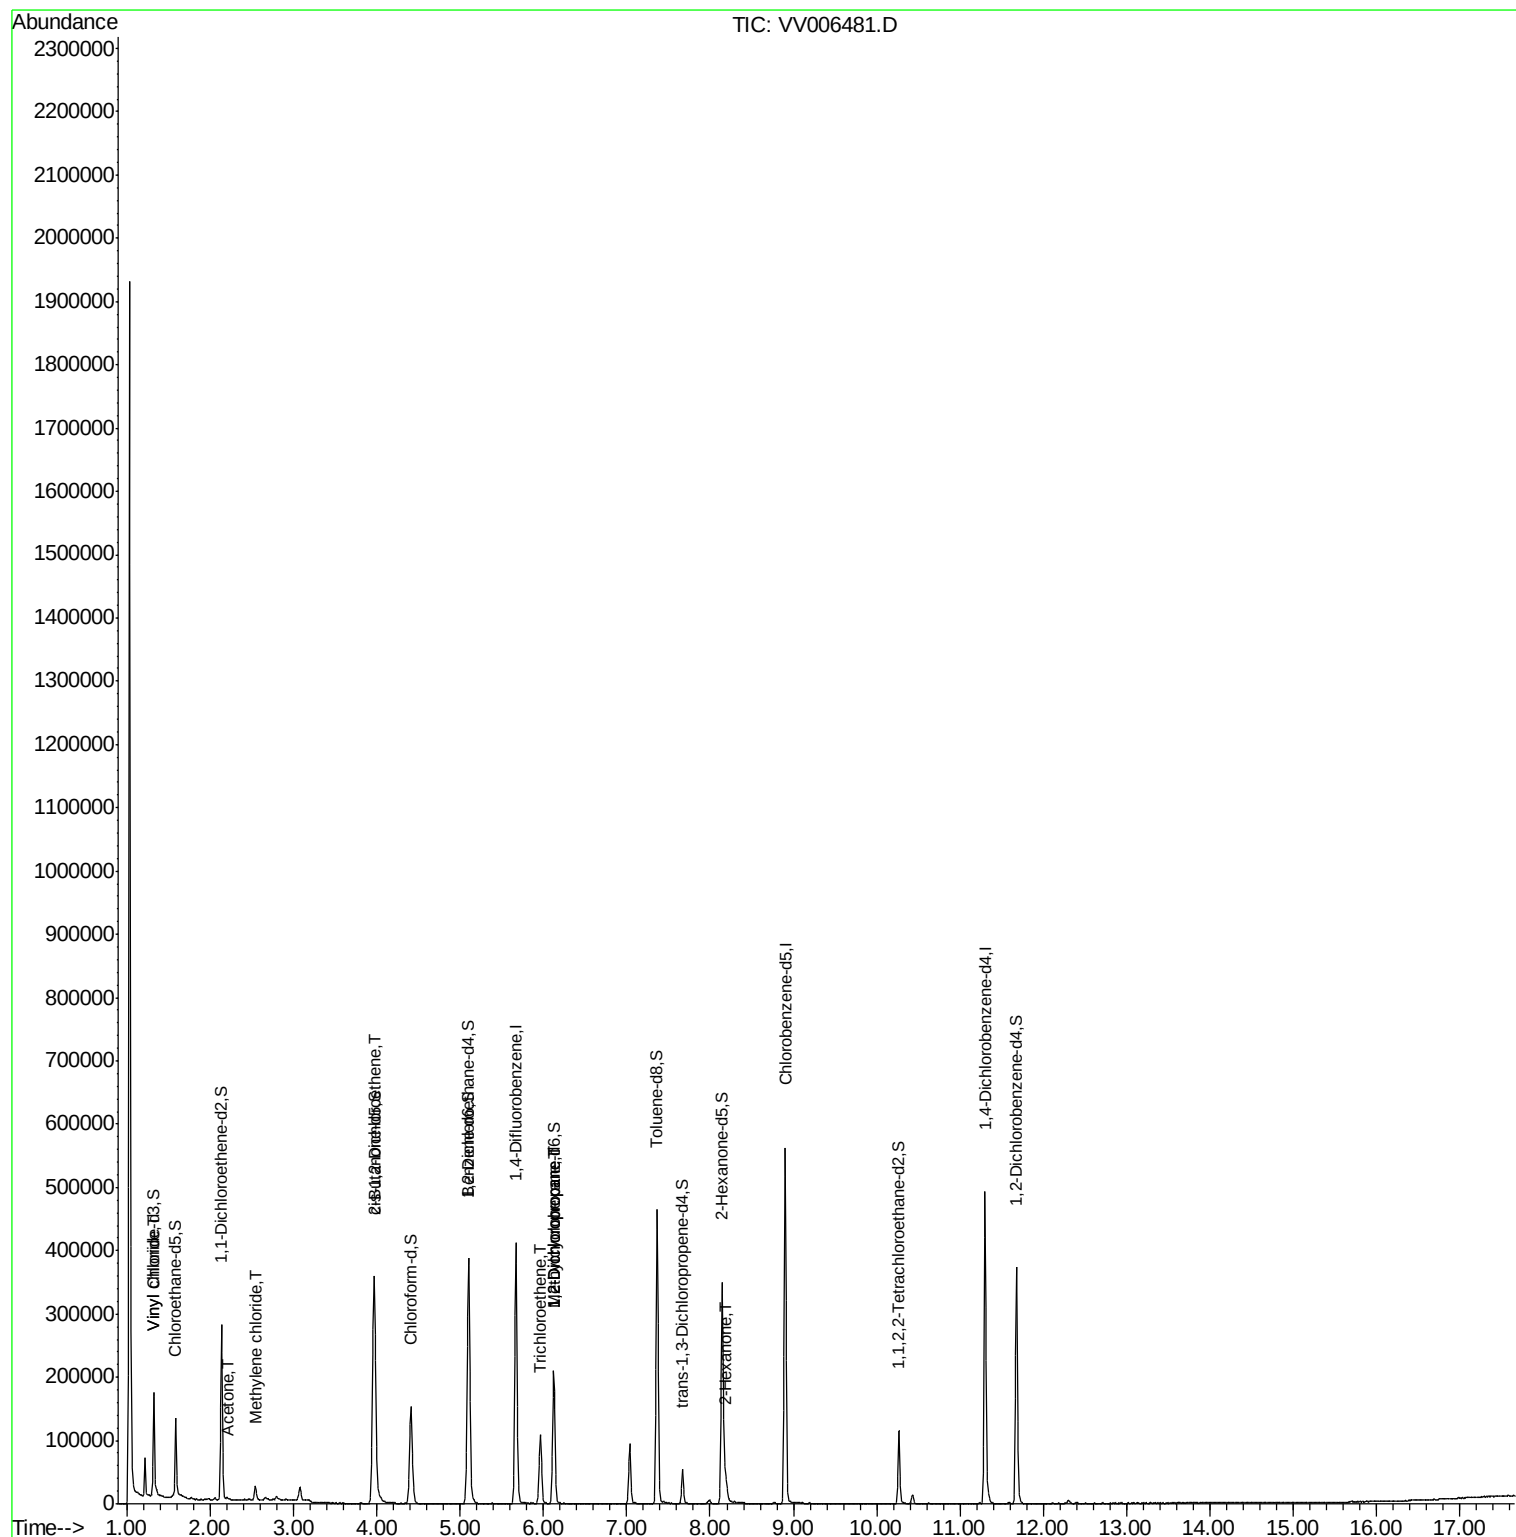

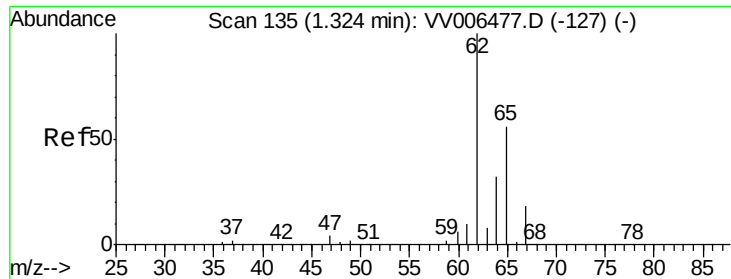

#5

Vinyl chloride

Concen: 0.298 ug/L

RT: 1.33 min Scan# 136

Delta R.T. 0.00 min

Lab File: VV006481.D

Acq: 27 Jun 2018 15:18

Instrument :

MSVOA\_V

ClientSampleId :


DAZA5DL

Tgt Ion: 62 Resp: 9038

Ion Ratio Lower Upper




62 100

64 46.8 23.1 42.9#

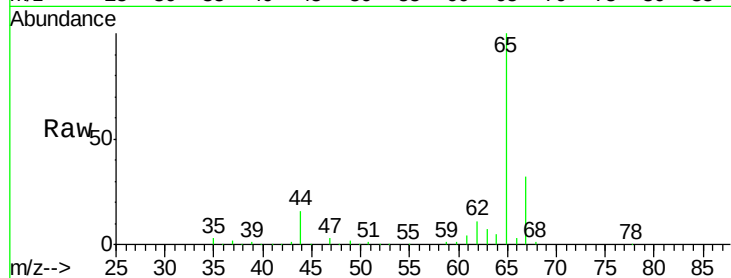

Abundance Ion 62.00 (61.70 to 62.70): VV0

Ion 64.10 (63.80 to 64.80): VV0

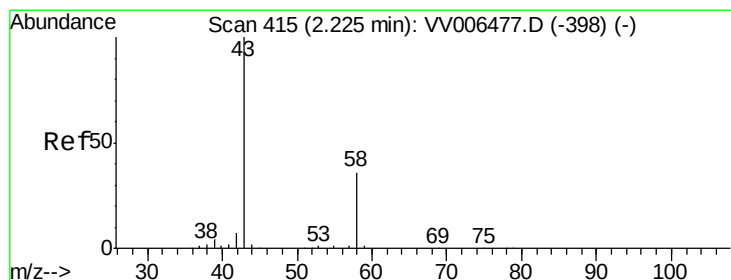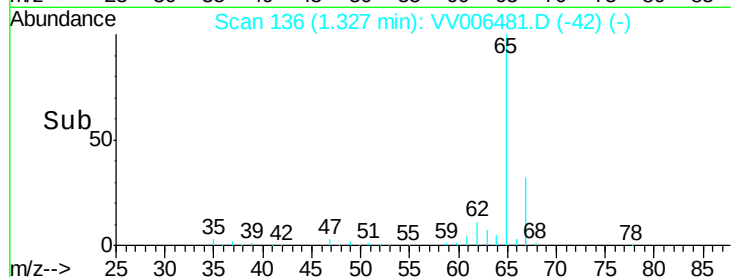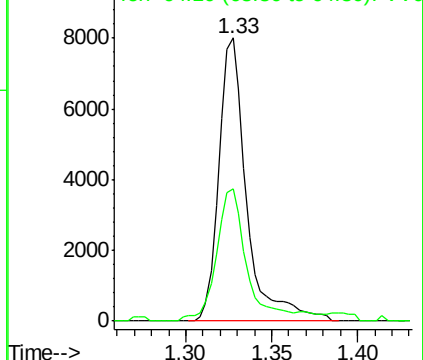

#13

Acetone

Concen: 0.744 ug/L

RT: 2.21 min Scan# 411

Delta R.T. -0.01 min

Lab File: VV006481.D


Acq: 27 Jun 2018 15:18

Tgt Ion: 43 Resp: 2085

Ion Ratio Lower Upper



43 100


58 36.4 0.0 77.4

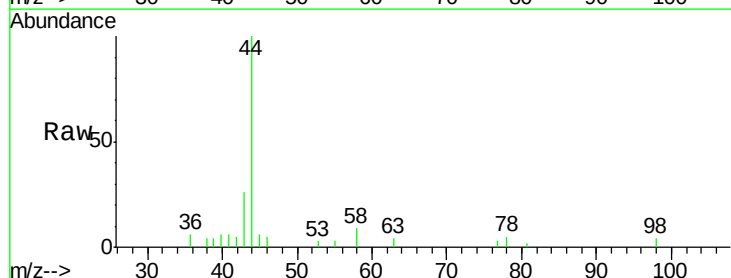

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0



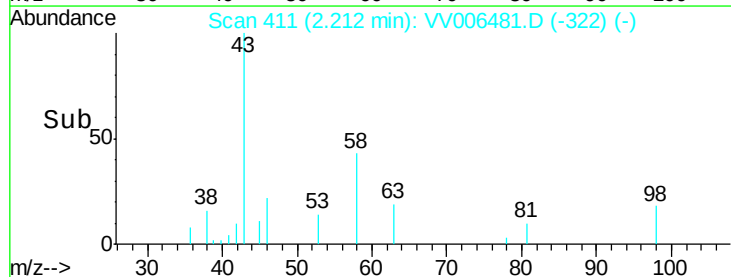
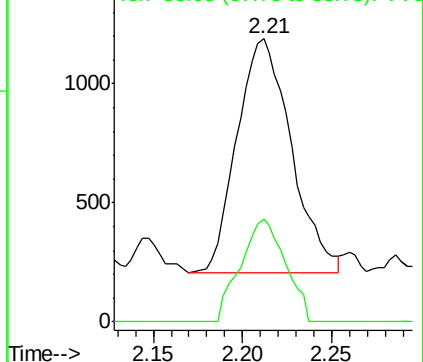


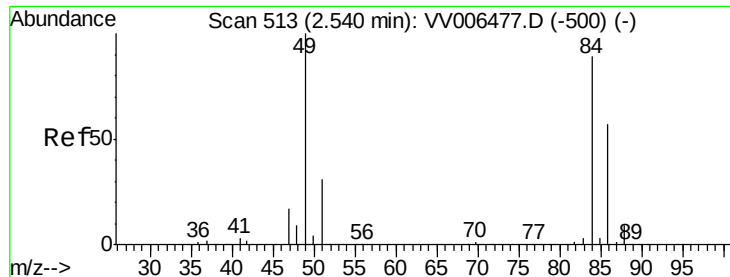

#16  
Methylene chloride  
Concen: 0.350 ug/L  
RT: 2.54 min Scan# 514  
Delta R.T. 0.00 min  
Lab File: VV006481.D  
Acq: 27 Jun 2018 15:18




Instrument :  
MSVOA\_V  
ClientSampleId :  
DAZA5DL


Tgt Ion: 84 Resp: 9198  
Ion Ratio Lower Upper  
84 100  
86 59.8 44.2 82.2  
49 104.7 79.0 146.8

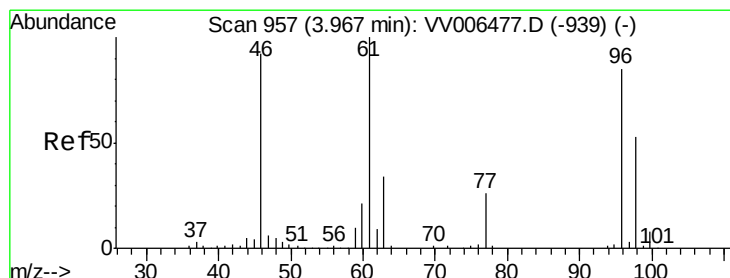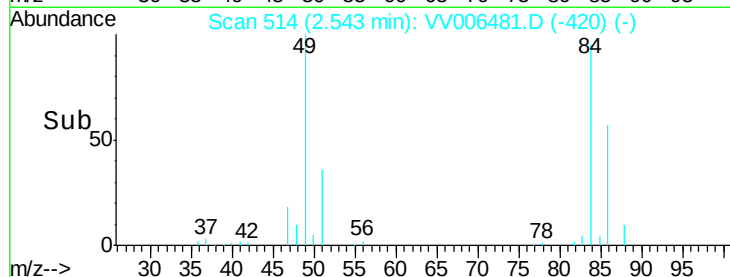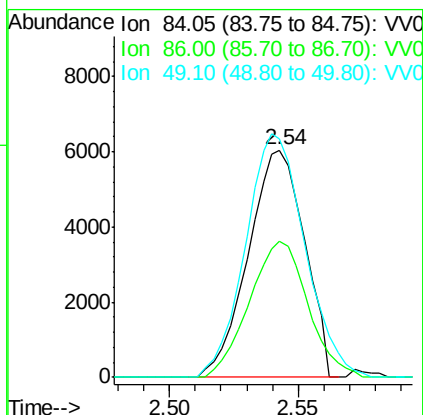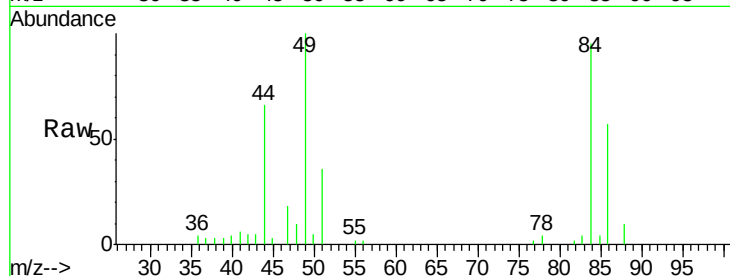

#22  
cis-1,2-Dichloroethene  
Concen: 5.979 ug/L  
RT: 3.97 min Scan# 958  
Delta R.T. 0.00 min  
Lab File: VV006481.D  
Acq: 27 Jun 2018 15:18

Tgt Ion: 96 Resp: 161556  
Ion Ratio Lower Upper  
96 100  
61 116.8 81.8 151.8  
68 0.0 0.0 0.0

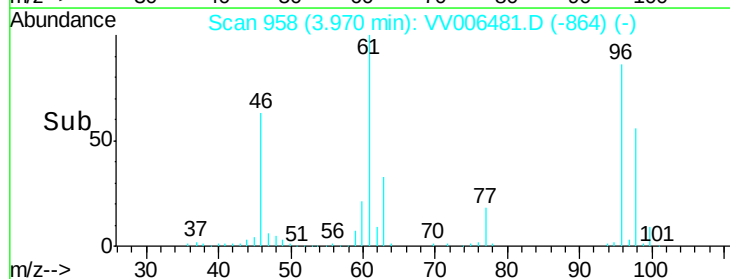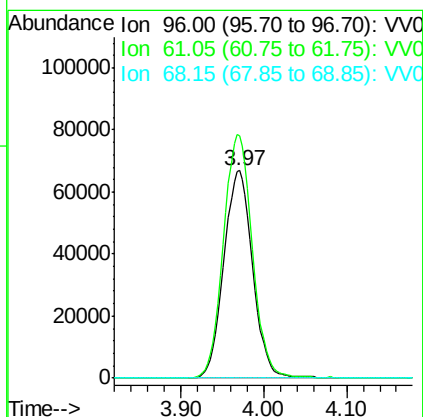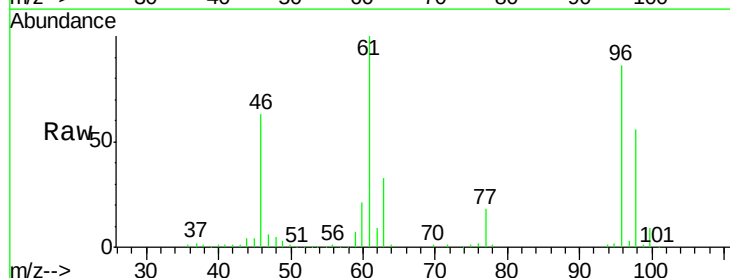


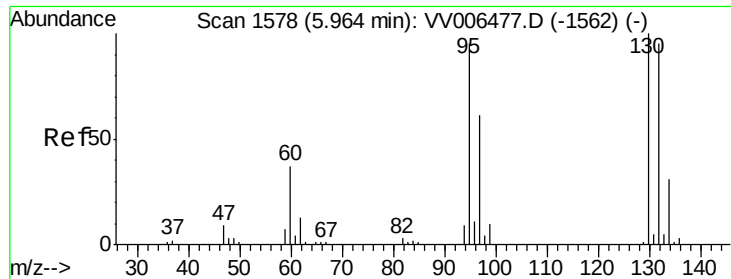




#34  
 Trichloroethene  
 Concen: 1.251 ug/L  
 RT: 5.96 min Scan# 1578  
 Delta R.T. -0.00 min  
 Lab File: VV006481.D  
 Acq: 27 Jun 2018 15:18

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 DAZA5DL

Tgt Ion: 95 Resp: 35067  
 Ion Ratio Lower Upper  
 95 100  
 97 65.7 44.6 82.8  
 132 103.3 70.1 130.1  
 130 107.1 73.3 136.1

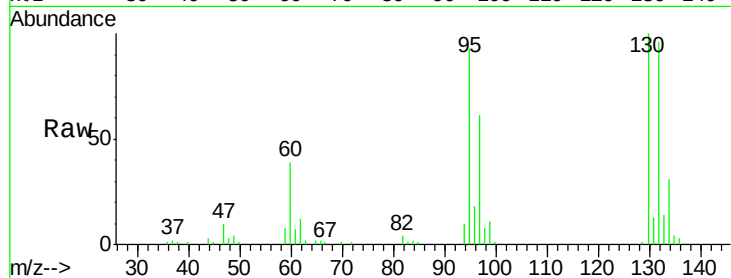


Abundance Ion 95.00 (94.70 to 95.70): VV0  
 Ion 96.95 (96.65 to 97.65): VV0  
 Ion 131.95 (131.65 to 132.65): V  
 Ion 129.95 (129.65 to 130.65): V

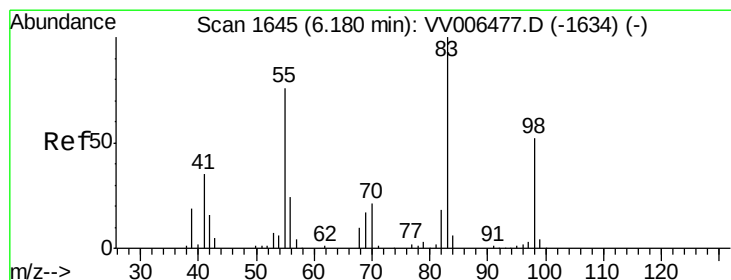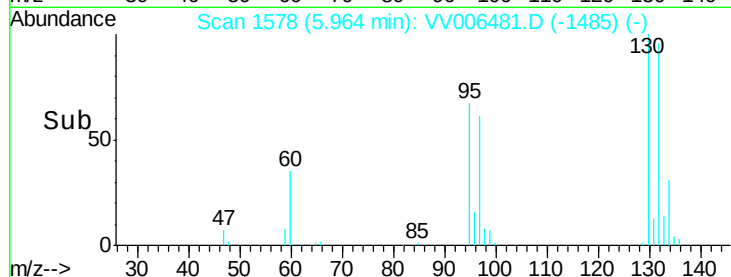
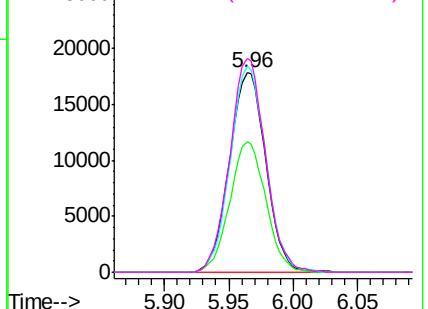



#35  
 Methylcyclohexane  
 Concen: 0.630 ug/L  
 RT: 6.12 min Scan# 1628  
 Delta R.T. -0.05 min  
 Lab File: VV006481.D  
 Acq: 27 Jun 2018 15:18

Tgt Ion: 83 Resp: 25669  
 Ion Ratio Lower Upper  
 83 100  
 55 0.4 57.5 86.3#  
 98 0.0 39.6 59.4#

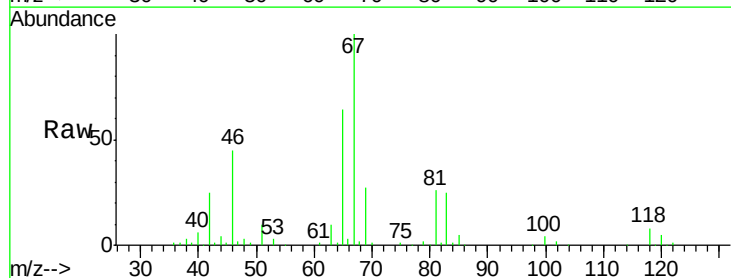

Abundance Ion 83.15 (82.85 to 83.85): VV0  
 Ion 55.10 (54.80 to 55.80): VV0  
 Ion 98.15 (97.85 to 98.85): VV0



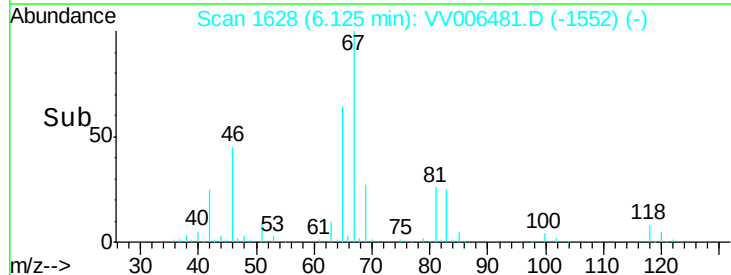
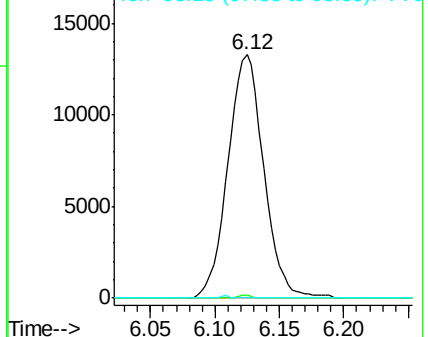


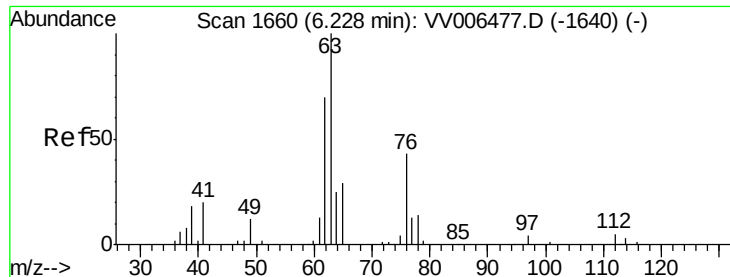

#37  
 1,2-Dichloropropane  
 Concen: 0.449 ug/L  
 RT: 6.12 min Scan# 1628  
 Delta R.T. -0.10 min  
 Lab File: VV006481.D  
 Acq: 27 Jun 2018 15:18

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 DAZA5DL

Tgt Ion: 63 Resp: 10760  
 Ion Ratio Lower Upper  
 63 100  
 112 0.0 4.0 6.0#

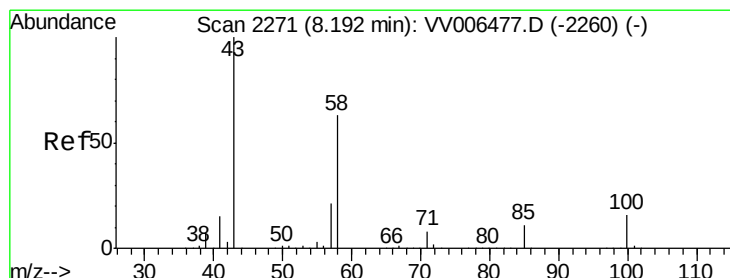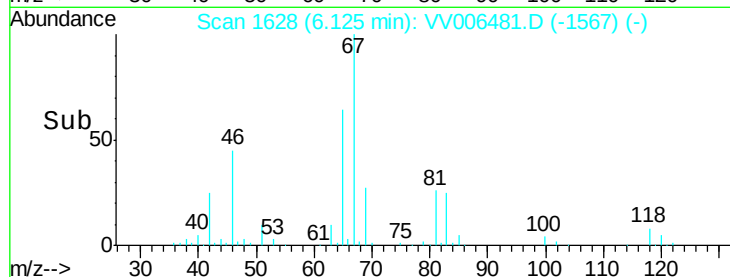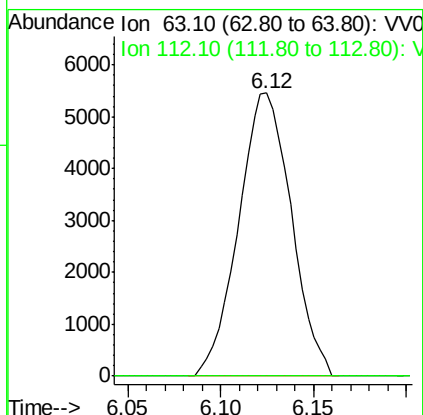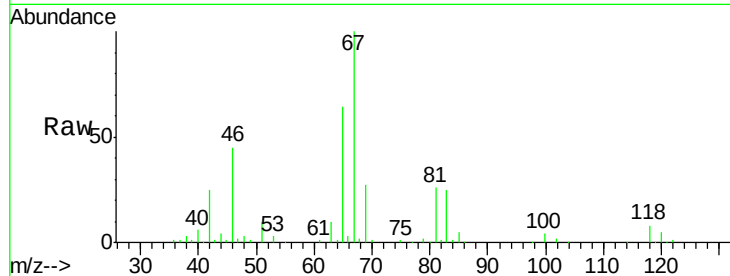

#48  
 2-Hexanone  
 Concen: 2.269 ug/L  
 RT: 8.19 min Scan# 2270  
 Delta R.T. -0.00 min  
 Lab File: VV006481.D  
 Acq: 27 Jun 2018 15:18

Tgt Ion: 43 Resp: 19027  
 Ion Ratio Lower Upper  
 43 100  
 58 47.5 49.9 74.9#  
 57 16.6 17.3 25.9#  
 100 8.9 12.5 18.7#

