

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062718\
 Data File : VV006478.D
 Acq On : 27 Jun 2018 12:08
 Operator : SY/MD
 Sample : VV0627WBL01
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK65

Quant Time: Jun 28 01:20:55 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jun 28 01:18:56 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	363240	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	327752	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	143424	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	122629	5.13	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.60%
7) Chloroethane-d5	1.59	69	97345	5.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.20%
11) 1,1-Dichloroethene-d2	2.13	63	159659	3.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.40%
20) 2-Butanone-d5	3.97	46	204404	45.67	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.34%
24) Chloroform-d	4.41	84	179728	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.20%
26) 1,2-Dichloroethane-d4	5.09	65	87678	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.00%
32) Benzene-d6	5.10	84	405443	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
36) 1,2-Dichloropropane-d6	6.12	67	118671	4.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.40%
41) Toluene-d8	7.36	98	366238	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.60%
43) trans-1,3-Dichloropropene-	7.67	79	35972	3.84	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.80%
46) 2-Hexanone-d5	8.14	63	150485	40.55	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.10%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	62380	4.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	125061	4.69	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.80%


Target Compounds					Ovalue
16) Methylene chloride	2.54	84	6408	0.25 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062718\
Data File : VV006478.D
Acq On : 27 Jun 2018 12:08
Operator : SY/MD
Sample : VV0627WBL01
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK65

Quant Time: Jun 28 01:20:55 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 28 01:18:56 2018
Response via : Initial Calibration

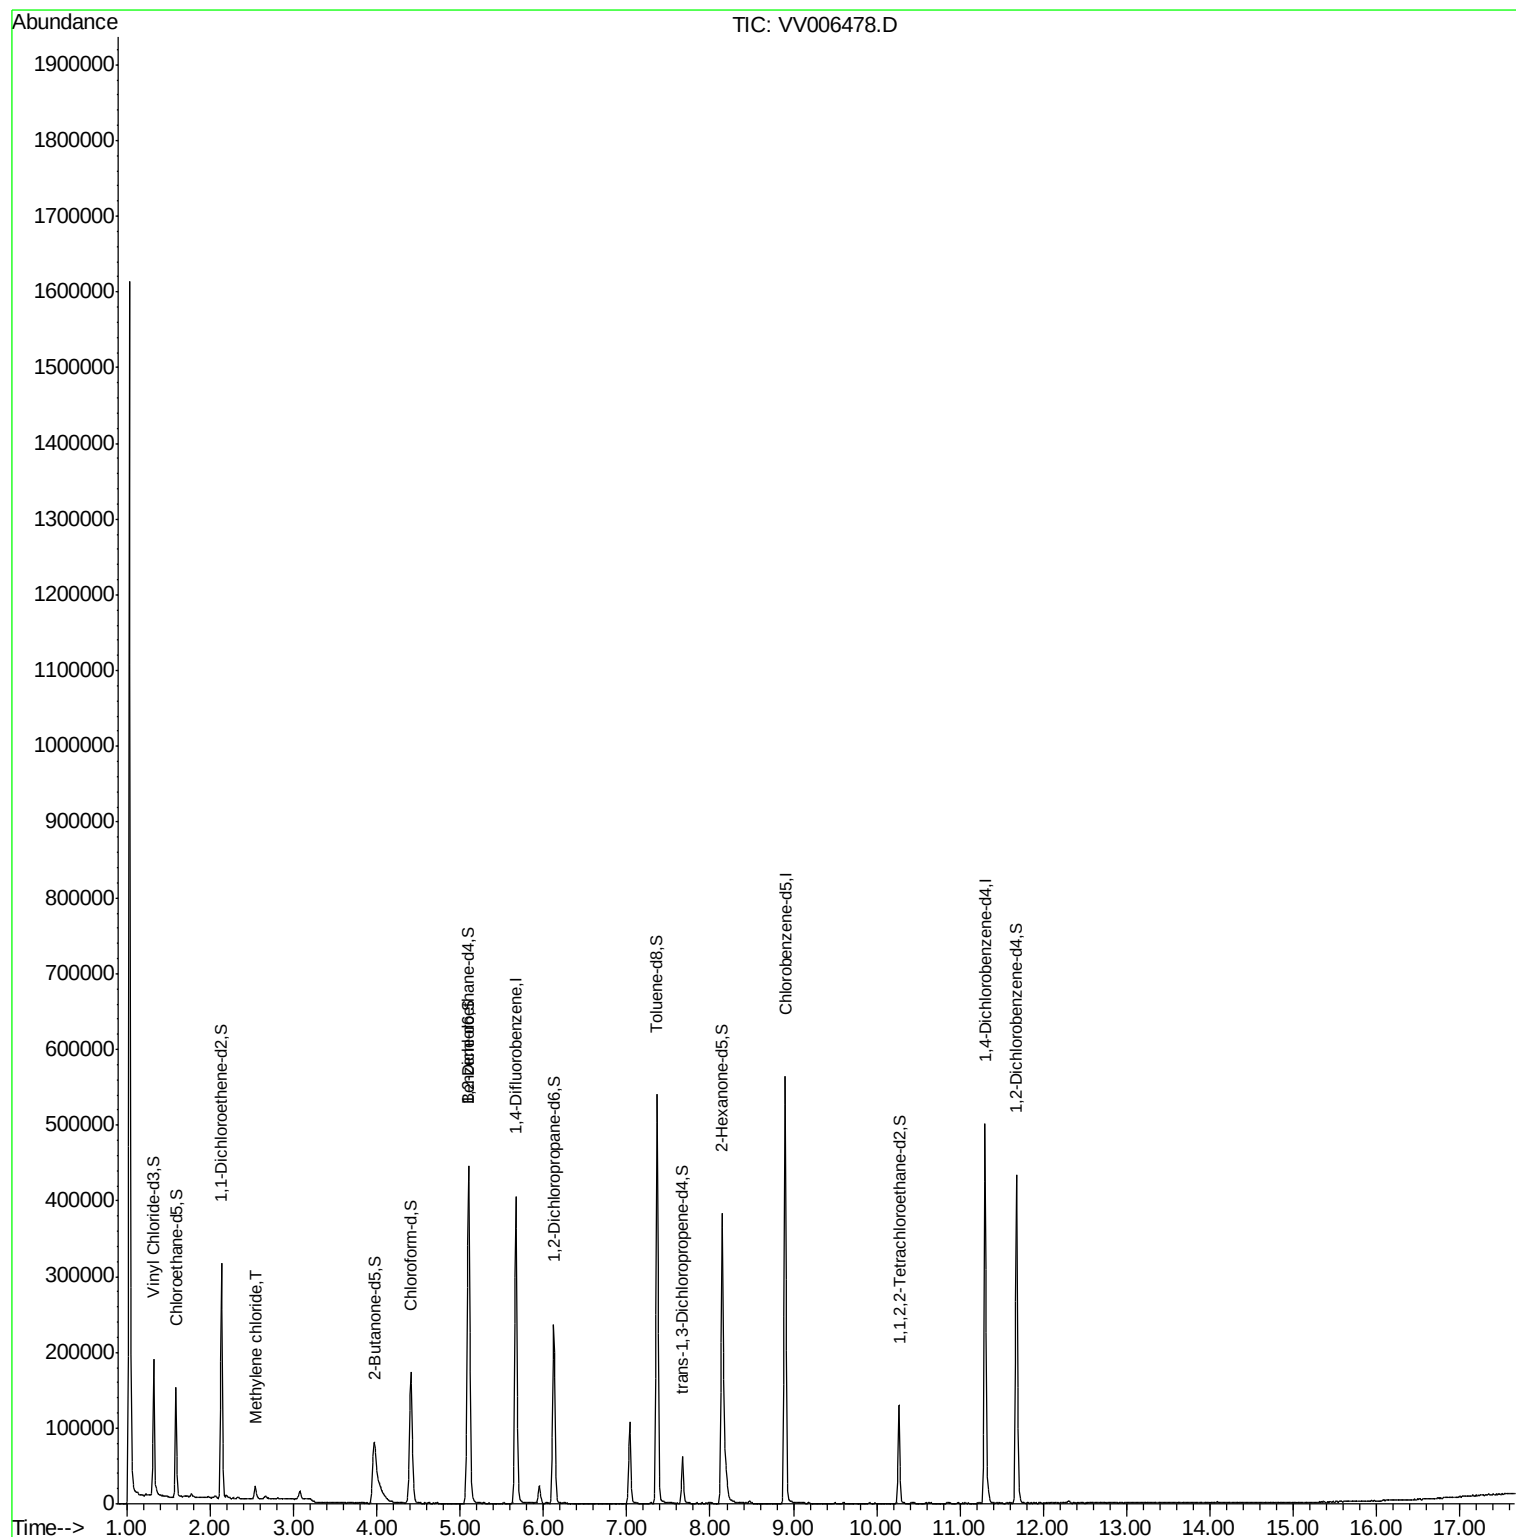

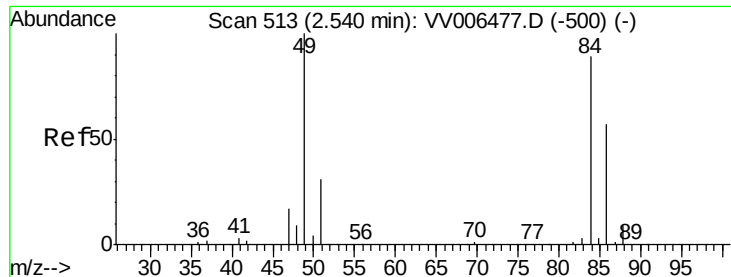

#16
Methylene chloride
Concen: 0.25 ug/L
RT: 2.54 min Scan# 513
Delta R.T. -0.00 min
Lab File: VV006478.D
Acq: 27 Jun 2018 12:08

Instrument :
MSVOA_V
ClientSampleId :
VBLK65

Tot Ion: 84 Resp: 6408

Ion	Ratio	Lower	Upper
84	100		
86	63.2	44.2	82.2
49	114.0	79.0	146.8

