

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062718\
 Data File : VV006479.D
 Acq On : 27 Jun 2018 12:49
 Operator : SY/MD
 Sample : J3673-06DL 400X
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DAZA1DL

Quant Time: Jun 28 01:22:51 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jun 28 01:18:56 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	329516	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	296717	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	127199	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	85449	3.94	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.80%
7) Chloroethane-d5	1.59	69	75120	4.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.00%
11) 1,1-Dichloroethene-d2	2.13	63	118235	3.08	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.60%
20) 2-Butanone-d5	3.97	46	170918	42.10	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.20%
24) Chloroform-d	4.41	84	161071	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.20%
26) 1,2-Dichloroethane-d4	5.09	65	82462	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.40%
32) Benzene-d6	5.10	84	351624	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
36) 1,2-Dichloropropane-d6	6.12	67	108911	4.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.60%
41) Toluene-d8	7.36	98	309743	4.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.60%
43) trans-1,3-Dichloropropene-	7.67	79	32043	3.78	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.60%
46) 2-Hexanone-d5	8.14	63	151120	44.99	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.98%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	60340	4.27	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	113930	4.82	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.40%


Target Compounds					Ovalue
34) Trichloroethene	5.96	95	183591	7.32 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062718\
Data File : VV006479.D
Acq On : 27 Jun 2018 12:49
Operator : SY/MD
Sample : J3673-06DL 400X
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DAZA1DL

Quant Time: Jun 28 01:22:51 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 28 01:18:56 2018
Response via : Initial Calibration

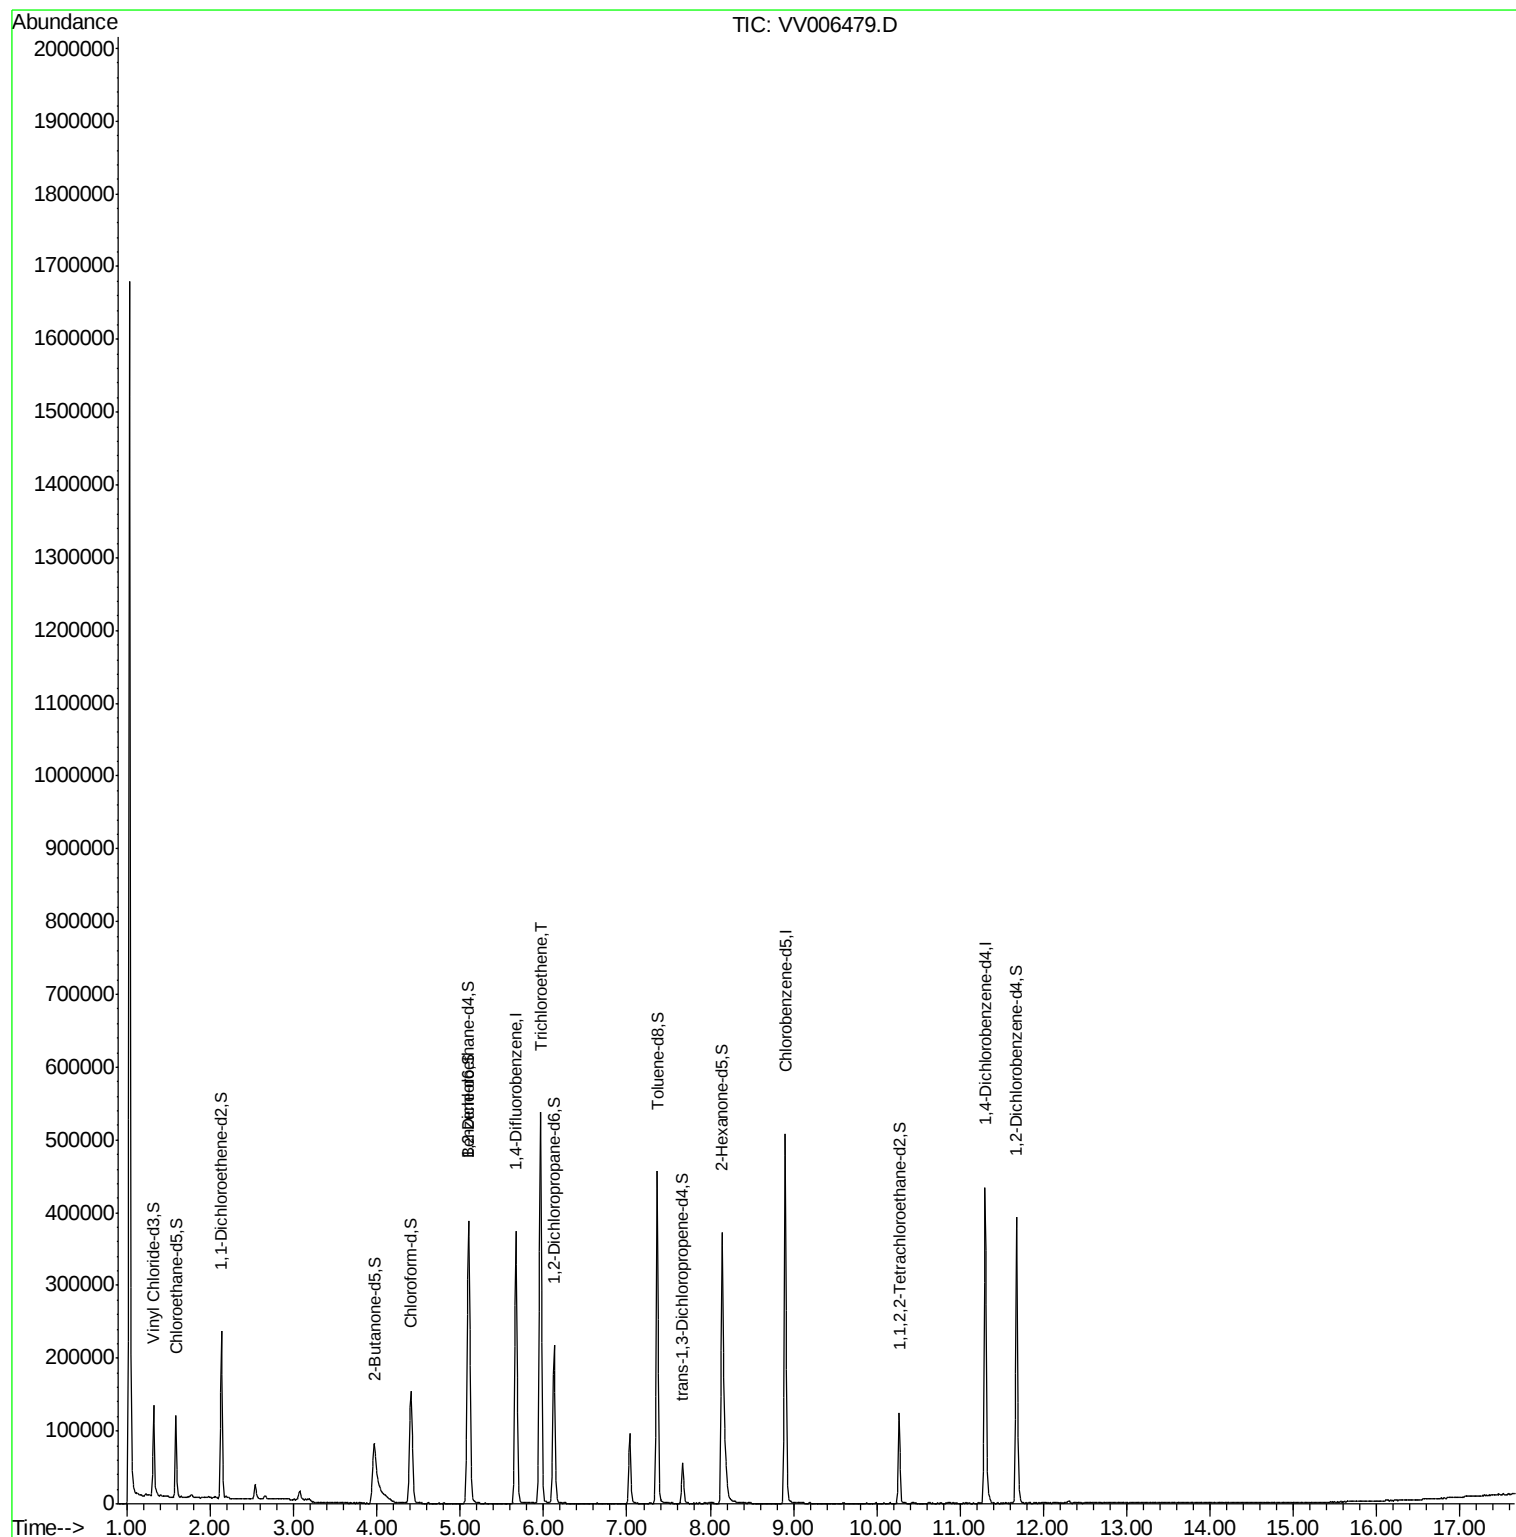

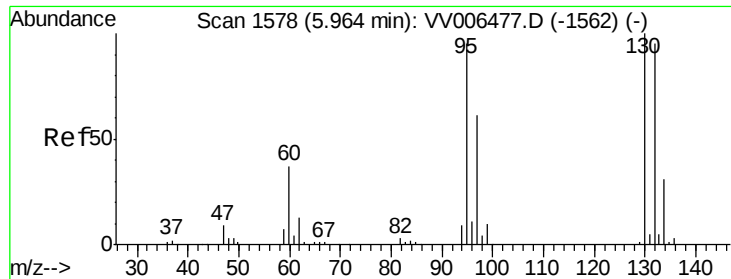

#34

Trichloroethene

Concen: 7.32 ug/L

RT: 5.96 min Scan# 1578

Delta R.T. 0.00 min

Lab File: VV006479.D


Acq: 27 Jun 2018 12:49

Instrument :

MSVOA_V

ClientSampleId :

DAZA1DL

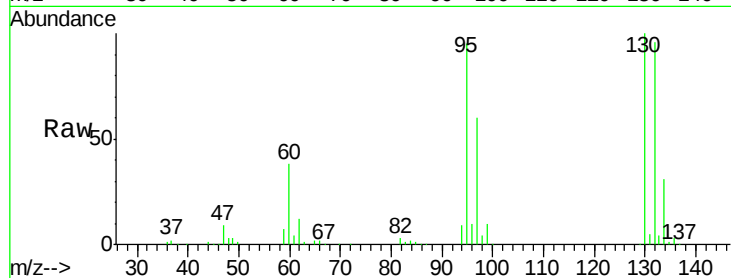

Tot Ion: 95 Resp: 183591

Ion Ratio Lower Upper

95 100

97 63.4 44.6 82.8

132 101.0 70.1 130.1

130 105.0 73.3 136.1

Abundance

Ion 95.00 (94.70 to 95.70): VV0

Ion 96.95 (96.65 to 97.65): VV0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

