


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062824\
Data File : VV036337.D
Acq On : 28 Jun 2024 08:11
Operator : SY/MD
Sample : BFB332
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB332

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062724SMA.M
Title : VOC Analysis
Last Update : Wed Jul 03 05:08:41 2024

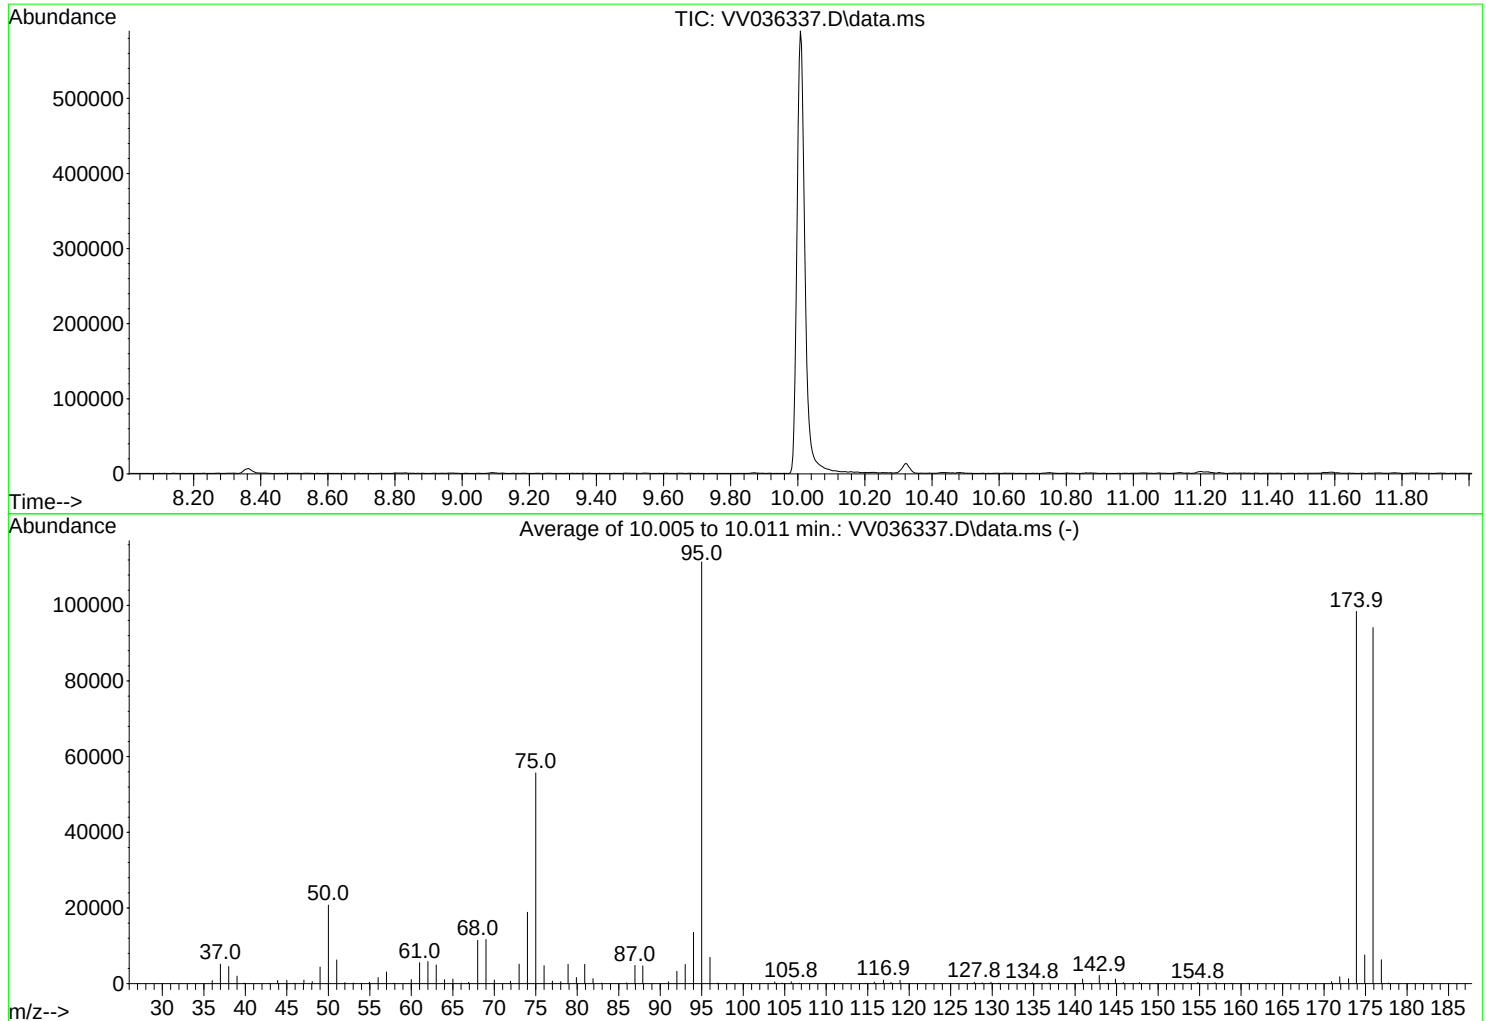

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	20784	PASS
75	95	30	80	50.0	55709	PASS
95	95	100	100	100.0	111496	PASS
96	95	5	9	6.2	6942	PASS
173	174	0.00	2	1.3	1322	PASS
174	95	50	120	88.2	98368	PASS
175	174	5	9	7.7	7574	PASS
176	174	95	101	95.7	94091	PASS
177	176	5	9	6.7	6300	PASS

m/z	Abundance
39.90	268.0
43.90	355.0

Instrument :
MSVOA_V
ClientSampleId :
BFB332

m/z	Abundance
36.00	766.0
37.00	5069.0
38.00	4569.0
39.00	1874.0
39.80	473.0
43.90	1158.0
45.00	857.0
45.90	126.0
47.00	936.0
48.00	556.0
49.00	4342.0
50.00	20248.0
51.00	6217.0
52.00	328.0
53.00	166.0
53.90	129.0
55.00	373.0
56.00	1565.0
57.00	2974.0
57.90	114.0
60.00	912.0
61.00	5379.0
62.00	5627.0
63.00	4821.0
64.00	1088.0
65.00	1225.0
66.10	153.0
66.90	355.0
68.00	11381.0
69.00	11410.0
70.00	1021.0
72.00	600.0
73.00	5152.0
74.00	18416.0
75.00	54808.0
76.00	4564.0
77.00	639.0
78.00	474.0
78.90	4999.0
79.90	1559.0
80.90	5214.0
81.90	1258.0
83.00	149.0
85.90	198.0
87.00	4569.0
87.90	4549.0
91.00	441.0
92.00	3218.0
93.00	4896.0
94.00	13348.0
95.00	107392.0
96.00	6790.0
96.90	173.0
103.80	463.0
104.70	146.0
105.80	513.0
106.70	125.0
110.90	124.0
114.70	145.0
115.80	452.0
116.90	909.0
117.80	320.0
118.90	903.0
127.80	379.0
128.80	194.0
129.80	394.0
130.80	185.0
134.80	236.0
136.80	208.0
140.90	1139.0
141.90	146.0
142.90	2089.0
143.90	146.0
144.80	1216.0
145.80	278.0
147.70	271.0
152.80	105.0
154.80	345.0
156.90	237.0
158.80	130.0
160.90	129.0
170.90	533.0
171.90	1700.0
172.90	1297.0
173.90	93144.0
174.90	7451.0
175.90	89808.0
176.90	6189.0
177.80	182.0

Instrument :
MSVOA_V
ClientSampleId :
BFB332

m/z	Abundance
36.00	815.0
37.00	5380.0
38.00	4668.0
39.00	2065.0
39.90	439.0
43.90	1235.0
45.00	843.0
45.90	101.0
47.10	968.0
48.10	539.0
49.00	4542.0
50.00	21600.0
51.00	6538.0
52.00	310.0
53.00	181.0
53.90	140.0
54.90	399.0
56.00	1658.0
57.00	3148.0
57.90	105.0
60.00	1077.0
61.00	5708.0
62.00	6083.0
63.00	5095.0
64.00	1091.0
65.00	1249.0
66.10	151.0
66.90	360.0
68.00	11953.0
69.00	12038.0
70.00	1024.0
71.90	641.0
73.00	5311.0
74.00	19392.0
75.00	57432.0
76.00	4914.0
77.00	687.0
78.00	508.0
78.90	5366.0
79.90	1688.0
80.90	5288.0
81.90	1368.0
83.00	180.0
86.00	225.0
86.90	4985.0
87.90	4759.0
91.00	487.0
92.00	3327.0
93.00	5205.0
94.00	14030.0
95.00	115320.0
96.00	7200.0
97.00	186.0
103.80	488.0
104.70	178.0
105.80	517.0
106.70	152.0
110.90	150.0
114.80	154.0
115.80	448.0
116.90	948.0
117.80	359.0
118.90	929.0
127.80	387.0
128.80	210.0
129.90	370.0
130.80	187.0
134.80	239.0
136.80	194.0
139.80	107.0
140.90	1250.0
141.80	125.0
142.90	2249.0
143.80	167.0
144.90	1266.0
145.80	319.0
146.90	108.0
147.80	314.0
152.80	109.0
154.80	330.0
156.80	259.0
158.80	156.0
160.80	128.0
170.90	558.0
171.90	1854.0
173.00	1343.0
173.90	101416.0
174.90	7900.0
175.90	97200.0
176.90	6528.0
177.80	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB332

m/z	Abundance
36.00	816.0
37.00	5065.0
38.00	4381.0
39.00	2002.0
39.90	369.0
42.80	118.0
44.00	1188.0
45.00	842.0
45.90	131.0
47.10	958.0
48.10	524.0
49.00	4285.0
50.00	20504.0
51.00	6029.0
52.00	290.0
53.00	189.0
54.00	174.0
54.90	354.0
56.00	1585.0
57.00	3082.0
57.90	113.0
60.00	1204.0
61.00	5533.0
62.00	5861.0
63.00	4884.0
64.00	986.0
65.00	1177.0
66.00	158.0
66.90	332.0
68.00	11109.0
69.00	11576.0
70.00	887.0
71.90	630.0
73.00	4972.0
74.00	18840.0
75.00	54888.0
76.00	4771.0
77.00	663.0
78.00	481.0
78.90	5024.0
79.90	1584.0
80.90	4830.0
81.90	1272.0
82.90	182.0
86.00	235.0
86.90	4877.0
87.90	4805.0
91.00	481.0
92.00	3231.0
93.00	5123.0
94.00	13414.0
95.00	111776.0
96.00	6836.0
97.00	192.0
103.80	469.0
104.70	172.0
105.80	457.0
106.80	160.0
110.80	133.0
114.80	131.0
115.80	428.0
116.90	956.0
117.80	357.0
118.90	814.0
123.80	104.0
127.90	374.0
128.80	214.0
129.90	345.0
130.80	167.0
134.90	180.0
136.90	167.0
139.80	129.0
140.90	1191.0
141.80	122.0
142.90	2085.0
143.80	166.0
144.90	1143.0
145.80	281.0
146.90	114.0
147.80	314.0
149.80	103.0
154.80	301.0
156.80	244.0
158.80	153.0
160.80	138.0
170.90	539.0
171.90	1903.0
173.00	1325.0
173.90	100544.0
174.90	7371.0
175.90	95264.0
176.90	6182.0

Instrument :
MSVOA_V
ClientSampleId :
BFB332

177.80

162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB332